

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095568.D

Acq On : 8 Feb 2018 14:32

Operator : SJ/JU

Sample : J1316-13

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 09 00:47:34 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




F6D36

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:39 PM

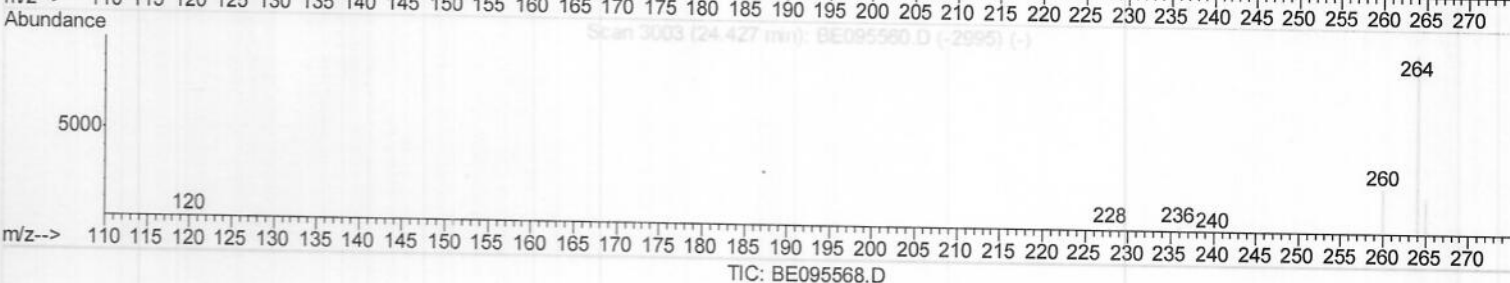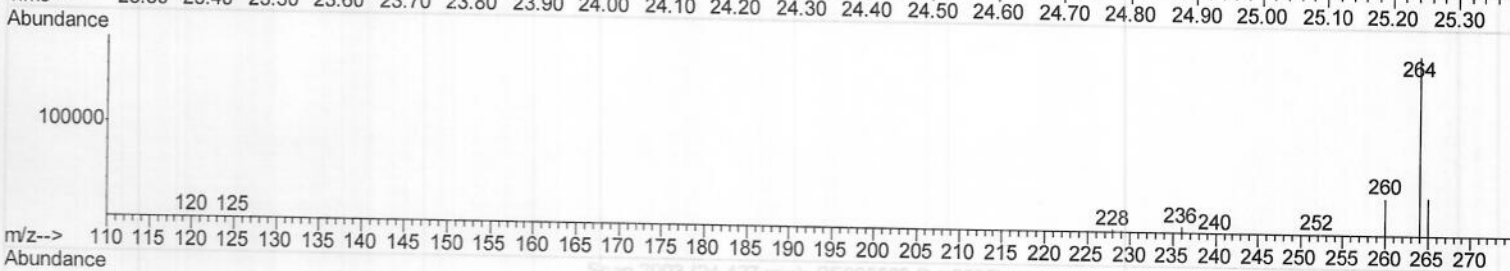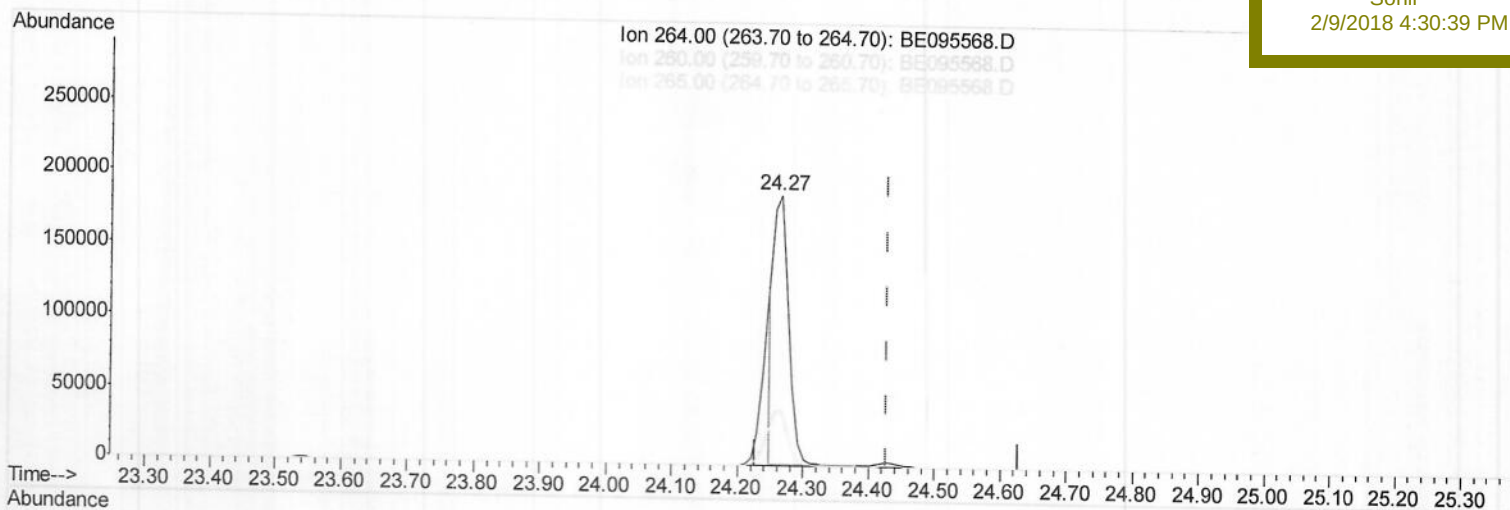

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 309537

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.95#
265.00	103.50	21.40#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095568.D

Acq On : 8 Feb 2018 14:32

Operator : SJ/JU

Sample : J1316-13

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 09 00:47:34 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :



F6D36

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:39 PM

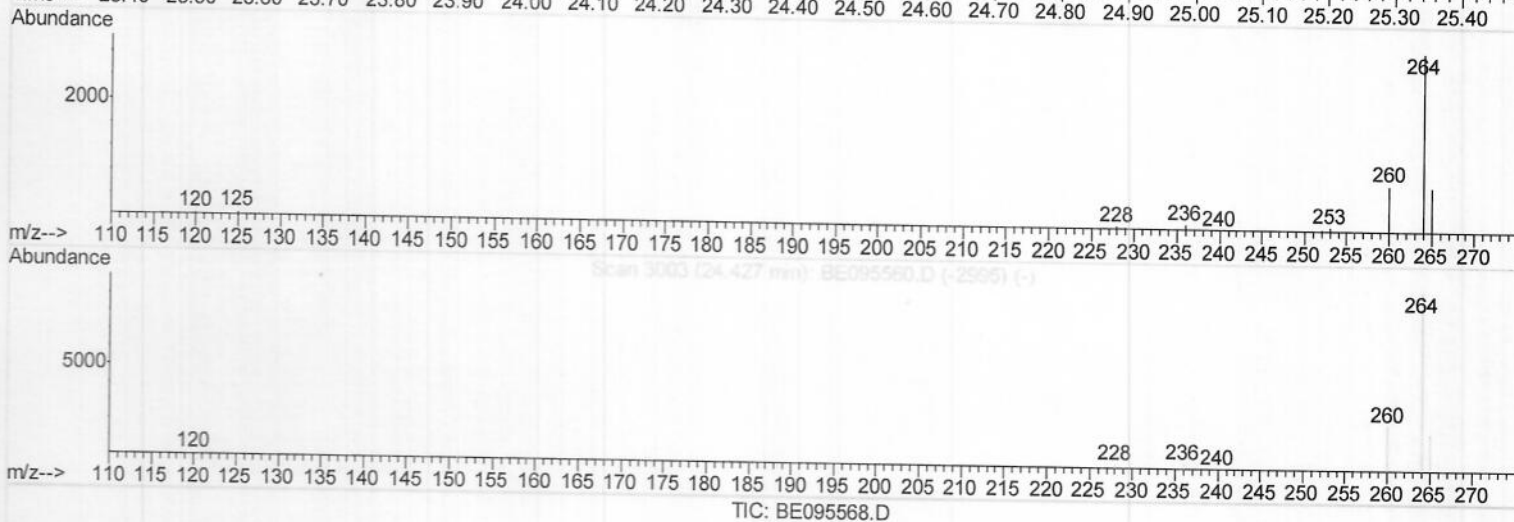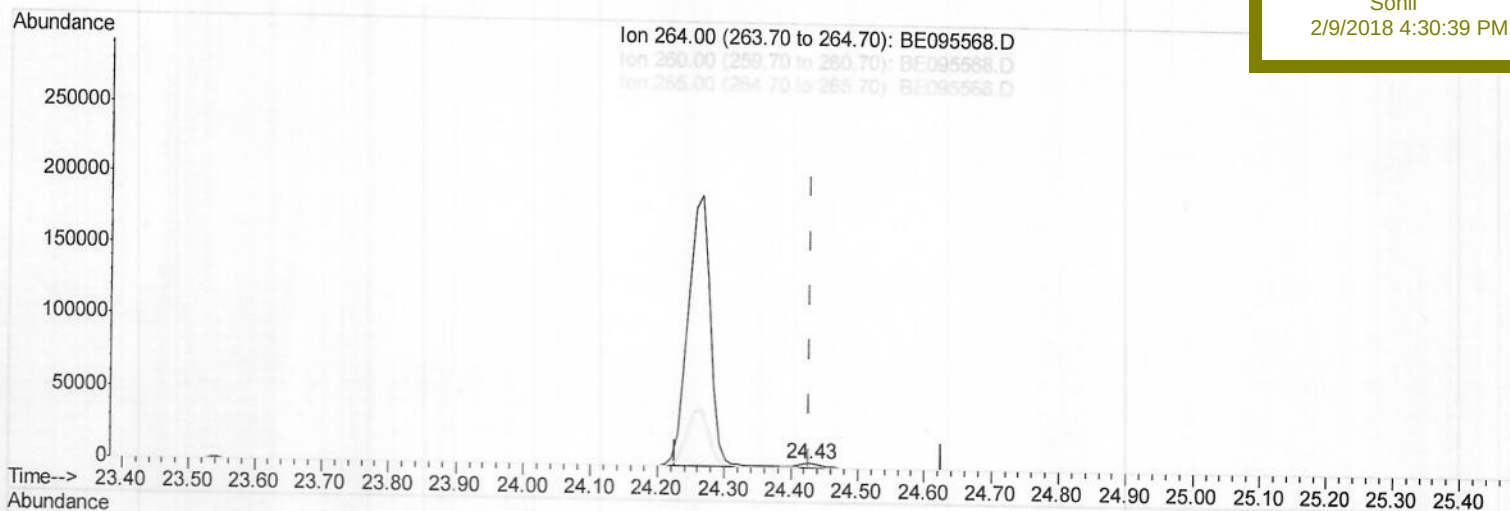

(20) Perylene-d12 (I)

24.427min (+0.001) 0.40ng/ul mS 5402113118

response 6049

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.90
265.00	103.50	25.82#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095568.D
Acq On : 8 Feb 2018 14:32
Operator : SJ/JU
Sample : J1316-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 09 01:17:57 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 00:43:28 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F6D36

Manual Integrations
APPROVED

Sohil
2/9/2018 4:30:39 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1586	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4348	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2775	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6490	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6641	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6049m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2027	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6101	0.25	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095568.D

Acq On : 8 Feb 2018 14:32

Operator : SJ/JU

Sample : J1316-13

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 09 01:17:57 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D36

Manual Integrations
APPROVED

Sohil

2/9/2018 4:30:39 PM

