

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095569.D

Acq On : 8 Feb 2018 15:07

Operator : SJ/JU

Sample : J1316-01

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 09 00:47:40 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6C84

Manual Integrations
APPROVED

Sohil

2/9/2018 4:30:42 PM

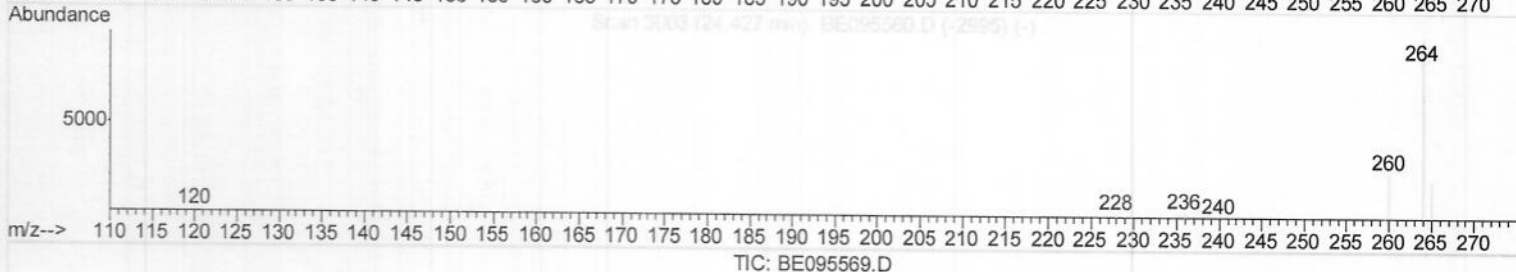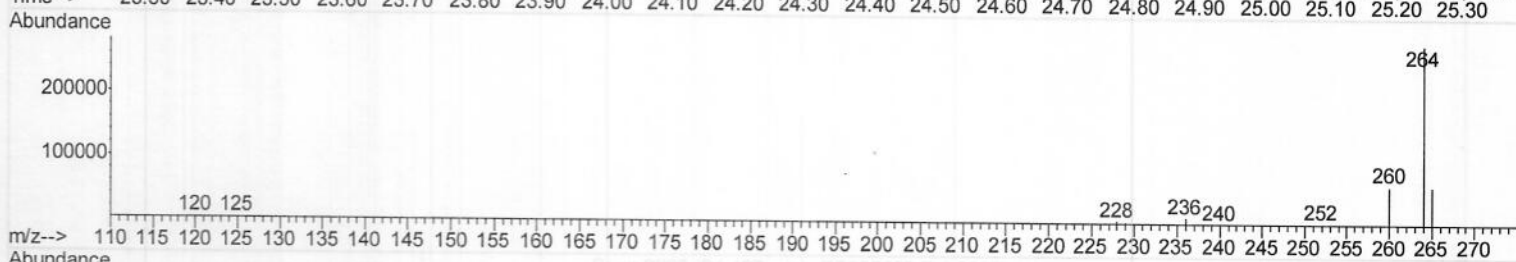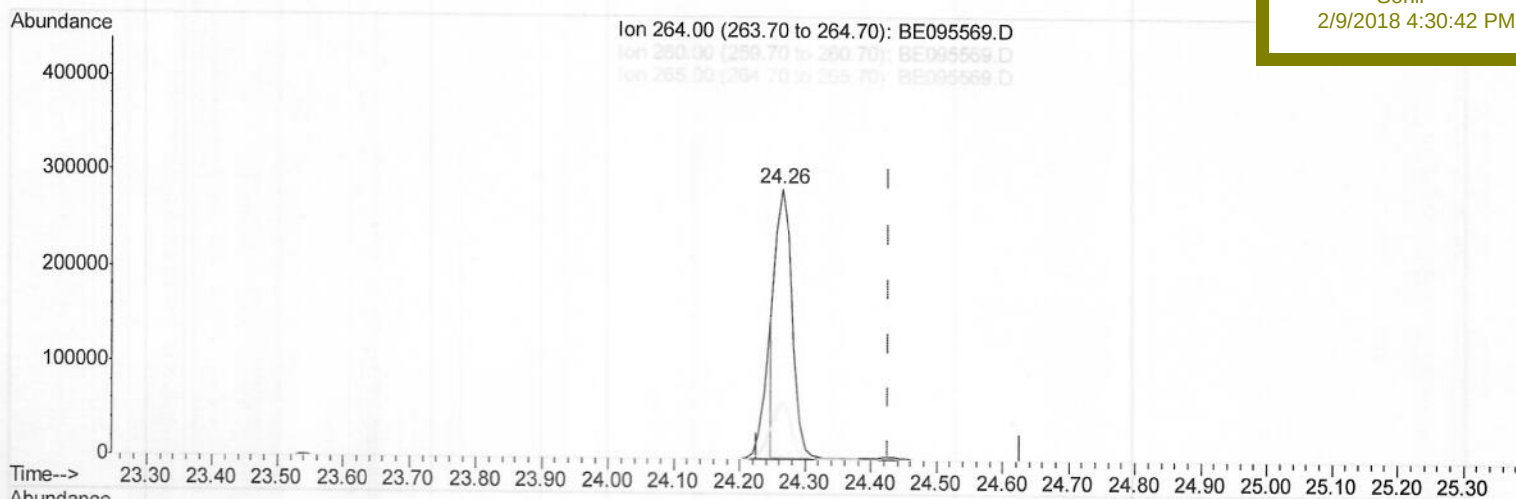

(20) Perylene-d12 (I)

24.264min (-0.162) 0.40ng/ul

response 500652

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.30#
265.00	103.50	21.35#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095569.D

Acq On : 8 Feb 2018 15:07

Operator : SJ/JU

Sample : J1316-01

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 09 00:47:40 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




F6C84

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:42 PM

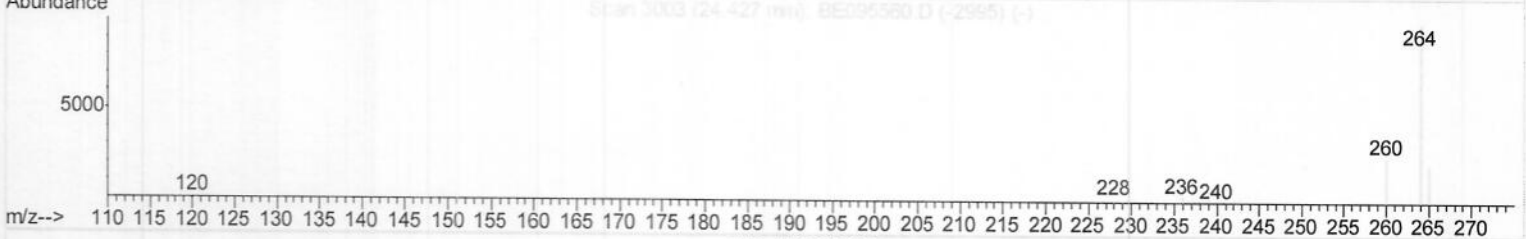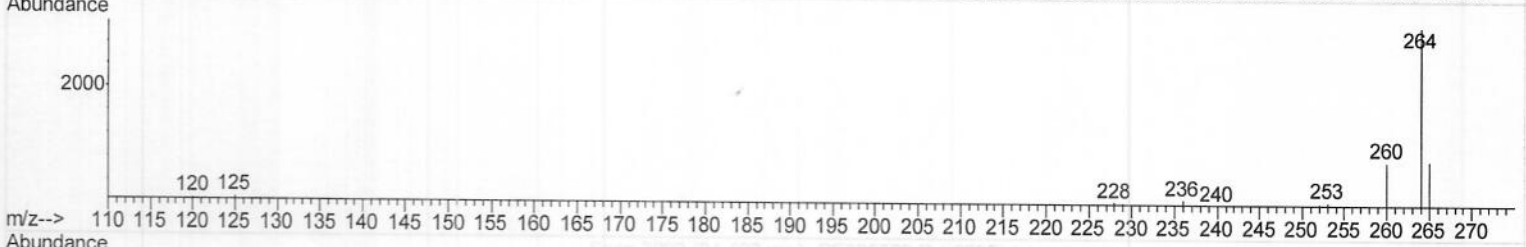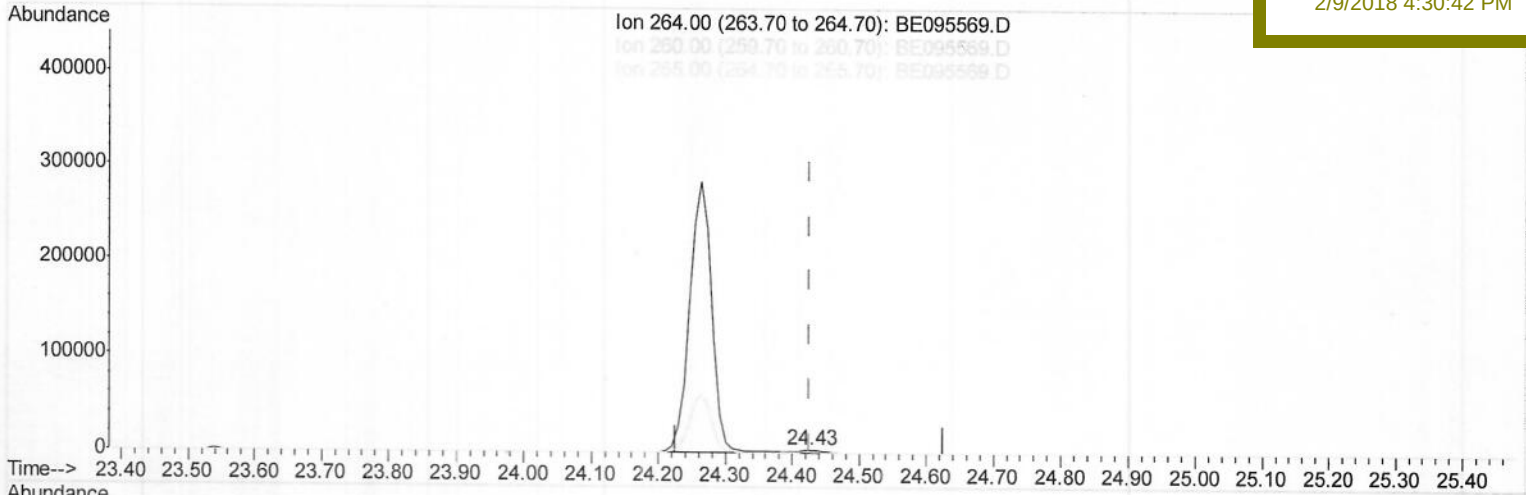

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m SJ 02/13/18

response 5790

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.58
265.00	103.50	26.09#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095569.D

Acq On : 8 Feb 2018 15:07

Operator : SJ/JU

Sample : J1316-01

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 09 01:20:07 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6C84

Manual Integrations
APPROVED

Sohil

2/9/2018 4:30:42 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1637	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4395	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3038	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6514	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6575	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	5790m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3169	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9057	0.36	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JY0213118

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095569.D

Acq On : 8 Feb 2018 15:07

Operator : SJ/JU

Sample : J1316-01

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 09 01:20:07 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 00:43:28 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6C84

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:42 PM

