

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095575.D

Acq On : 8 Feb 2018 18:42

Operator : SJ/JU

Sample : J1316-14

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Feb 09 03:44:16 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




F6D37

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:59 PM

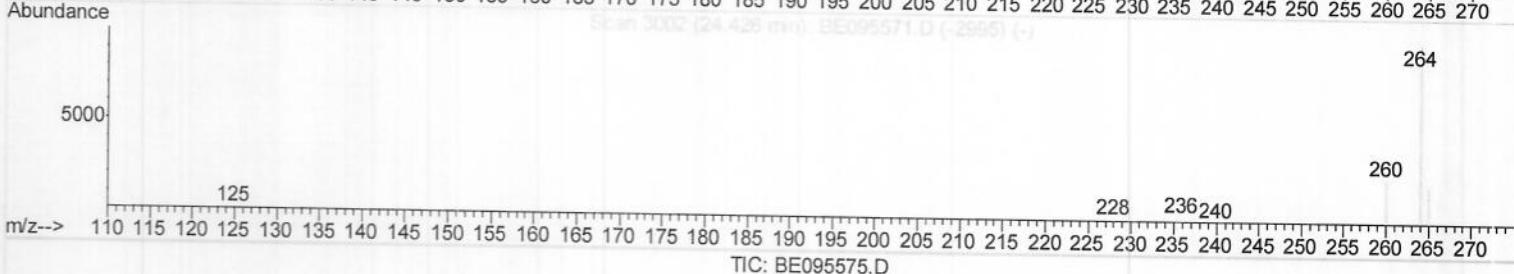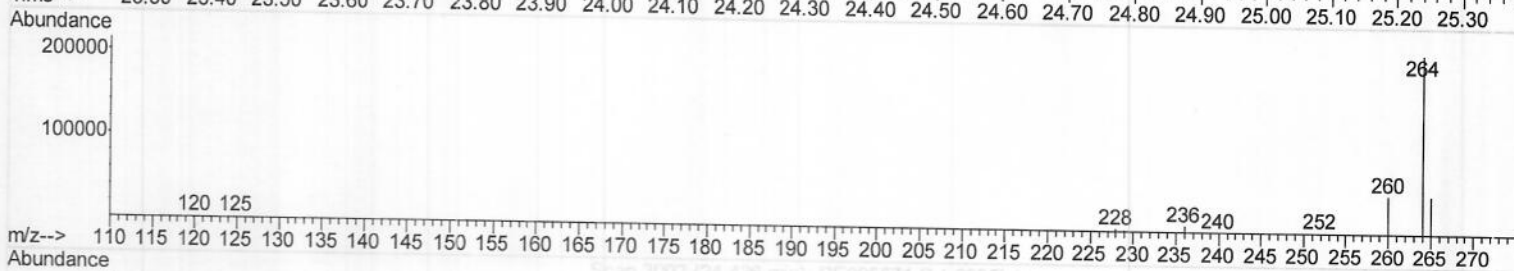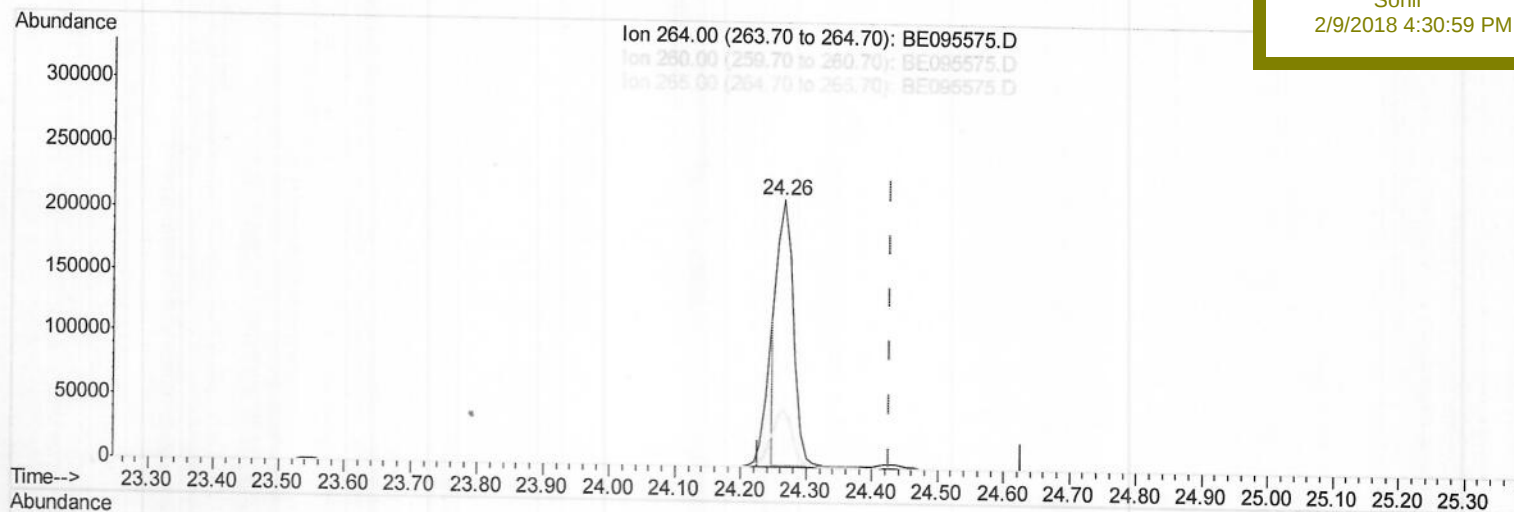

(20) Perylene-d12 (I)

24.264min (-0.162) 0.40ng/ul

response 366437

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.25#
265.00	103.50	21.25#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095575.D

Acq On : 8 Feb 2018 18:42

Operator : SJ/JU

Sample : J1316-14

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Feb 09 03:44:16 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E


Client Sampled :

F6D37

Manual Integrations
APPROVED

Sohil

2/9/2018 4:30:59 PM

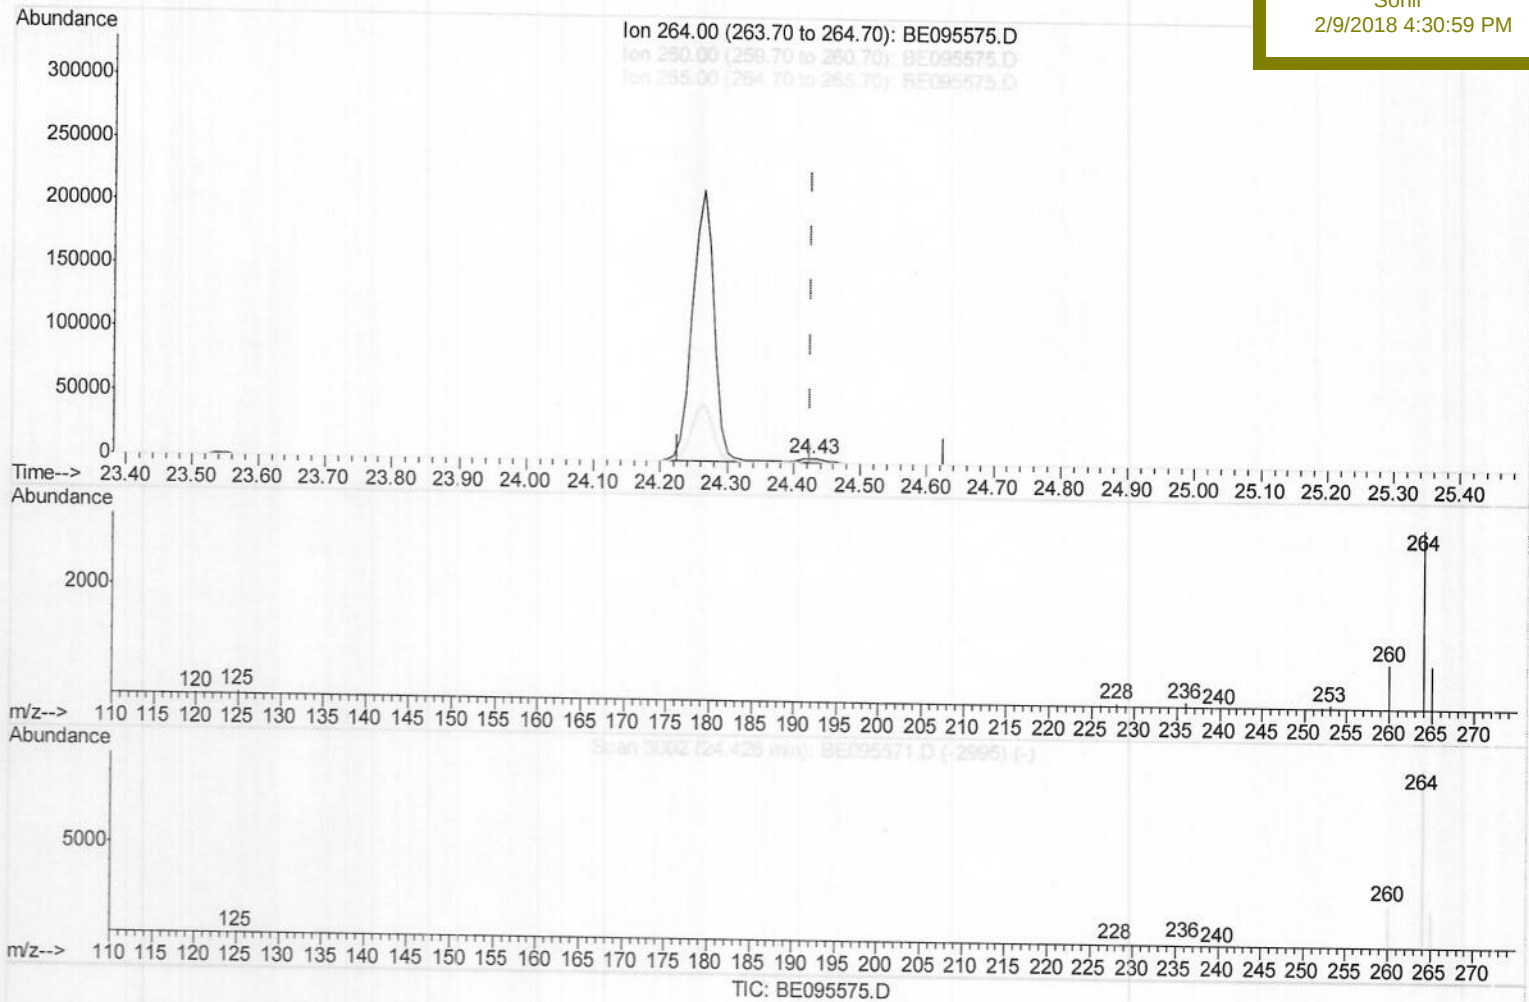

(20) Perylene-d12 (I)

24.427min (+0.000) 0.40ng/ul m J40213118

response 6279

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.98
265.00	103.50	25.68#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095575.D
Acq On : 8 Feb 2018 18:42
Operator : SJ/JU
Sample : J1316-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Feb 09 03:45:26 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F6D37

Manual Integrations
APPROVED

Sohil
2/9/2018 4:30:59 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1693	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4645	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3567	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7256	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6936	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6279m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2330	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6974	0.25	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.72	202	633	0.020	ng/ul	Ovalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095575.D

Acq On : 8 Feb 2018 18:42

Operator : SJ/JU

Sample : J1316-14

Misc :

ALS Vial : 16 Sample Multiplier: 1

Quant Time: Feb 09 03:45:26 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D37

Manual Integrations

APPROVED

Sohil

2/9/2018 4:30:59 PM

