

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095579.D

Acq On : 8 Feb 2018 21:06

Operator : SJ/JU

Sample : J1316-02

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 09 01:48:44 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :


F6C85

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:10 PM

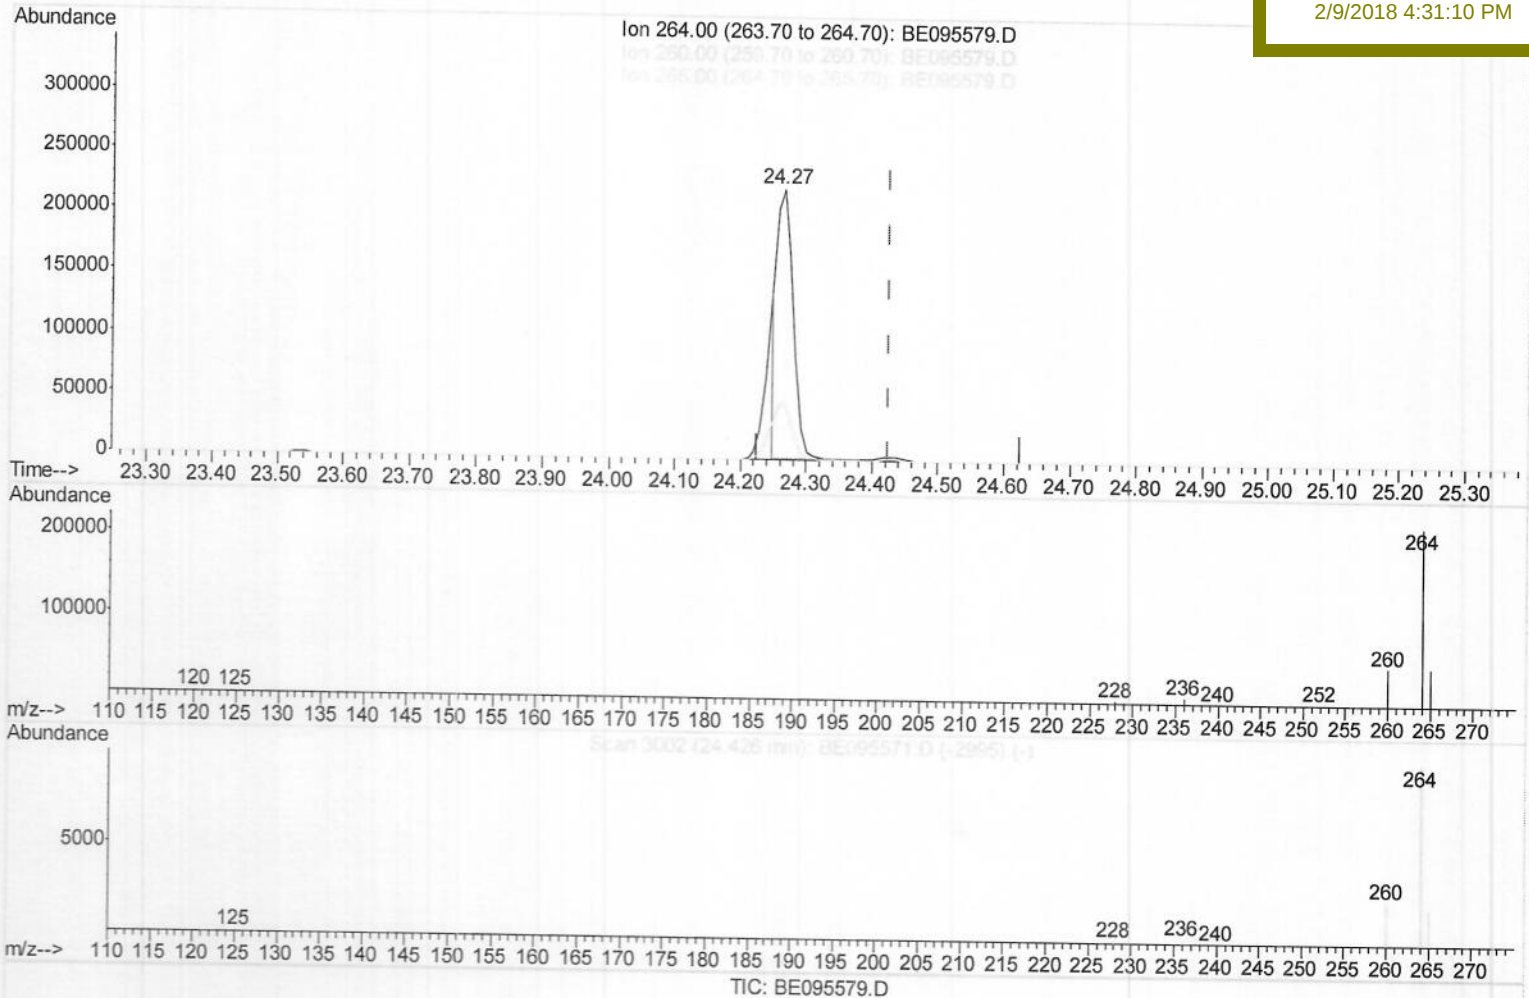

(20) Perylene-d12 (I)

24.265min (-0.161) 0.40ng/ul

response 386058

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.10#
265.00	103.50	21.44#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020618\

Data File : BE095579.D

Acq On : 8 Feb 2018 21:06

Operator : SJ/JU

Sample : J1316-02

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 09 01:48:44 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E



ClientSampleId :

F6C85

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:10 PM

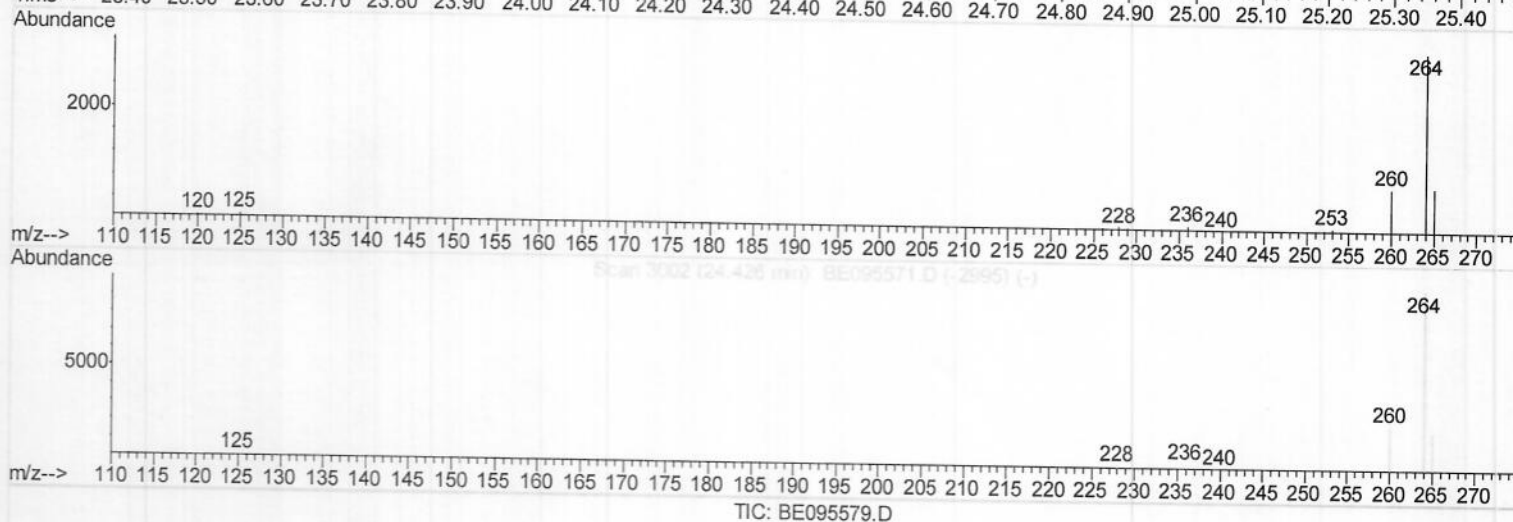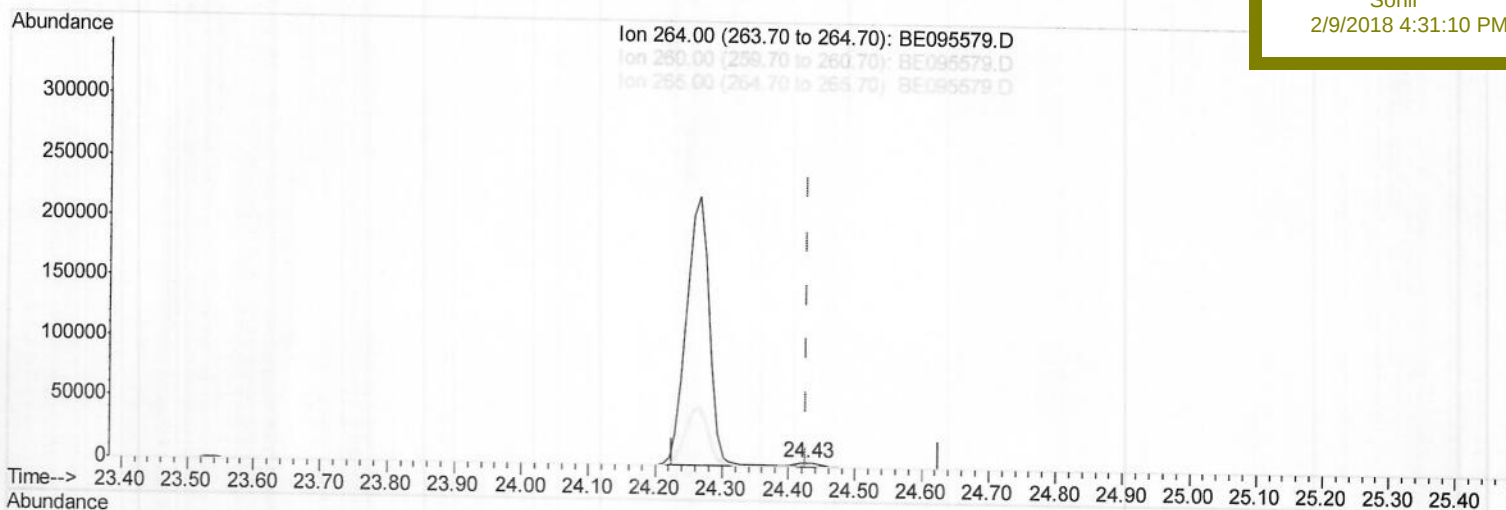

(20) Perylene-d12 (I)

24.427min (+0.001) 0.40ng/ul m } 5402113118

response 6065

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.26
265.00	103.50	25.82#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095579.D
Acq On : 8 Feb 2018 21:06
Operator : SJ/JU
Sample : J1316-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 09 03:53:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration

Instrument :
BNA_E
Client Sampled :
F6C85

Manual Integrations
APPROVED

Sohil
2/9/2018 4:31:10 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1636	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4492	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3008	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7119	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6851	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6065m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2609	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7649	0.28	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095579.D

Acq On : 8 Feb 2018 21:06

Operator : SJ/JU

Sample : J1316-02

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 09 03:53:04 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6C85

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:10 PM

