

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095584.D

Acq On : 9 Feb 2018 00:05

Operator : SJ/JU

Sample : J1316-20

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 09 04:07:13 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018


Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D01

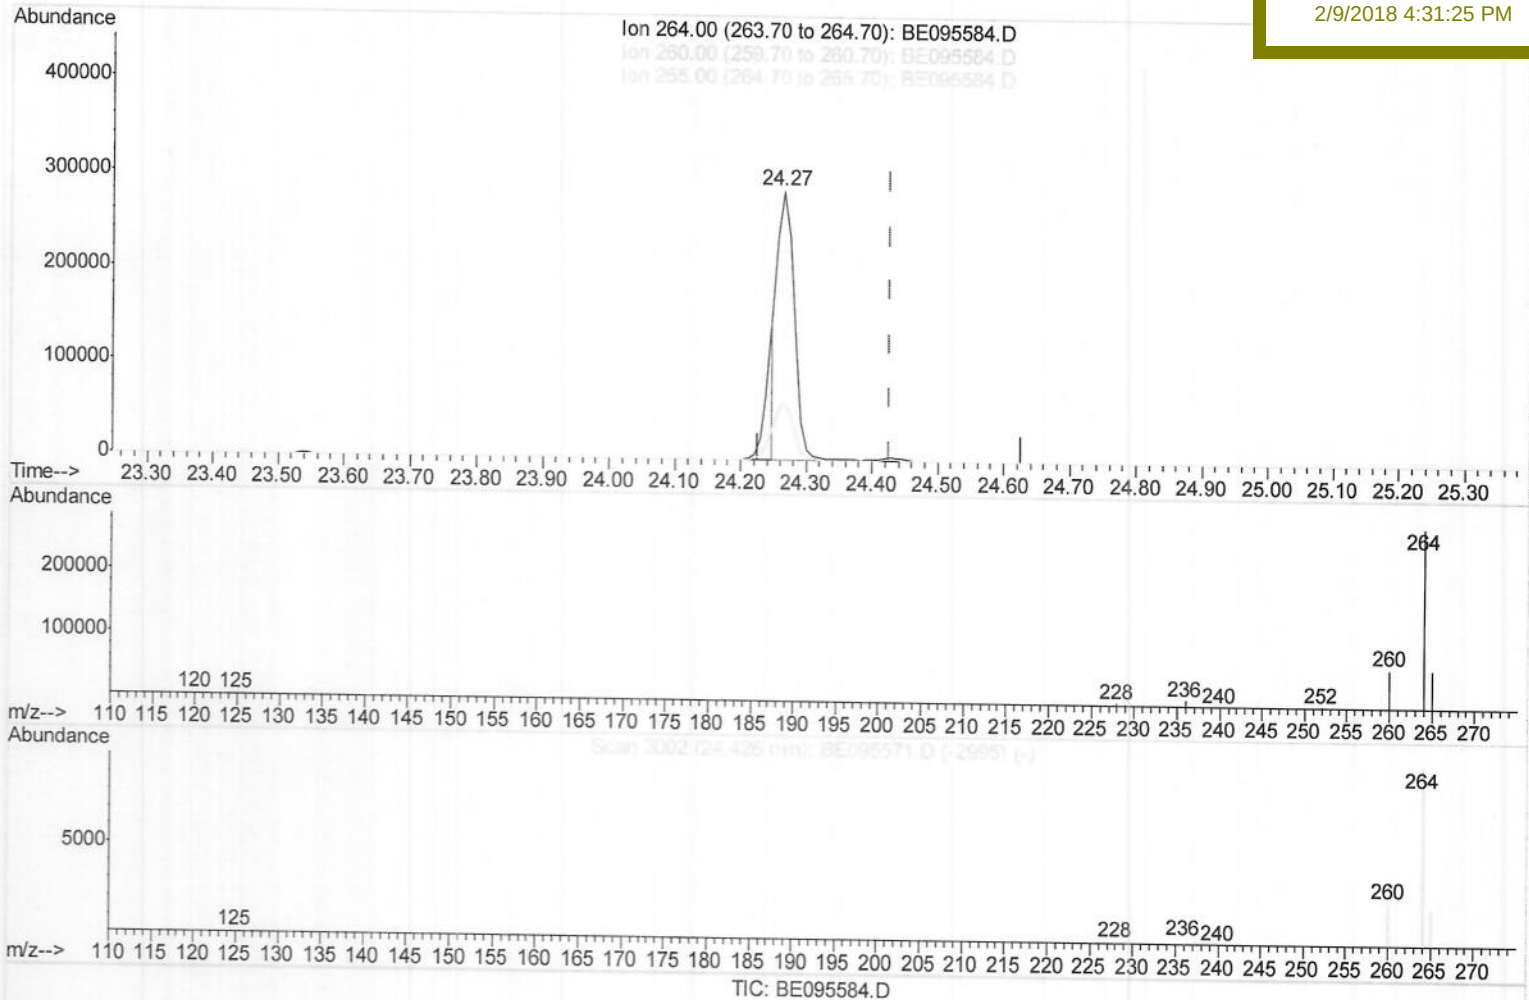Manual Integrations
APPROVEDSohil
2/9/2018 4:31:25 PM

(20) Perylene-d12 (I)

24.265min (-0.161) 0.40ng/ul

response 504096

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.30#
265.00	103.50	21.39#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095584.D

Acq On : 9 Feb 2018 00:05

Operator : SJ/JU

Sample : J1316-20

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 09 04:07:13 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6D01

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:25 PM

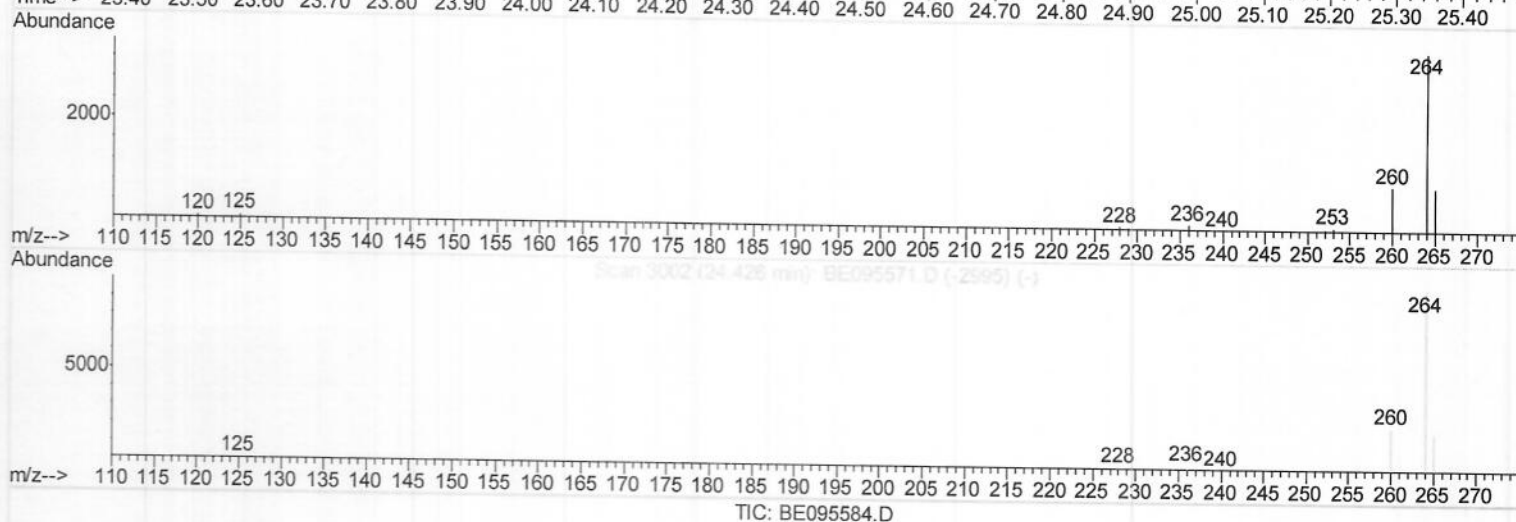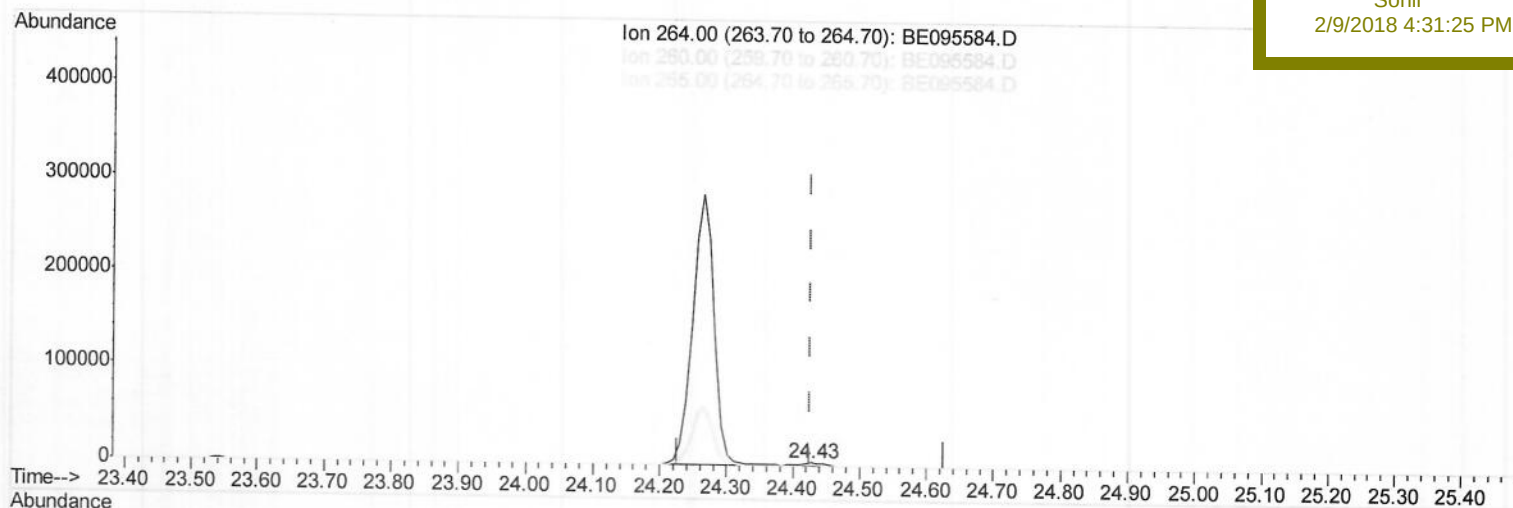

TIC: BE095584.D

(20) Perylene-d12 (I)

24.427min (+0.001) 0.40ng/ul m > 54 02/13/18

response 6763

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.62
265.00	103.50	25.03#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095584.D

Acq On : 9 Feb 2018 00:05

Operator : SJ/JU

Sample : J1316-20

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 09 04:09:17 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D01

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:25 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1764	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4922	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3274	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7382	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7516	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6763m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3127	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9355	0.33	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095584.D

Acq On : 9 Feb 2018 00:05

Operator : SJ/JU

Sample : J1316-20

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 09 04:09:17 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D01

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:25 PM

