

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095585.D

Acq On : 9 Feb 2018 00:41

Operator : SJ/JU

Sample : J1316-11

Misc :

ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 09 04:07:19 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E



ClientSampleId :

F6D34

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:29 PM

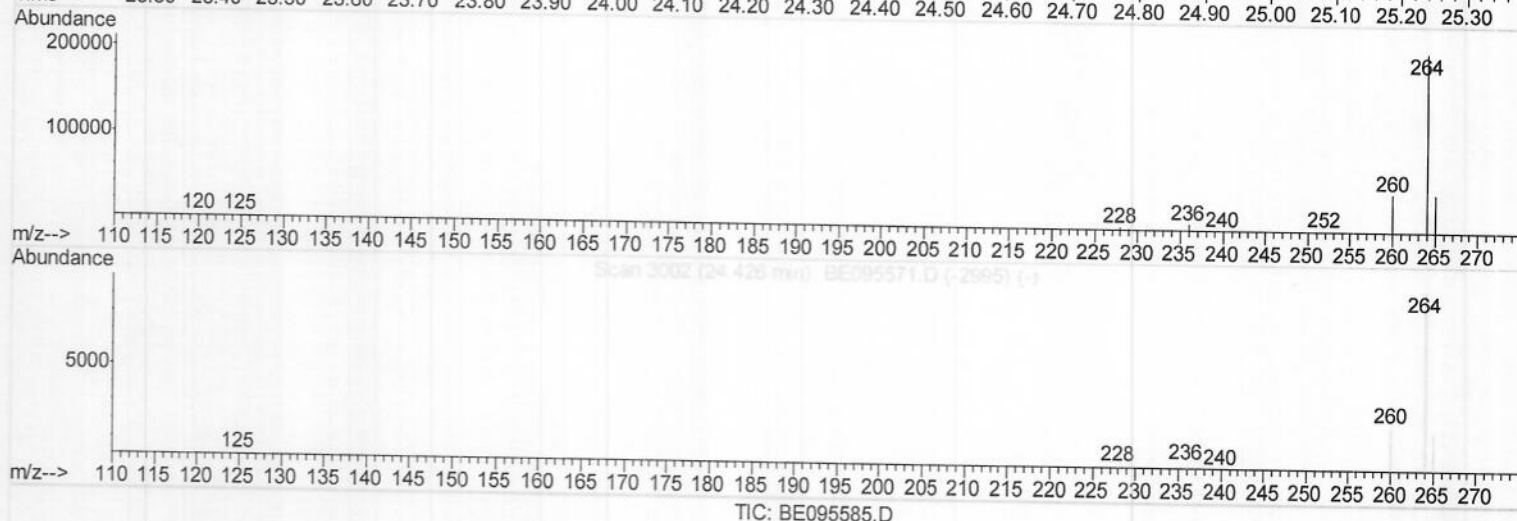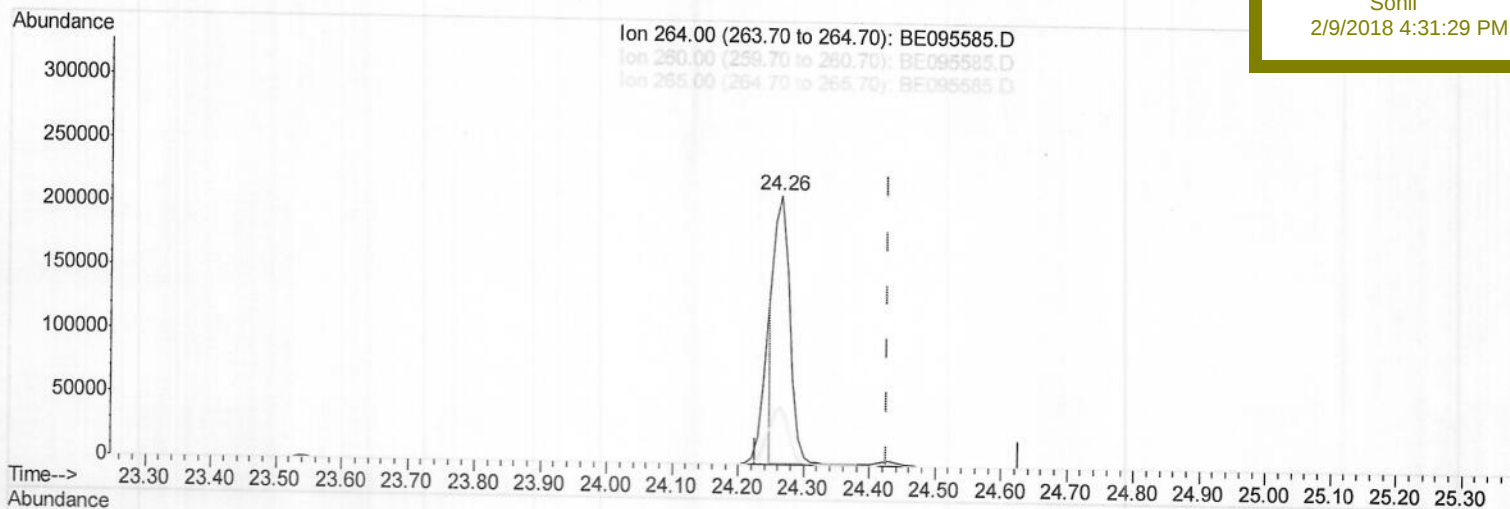

(20) Perylene-d12 (I)

24.265min (-0.161) 0.40ng/ul

response 349121

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.08#
265.00	103.50	21.44#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095585.D

Acq On : 9 Feb 2018 00:41

Operator : SJ/JU

Sample : J1316-11

Misc :

ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 09 04:07:19 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 01:31:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :



F6D34

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:29 PM

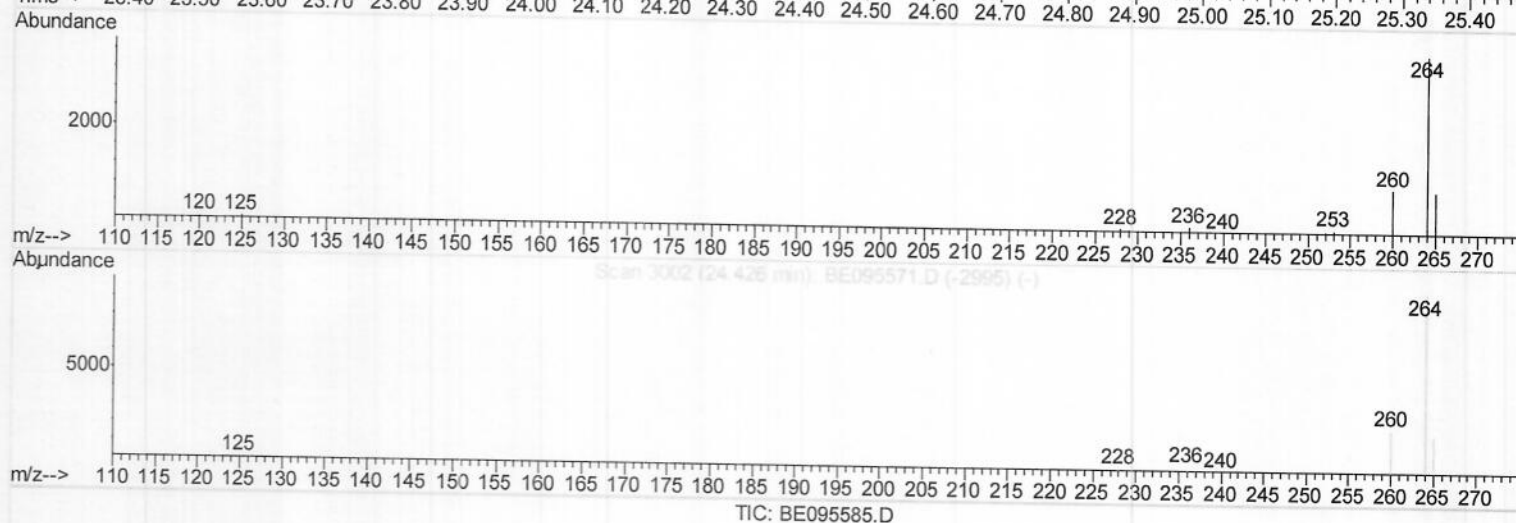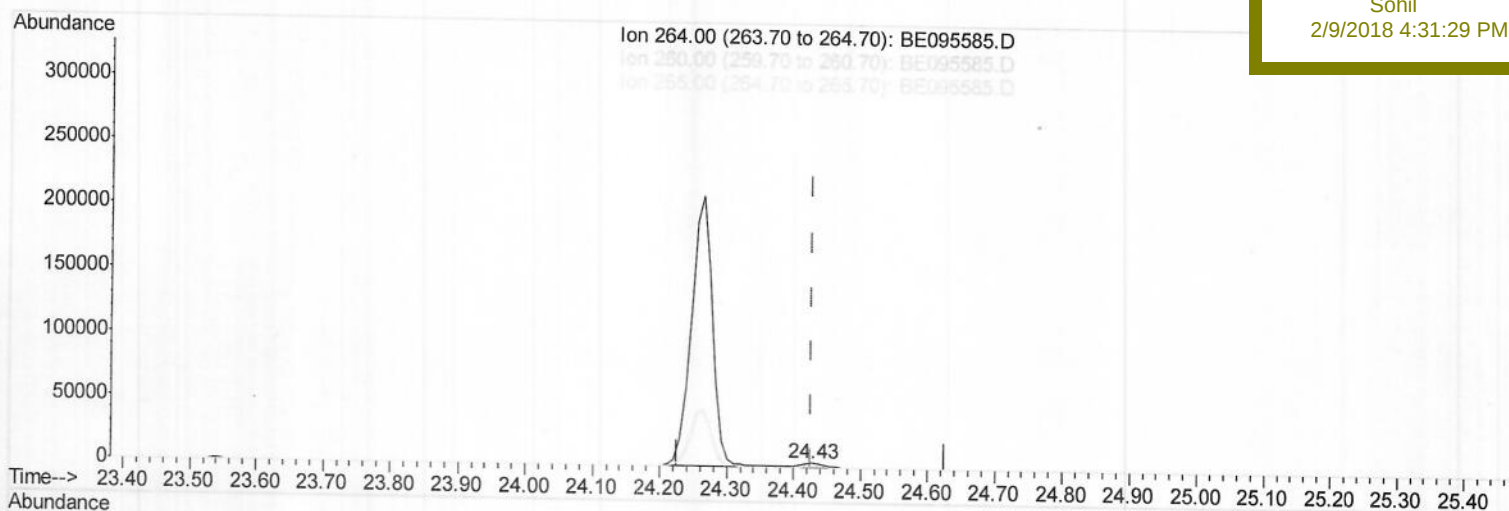

(20) Perylene-d12 (I)

24.427min (+0.001) 0.40ng/ul m 35402113118

response 7620

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.48
265.00	103.50	24.32#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095585.D
Acq On : 9 Feb 2018 00:41
Operator : SJ/JU
Sample : J1316-11
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 09 04:11:20 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration

Instrument :
BNA_E
Client Sampled :
F6D34

Manual Integrations
APPROVED

Sohil
2/9/2018 4:31:29 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1882	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5352	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3485	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8260	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8008	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7620m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2365	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6704	0.21	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095585.D
Acq On : 9 Feb 2018 00:41
Operator : SJ/JU
Sample : J1316-11
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 09 04:11:20 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 01:31:22 2018
Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D34

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:29 PM

