

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095587.D
 Acq On : 9 Feb 2018 2:46
 Operator : SJ/JU
 Sample : J1317-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 09 04:49:01 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 04:15:12 2018
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F6D07

Manual Integrations
 APPROVED

Sohil
 2/9/2018 4:31:35 PM

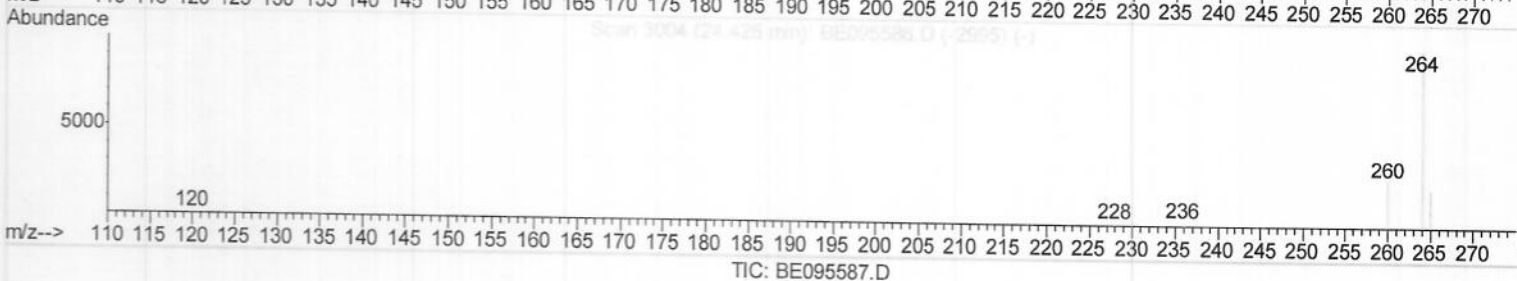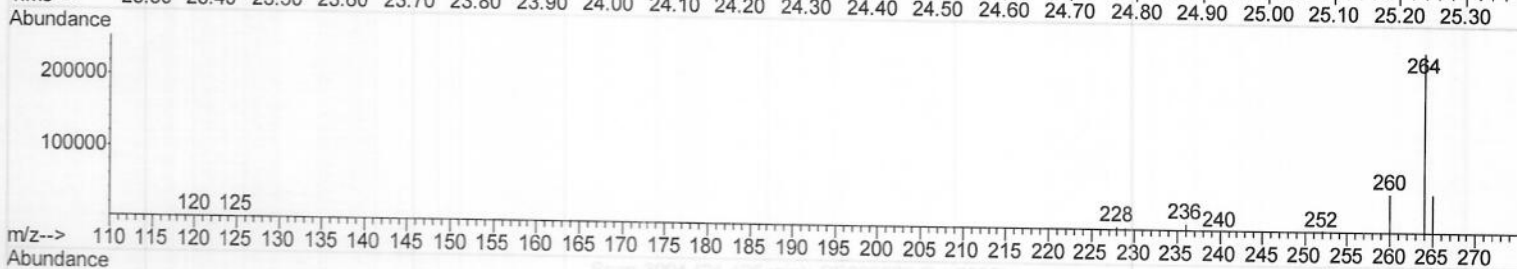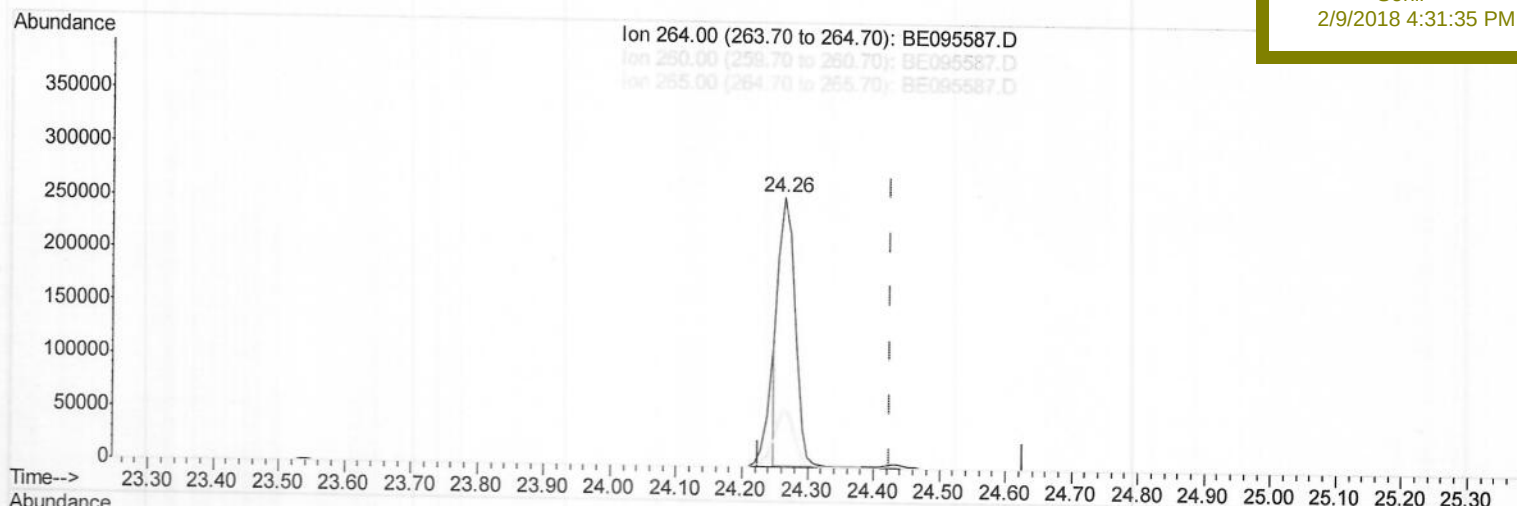

(20) Perylene-d12 (I)

24.264min (-0.162) 0.40ng/ul

response 450280

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.33#
265.00	103.50	21.22#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095587.D

Acq On : 9 Feb 2018 2:46

Operator : SJ/JU

Sample : J1317-14

Misc :

ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 09 04:49:01 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E



ClientSampleId :

F6D07

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:35 PM

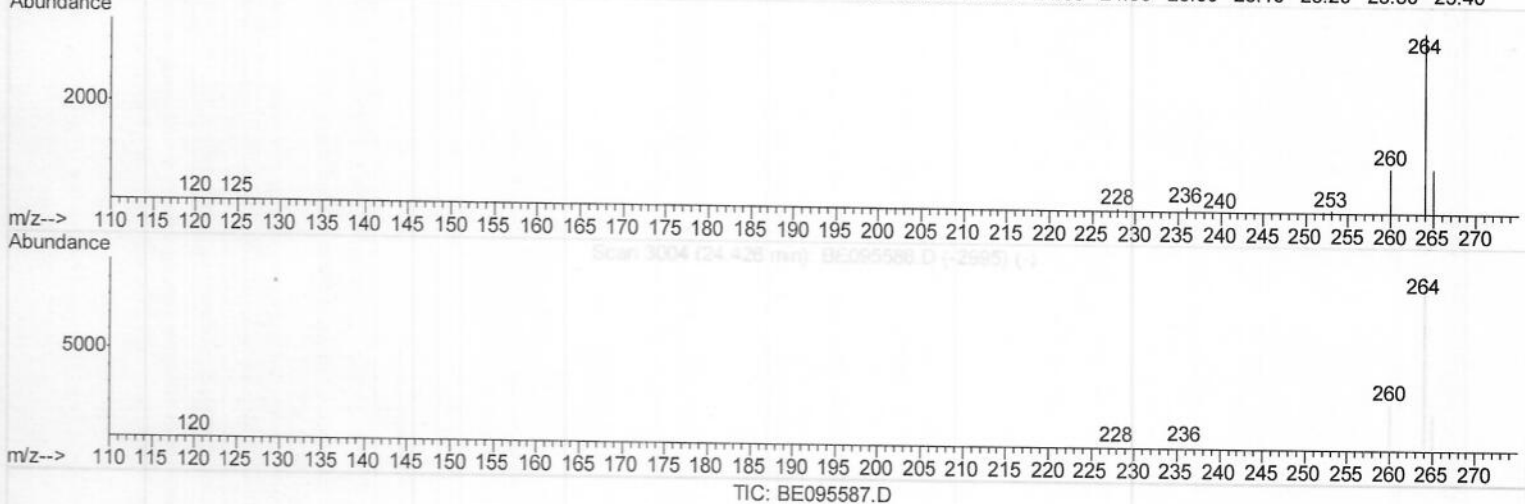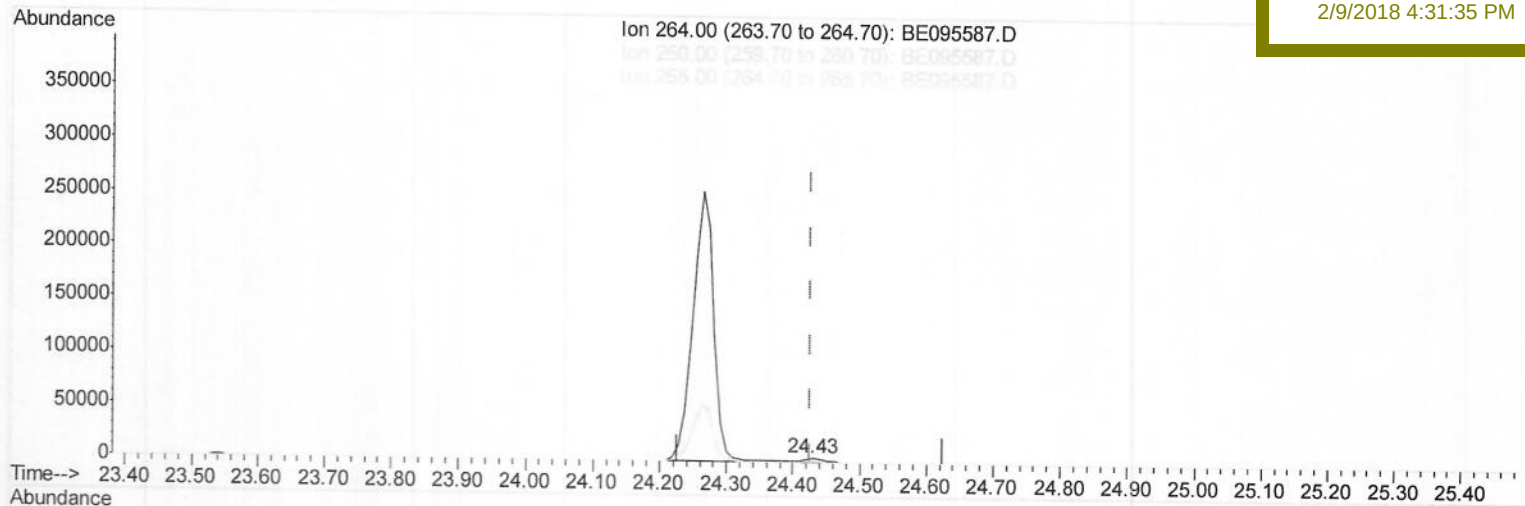

(20) Perylene-d12 (I)

24.426min (+0.000) 0.40ng/ul m> 540213118

response 6941

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.61
265.00	103.50	25.58#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095587.D

Acq On : 9 Feb 2018 2:46

Operator : SJ/JU

Sample : J1317-14

Misc :

ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 09 04:52:06 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6D07

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:35 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	1911	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5390	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3441	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8183	0.40	ng/ul	0.00
16) Chrysene-d12	21.79	240	7805	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6941m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2913	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7990	0.26	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095587.D
Acq On : 9 Feb 2018 2:46
Operator : SJ/JU
Sample : J1317-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 09 04:52:06 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 04:15:12 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F6D07

Manual Integrations
APPROVED

Sohil
2/9/2018 4:31:35 PM

