

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:28:49 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




F6C78

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:50 PM

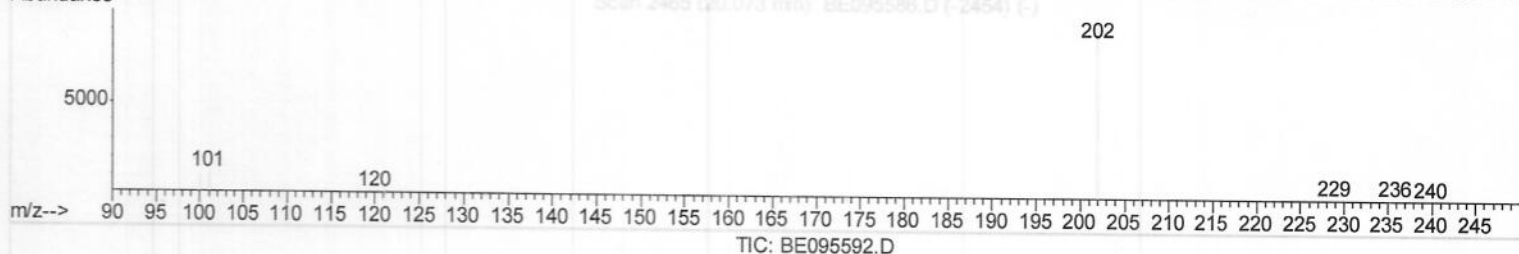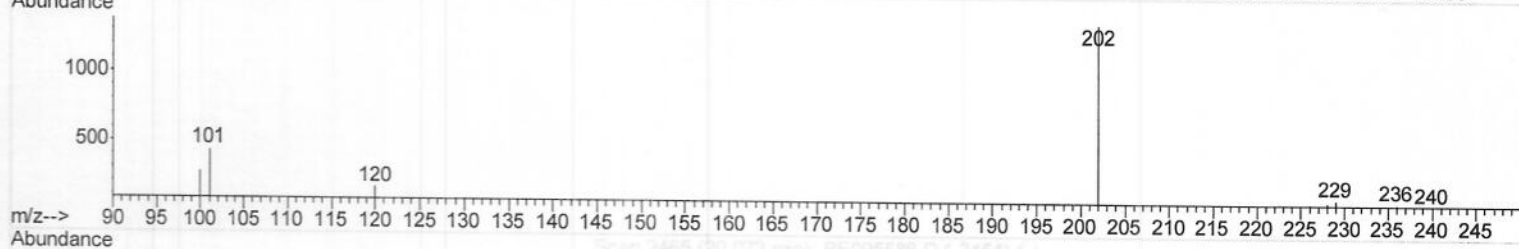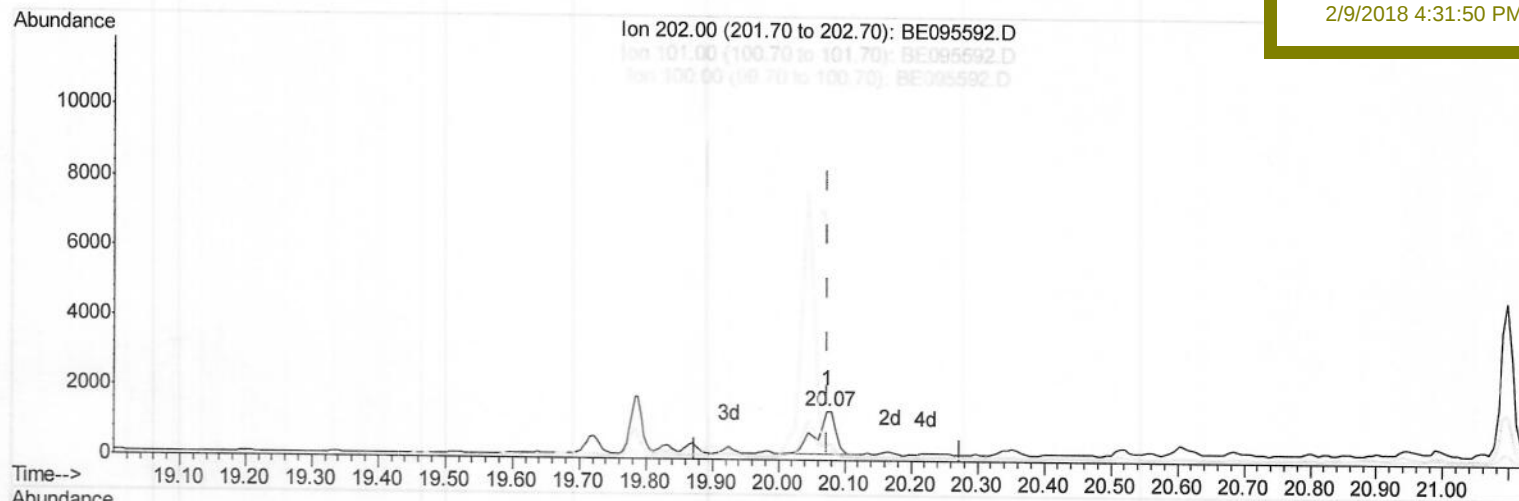

(17) Pyrene

20.073min (+0.000) 0.11ng/ul

response 3020

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	31.44#
100.00	19.50	19.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:28:49 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6C78

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:50 PM

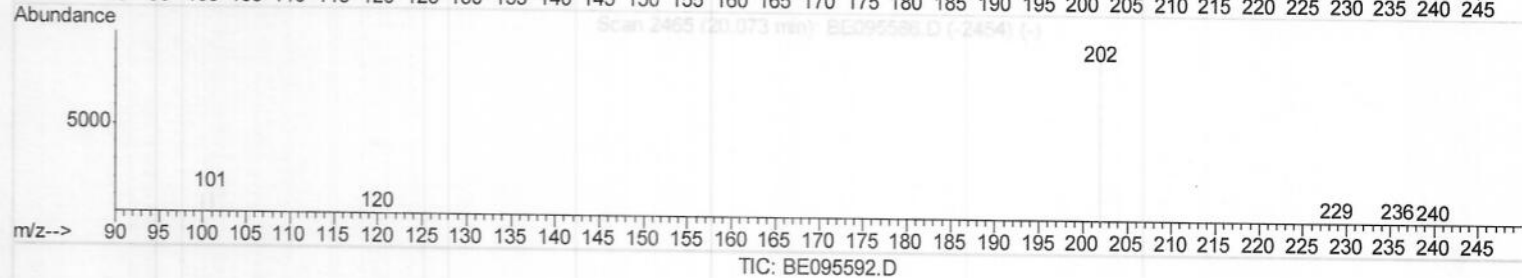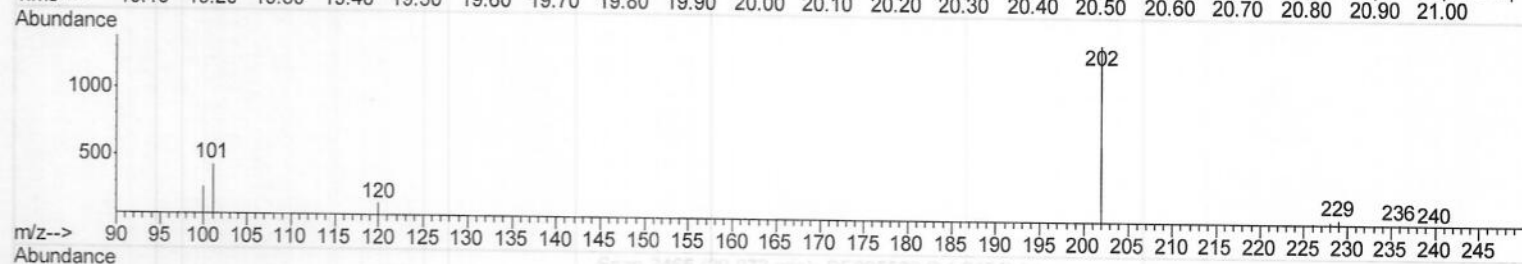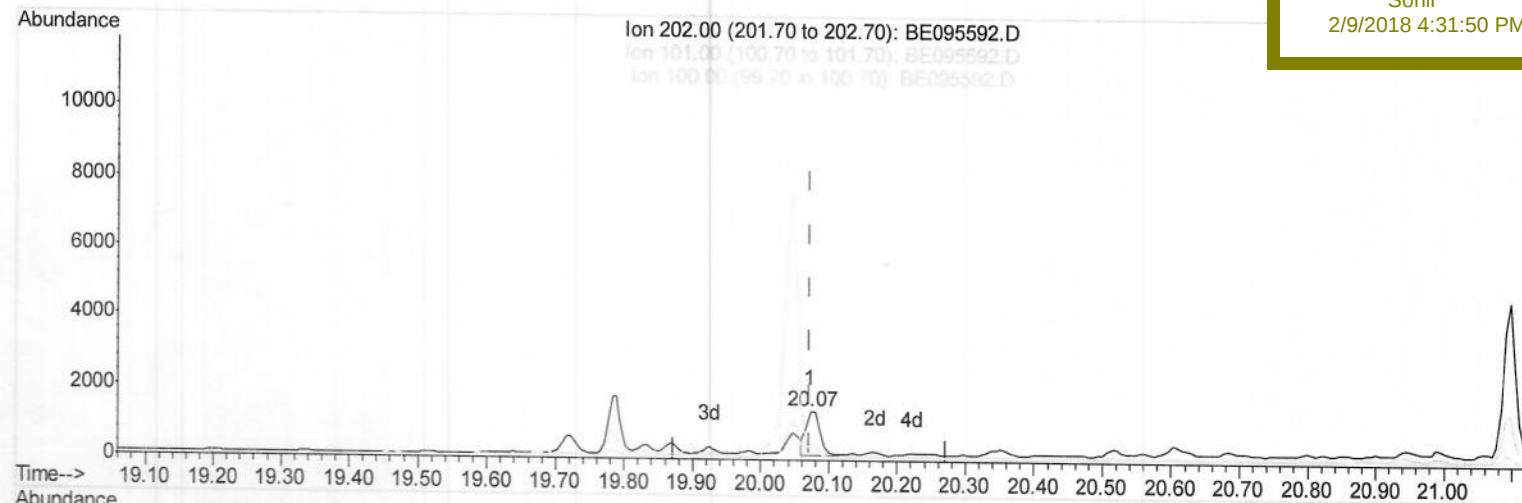

(17) Pyrene

20.073min (+0.000) 0.06ng/ul m) JY0213118

response 1710

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	31.44#
100.00	19.50	19.29
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:28:49 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :


F6C78

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:50 PM

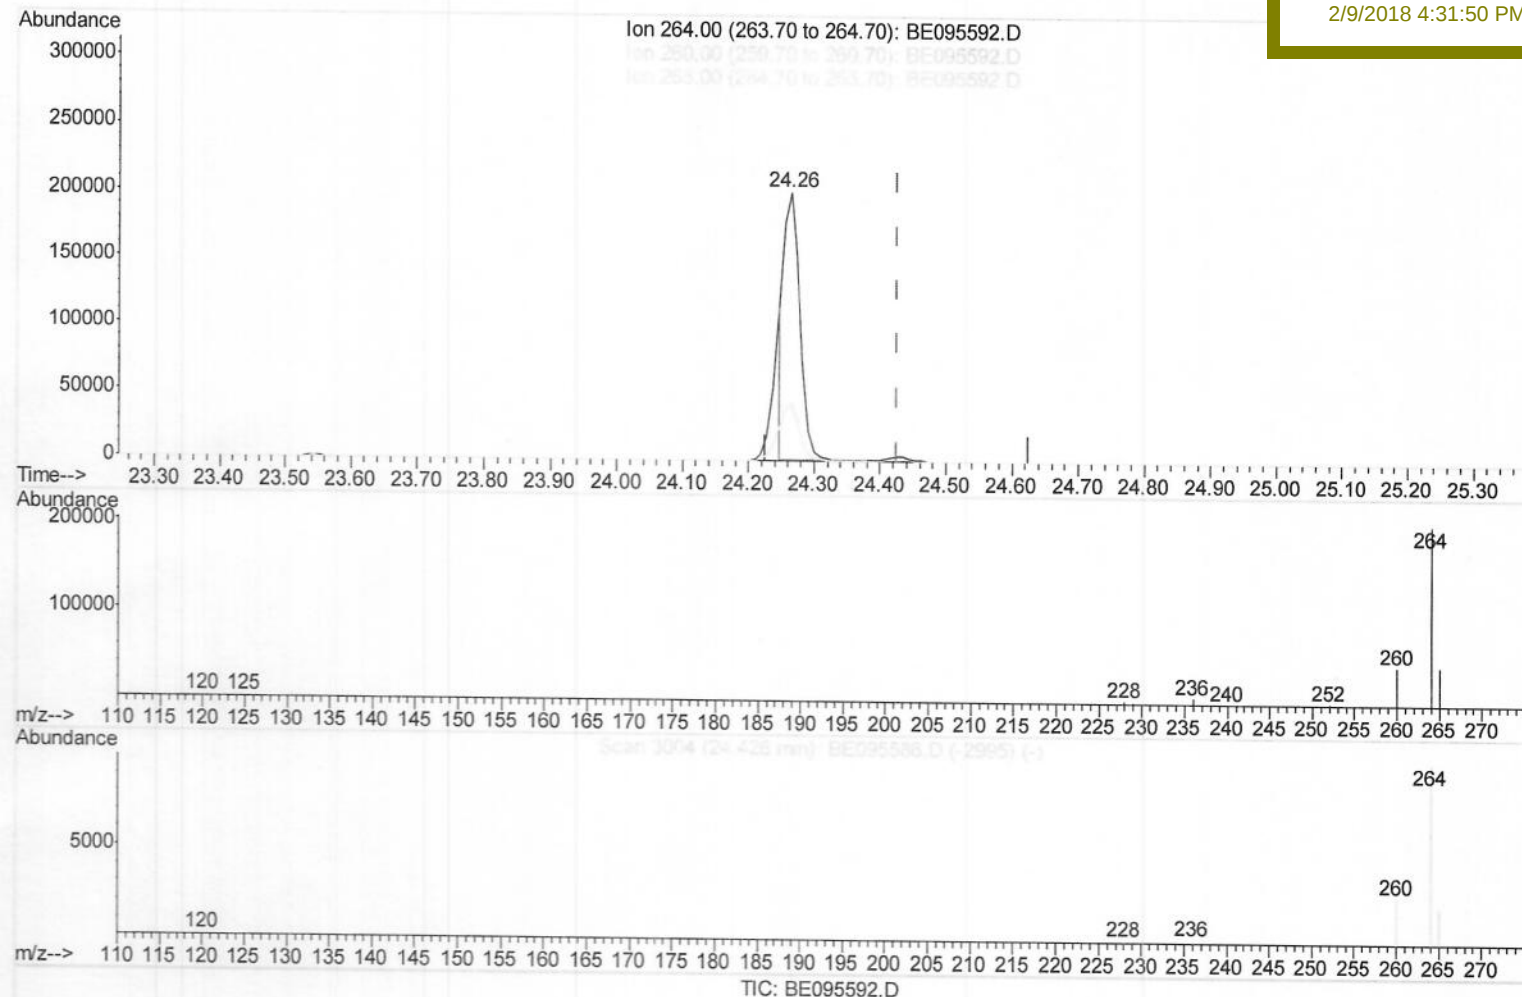

(20) Perylene-d12 (I)

24.264min (-0.162) 0.40ng/ul

response 343873

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.07#
265.00	103.50	21.37#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:28:49 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E



ClientSampleId :

F6C78

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:50 PM

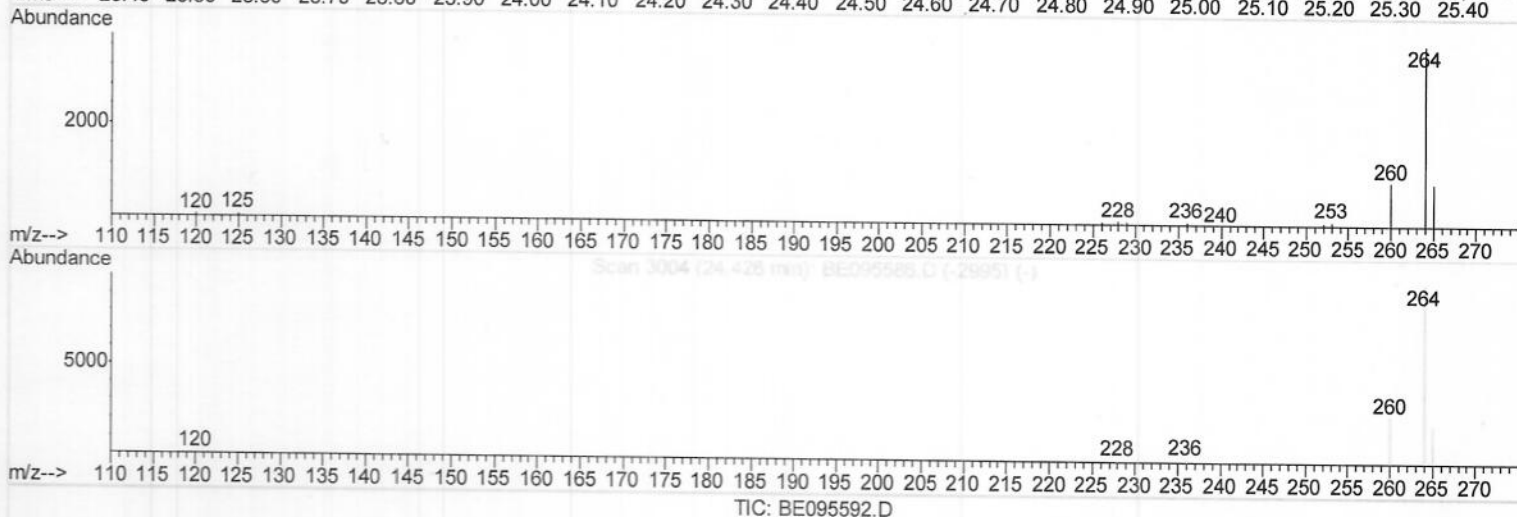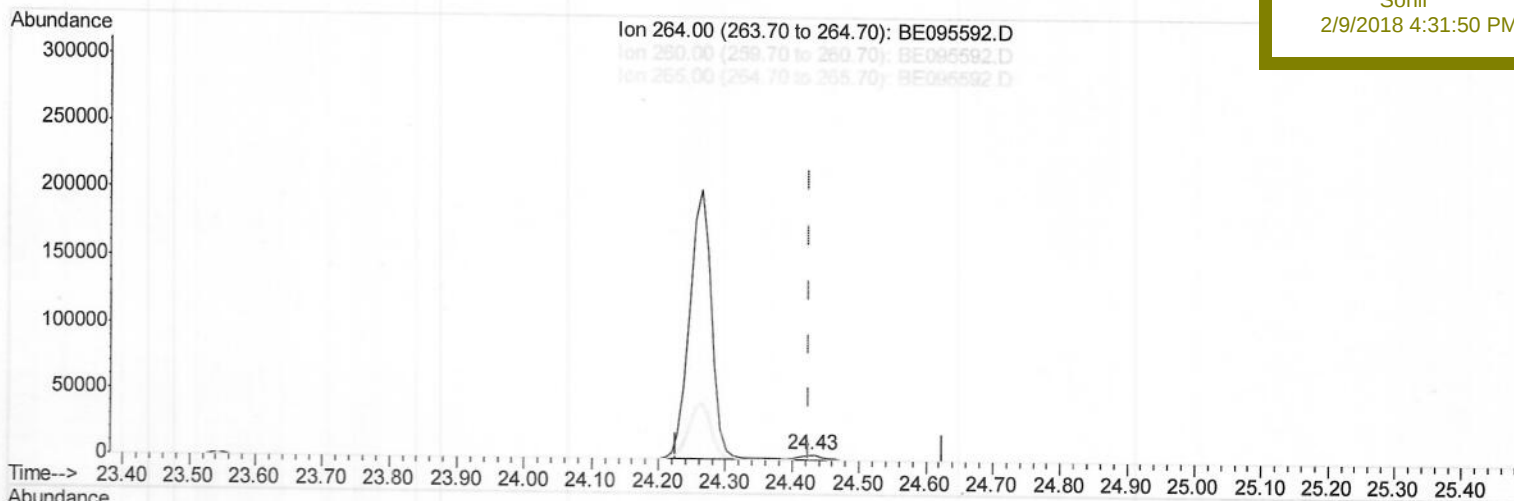

(20) Perylene-d12 (I)

24.426min (+0.000) 0.40ng/ul m > JY 02113118

response 7584

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.64
265.00	103.50	26.40#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:31:07 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6C78

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:50 PM

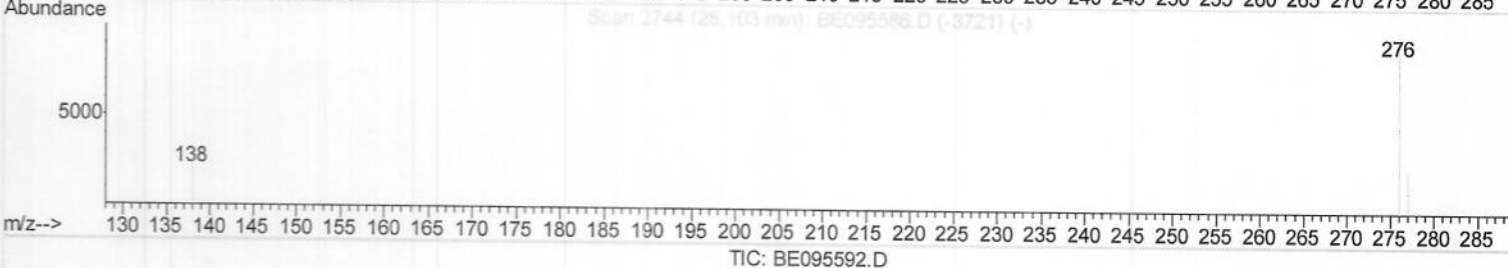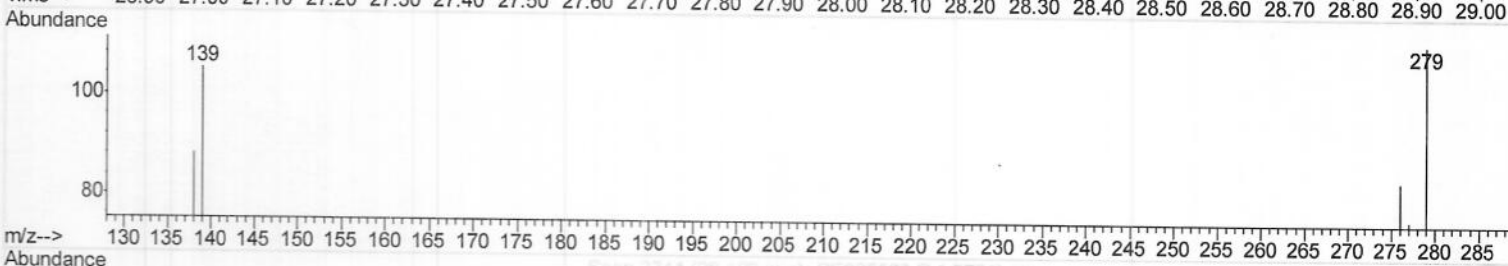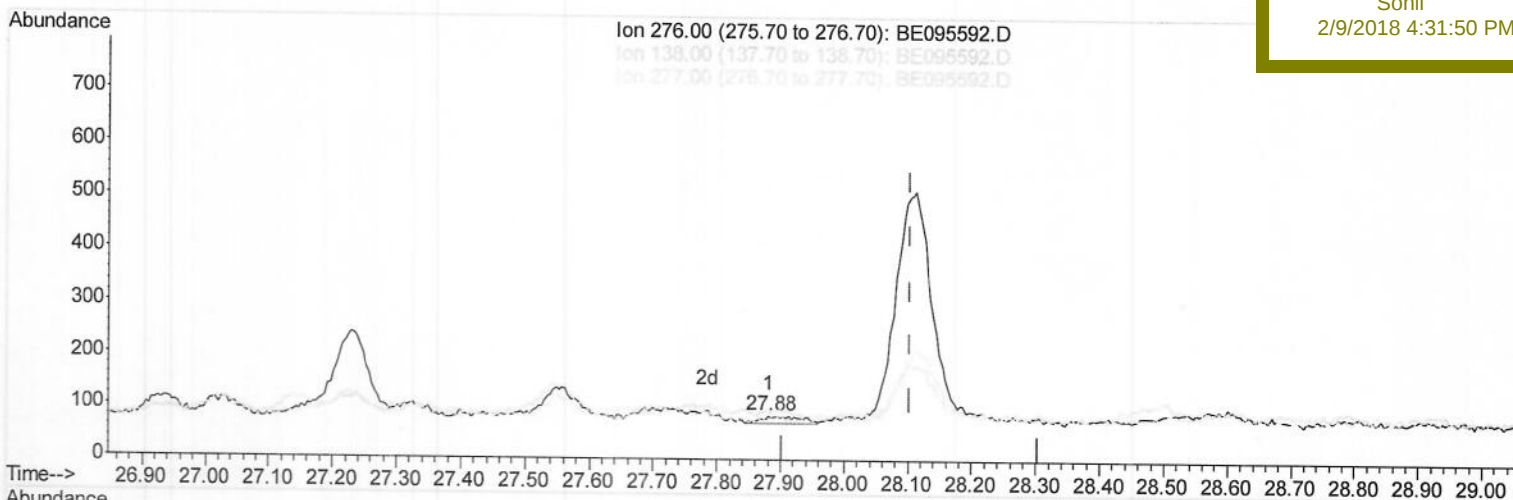

TIC: BE095592.D

(26) Benzo(g,h,i)perylene

27.881min (-0.223) 0.00ng/ul

response 48

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	104.76#
277.00	25.60	90.48#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:31:07 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




F6C78

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:50 PM

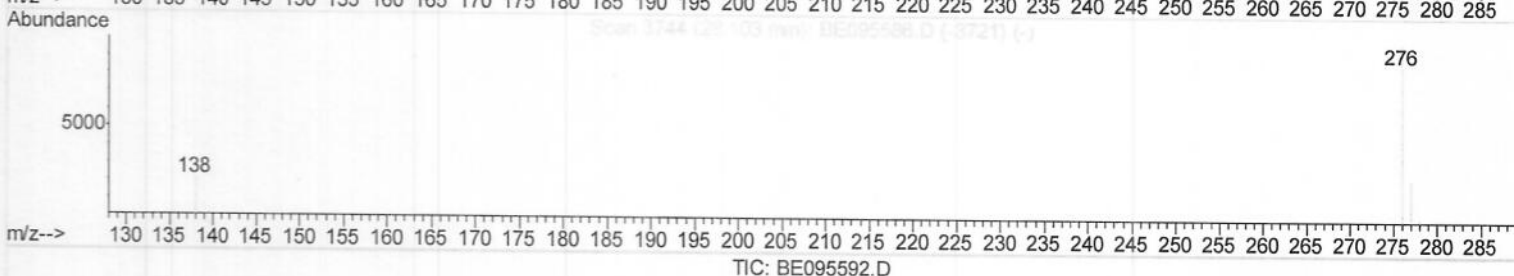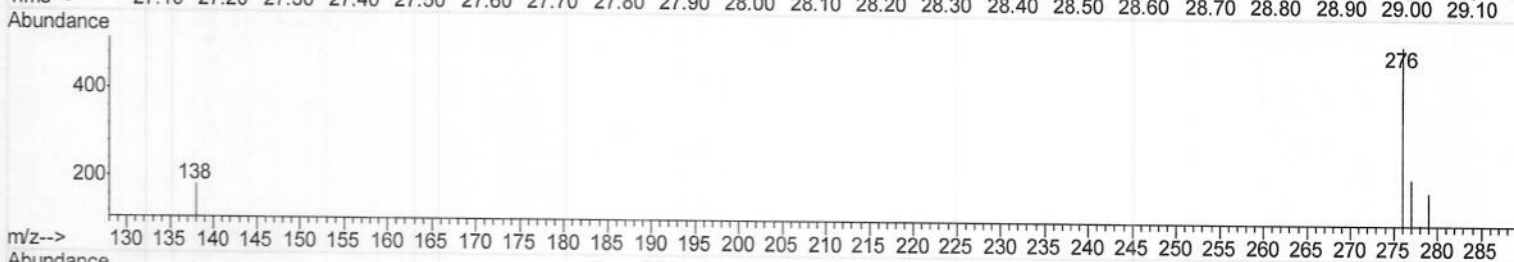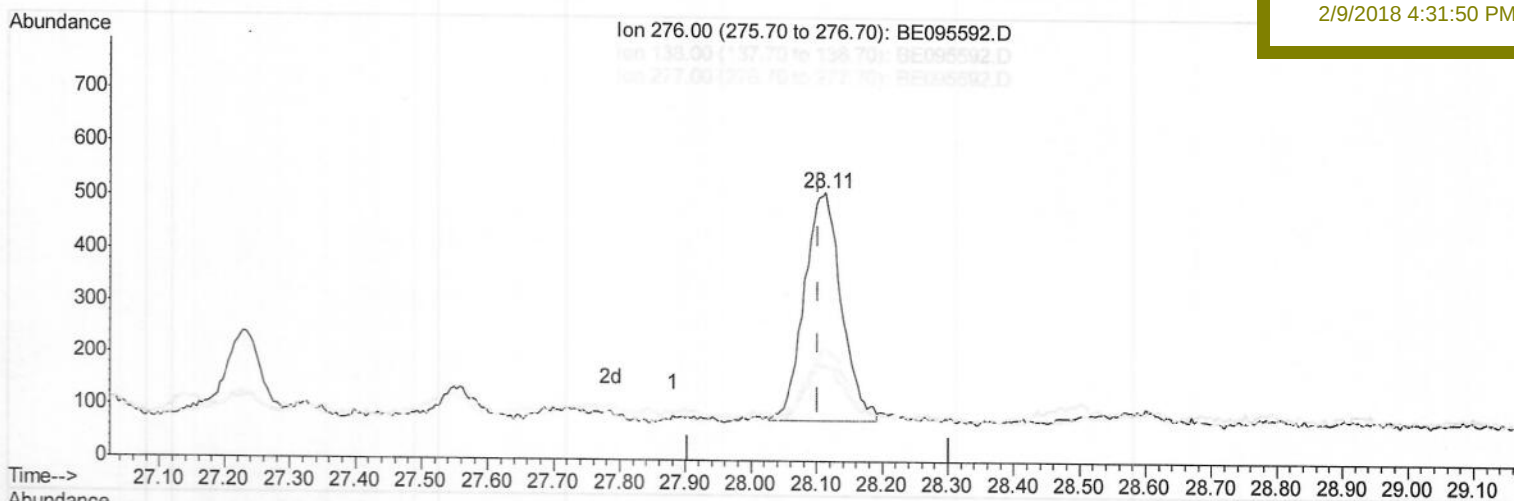

(26) Benzo(g,h,i)perylene

28.113min (+0.010) 0.08ng/ul m) J40213118

response 1708

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	35.35#
277.00	25.60	41.41#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:32:45 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E

Client Sample Id :

F6C78

Manual Integrations
APPROVED

Sohil

2/9/2018 4:31:50 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
--------------------	------	------	----------	------	-------	-----------

1) 1,4-Dichlorobenzene-d4	8.43	152	1927	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5608	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3606	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8528	0.40	ng/ul	0.00
16) Chrysene-d12	21.79	240	8088	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7584m)	0.40	ng/ul	0.00

J40213118

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.81	152	2393	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6843	0.21	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Ovalue
7) Acenaphthylene	14.74	152	674	0.039	ng/ul#	77
11) Pentachlorophenol	17.36	266	639	0.387	ng/ul	98
15) Fluoranthene	19.72	202	784	0.021	ng/ul	85
17) Pyrene	20.07	202	1710m)	0.063	ng/ul	
26) Benzo(a,h,i)perylene	28.11	276	1708m)	0.077	ng/ul	

J40213118

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\

Data File : BE095592.D

Acq On : 9 Feb 2018 5:45

Operator : SJ/JU

Sample : J1317-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 09 06:32:45 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 09 04:15:12 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6C78

Manual Integrations

APPROVED

Sohil

2/9/2018 4:31:50 PM

