

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
 Data File : BE095567.D
 Acq On : 8 Feb 2018 13:56
 Operator : SJ/JU
 Sample : J1316-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D41

Manual Integrations
 APPROVED

Sohil
 2/9/2018 4:30:36 PM

Quant Time: Feb 09 01:16:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 00:43:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1659	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4441	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2808	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6622	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6728	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	5998m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	1948	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6093	0.24	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	133	0.104	ng/ul	Ovalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020818\
Data File : BE095567.D
Acq On : 8 Feb 2018 13:56
Operator : SJ/JU
Sample : J1316-10
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D41

Manual Integrations
APPROVED

Sohil
2/9/2018 4:30:36 PM

Quant Time: Feb 09 01:16:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 00:43:28 2018
Response via : Initial Calibration

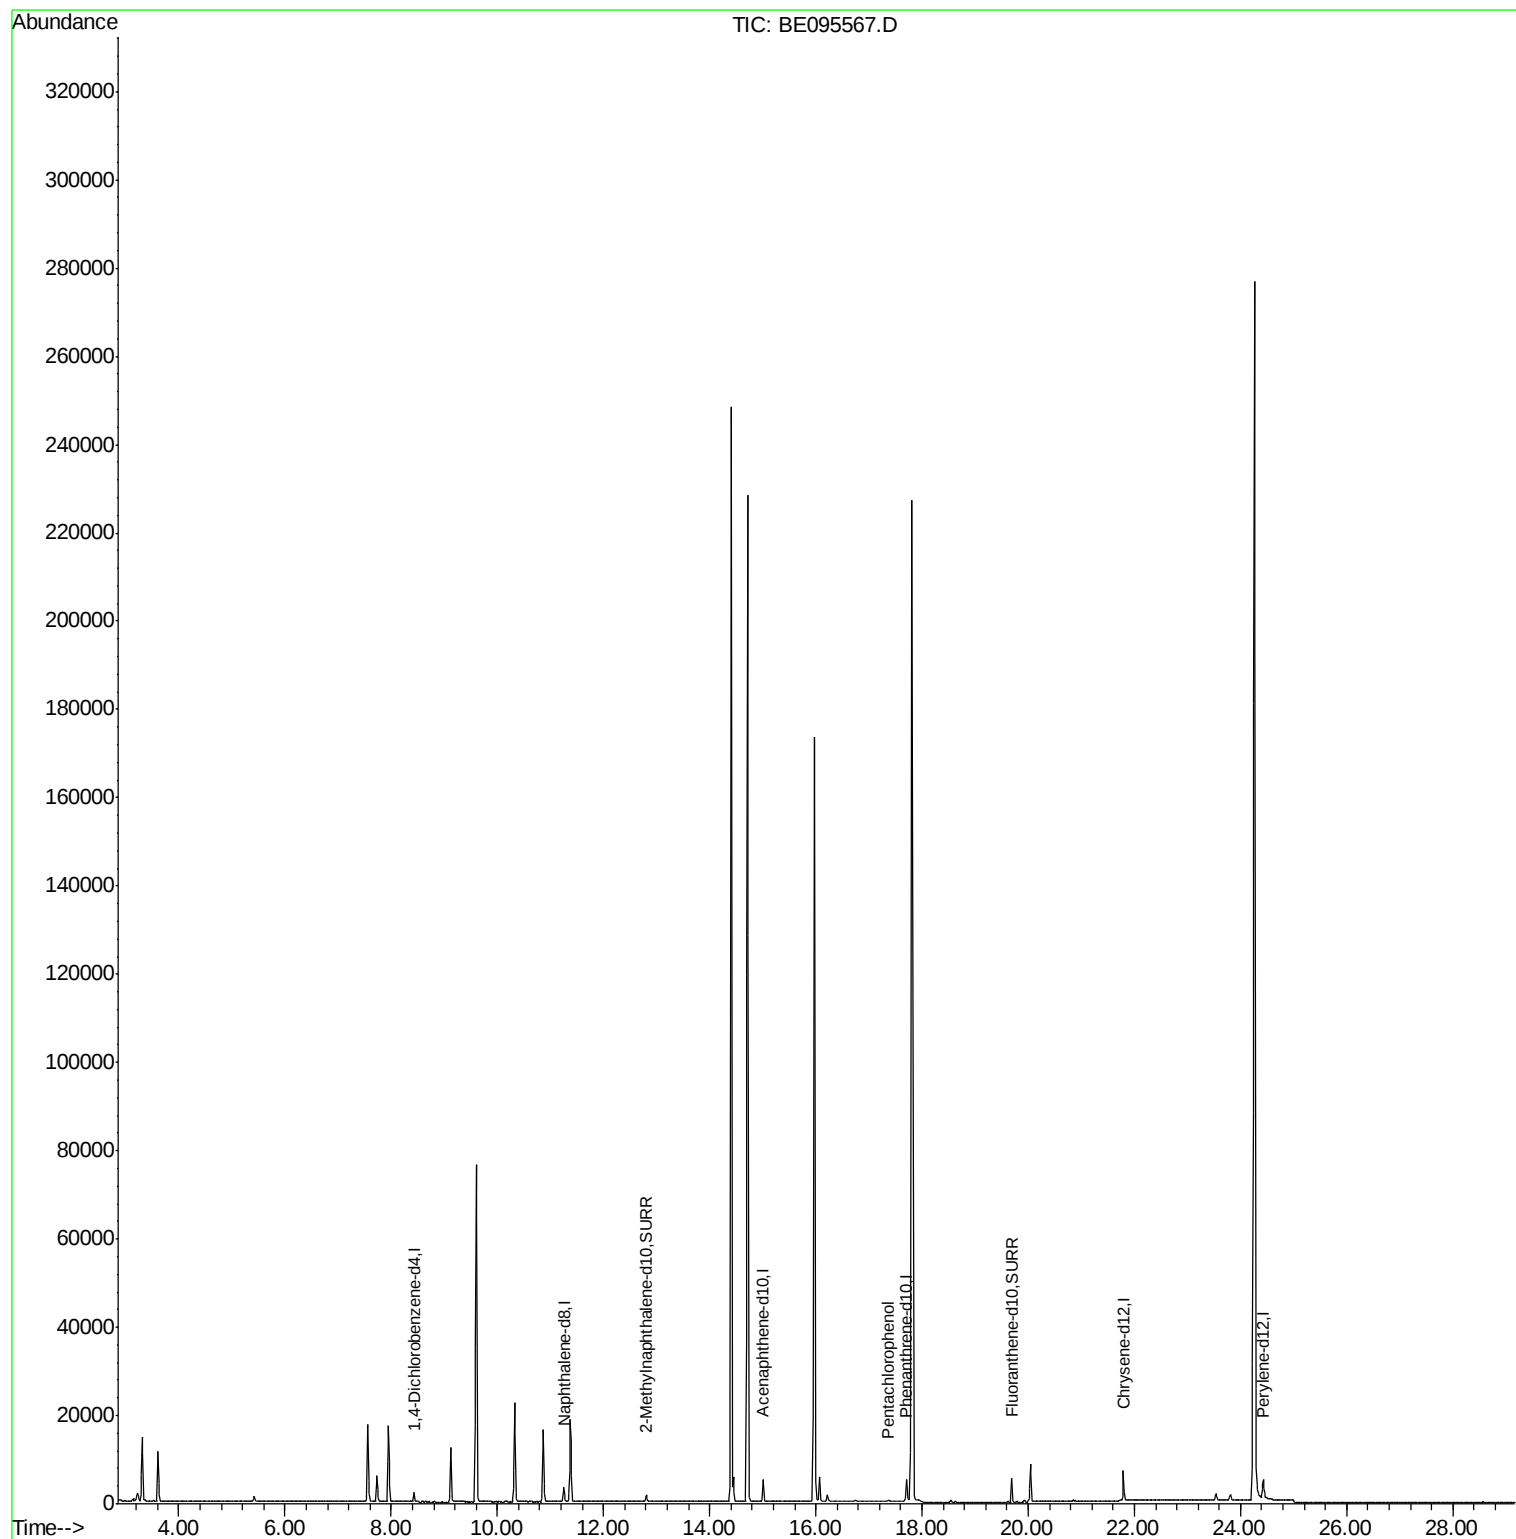

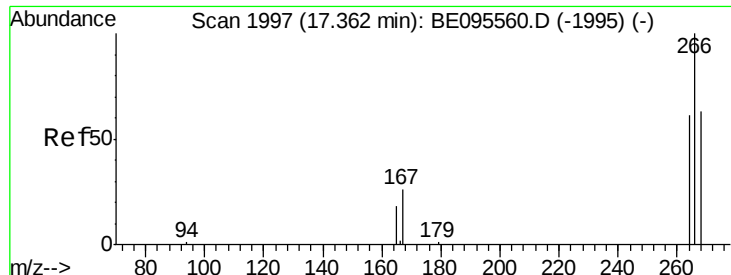

#11
 Pentachlorophenol
 Concen: 0.104 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095567.D
 Acq: 8 Feb 2018 13:56

Instrument :
 BNA_E
 ClientSampleId :
 F6D41

Tot Ion:	266	Resp:	133
Ion Ratio	Lower	Upper	
266	100		
264	53.4	47.9	71.9
268	54.9	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/9/2018 4:30:36 PM

