
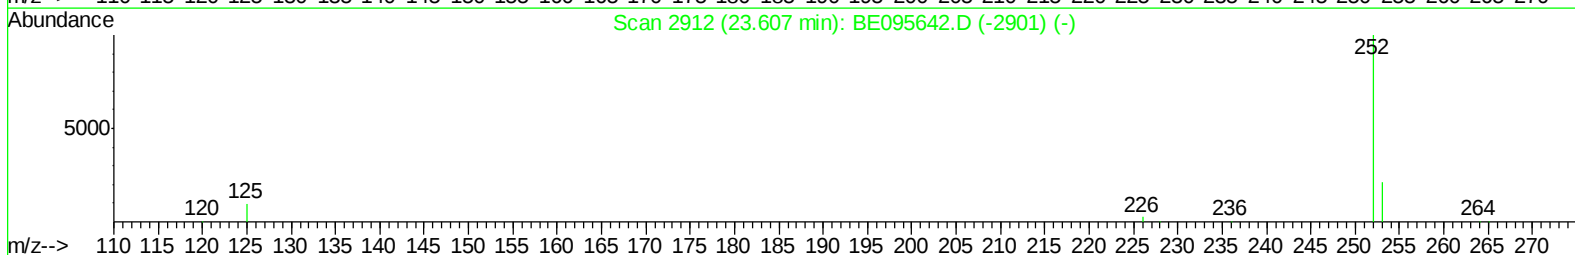
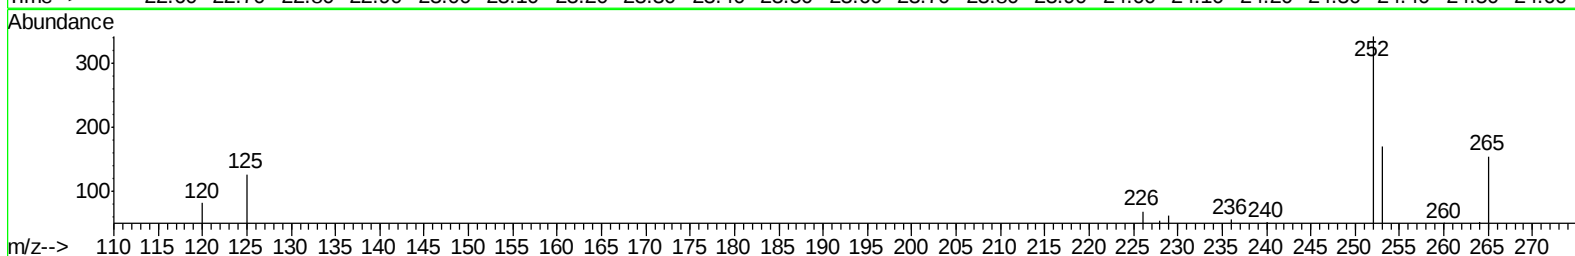


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095649.D
Acq On : 10 Feb 2018 16:40
Operator : SJ/JU
Sample : J1317-05DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Feb 12 01:59:34 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 01:48:13 2018
Response via : Initial Calibration

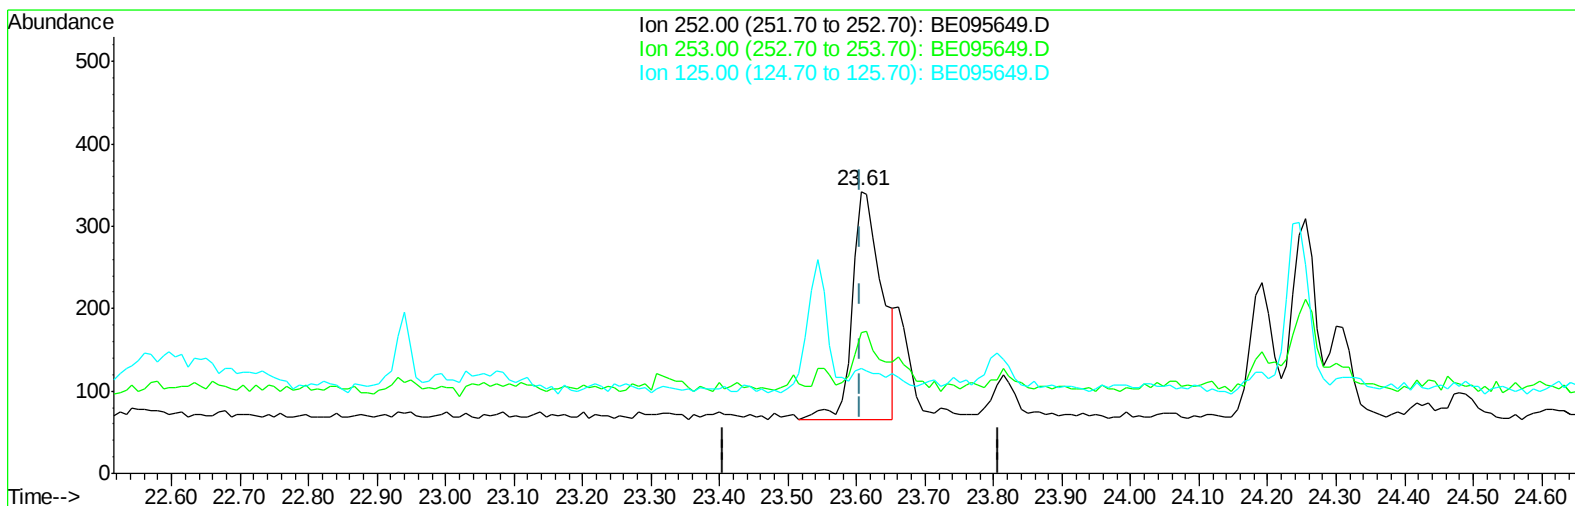

TIC: BE095649.D

(21) Benzo(b)fluoranthene

23.606min (-0.001) 0.03ng/ul m

response 843

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	50.00
125.00	17.50	37.13#
0.00	0.00	0.00