

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095607.D
 Acq On : 9 Feb 2018 14:48
 Operator : SJ/JU
 Sample : PB106255BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 09 23:41:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 23:40:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1506	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4125	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2701	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	6082	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	400041	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2345	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7588	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	1163	0.057	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095607.D
Acq On : 9 Feb 2018 14:48
Operator : SJ/JU
Sample : PB106255BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 09 23:41:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

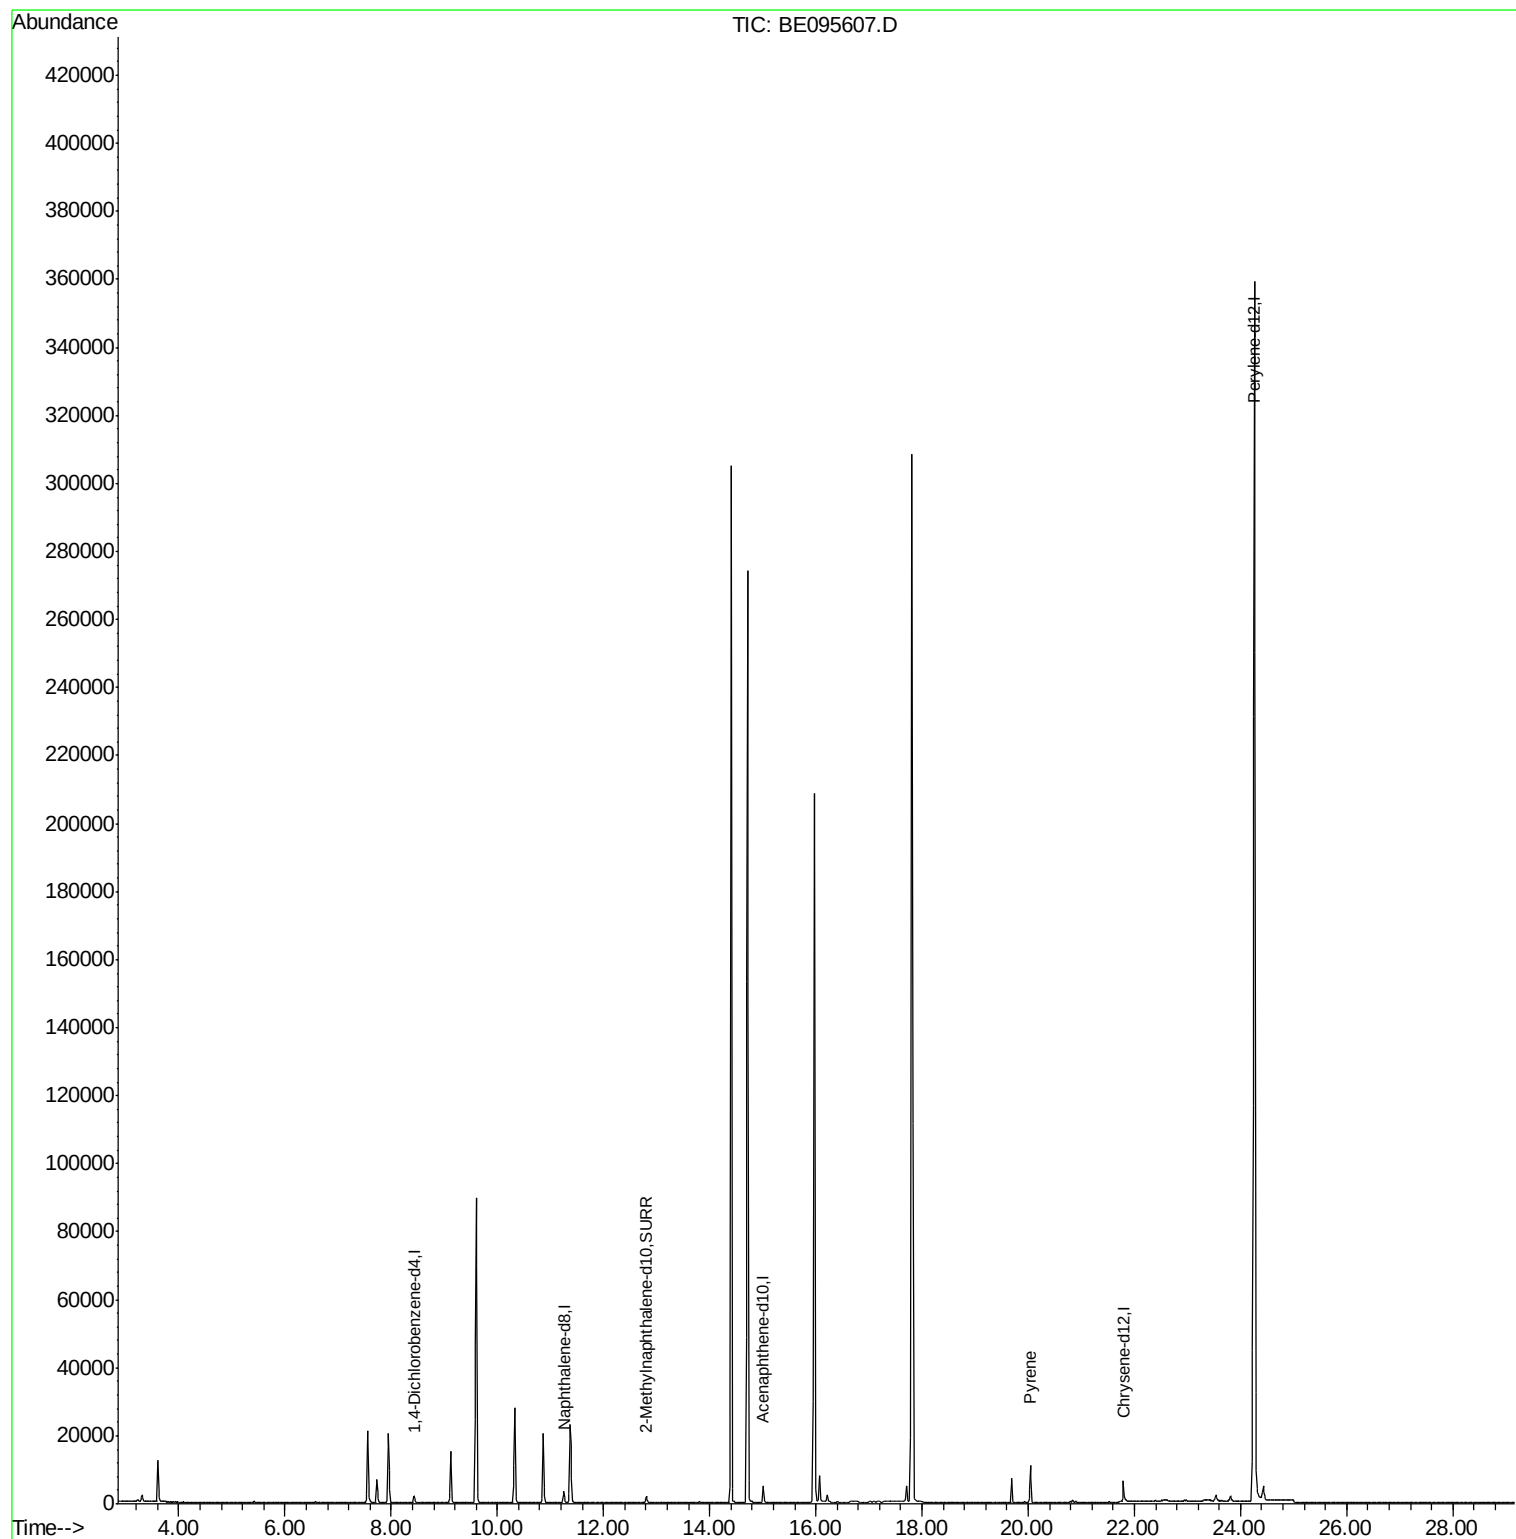

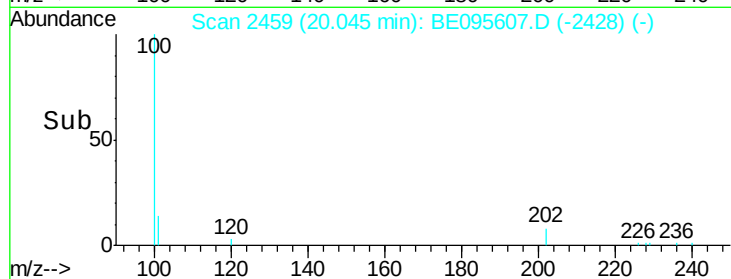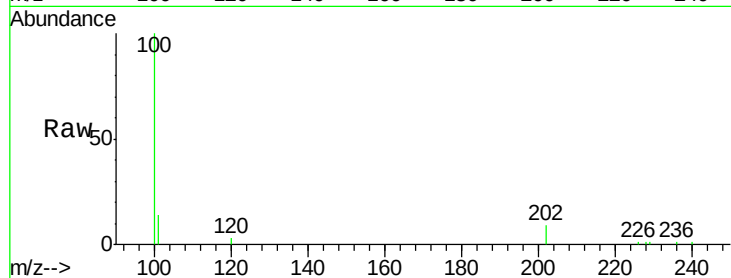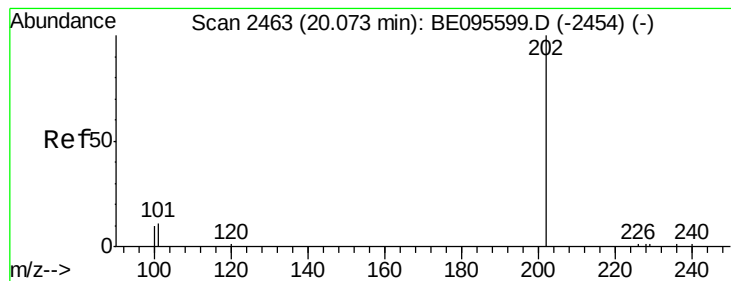

#17

Pvrene

Concen: 0.057 ng/ul

RT: 20.05 min Scan# 2459

Delta R.T. -0.03 min

Lab File: BE095607.D

Acq: 9 Feb 2018 14:48

Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 1163

Ion Ratio Lower Upper

202 100

101 163.6 18.2 27.4#

100 1132.5 15.6 23.4#

