

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095612.D
 Acq On : 9 Feb 2018 17:47
 Operator : SJ/JU
 Sample : J1339-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 10 00:57:18 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1569	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4498	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2981	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6742	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6205	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	350934	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2630	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6949	0.27	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	69517	53.235	ng/ul	98
12) Phenanthrene	17.75	178	735	0.032	ng/ul#	40
17) Pyrene	20.05	202	1271	0.061	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095612.D
Acq On : 9 Feb 2018 17:47
Operator : SJ/JU
Sample : J1339-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 10 00:57:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration




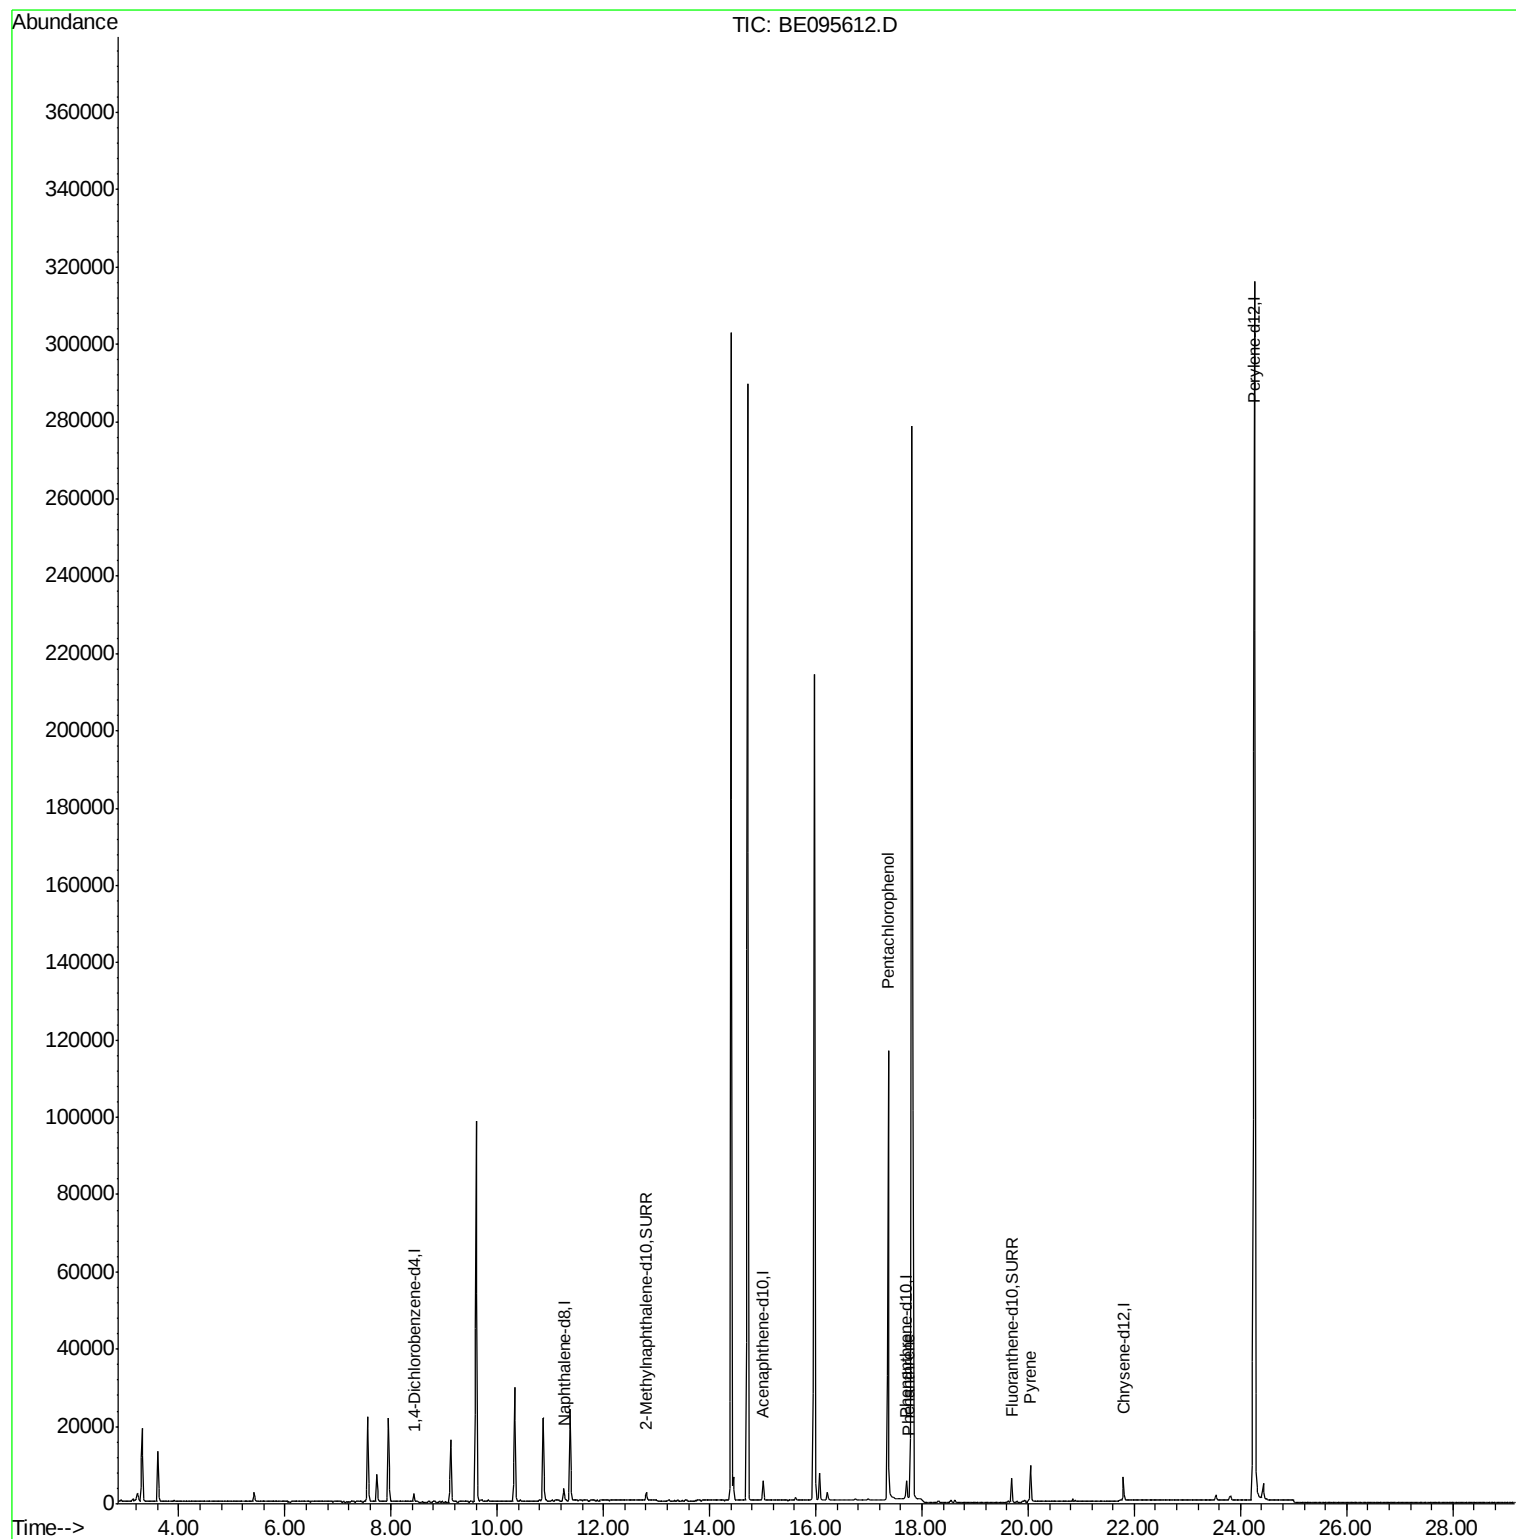


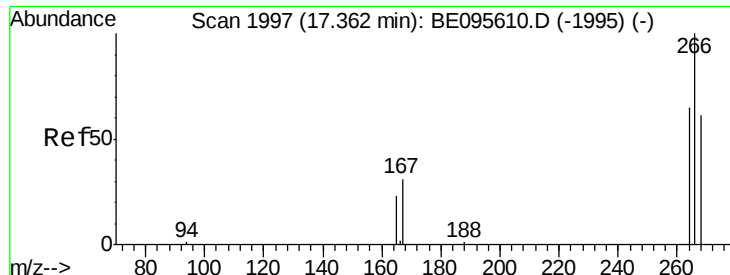

#11
 Pentachlorophenol
 Concen: 53.235 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095612.D
 Acq: 9 Feb 2018 17:47




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 69517
 Ion Ratio Lower Upper
 266 100
 264 62.7 47.9 71.9
 268 63.2 49.8 74.8

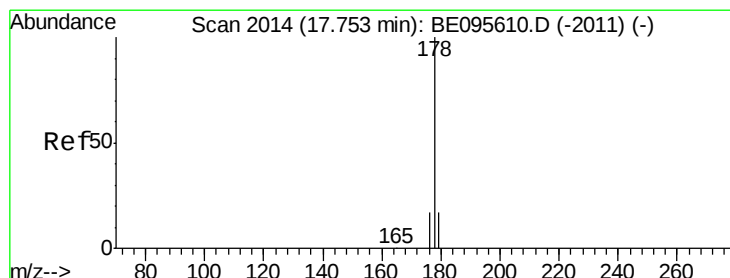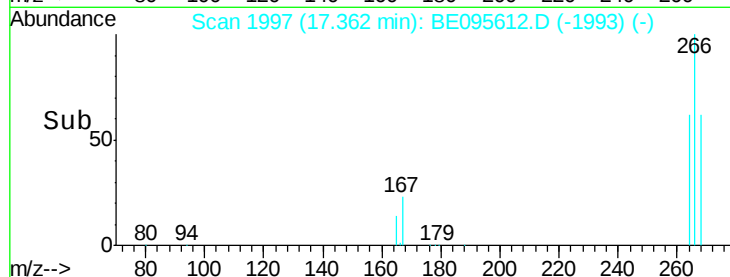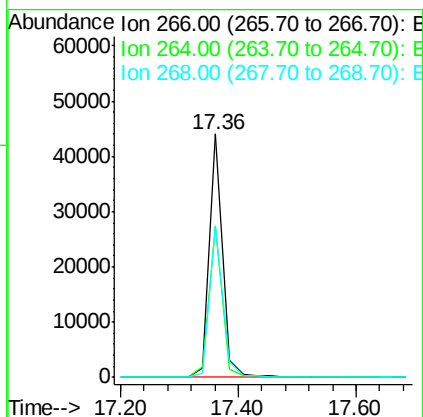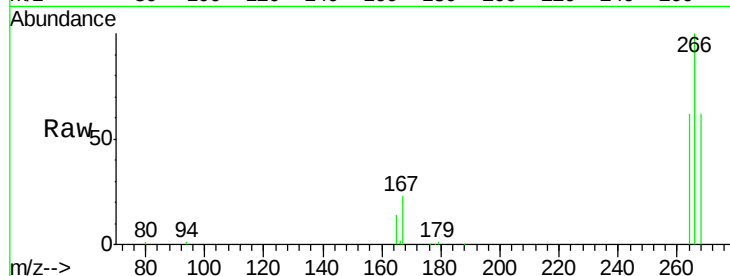

#12
 Phenanthrene
 Concen: 0.032 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095612.D
 Acq: 9 Feb 2018 17:47

Tgt Ion:178 Resp: 735
 Ion Ratio Lower Upper
 178 100
 179 57.5 18.4 27.6#
 176 36.5 13.6 20.4#

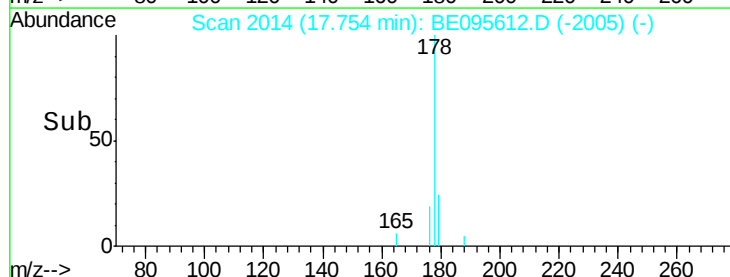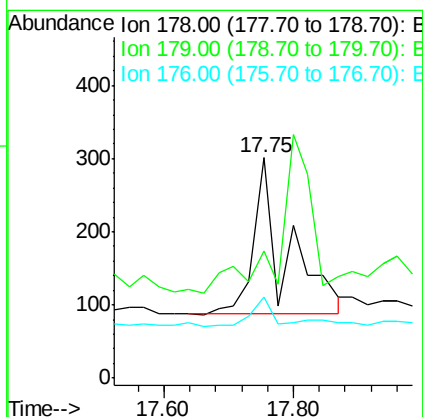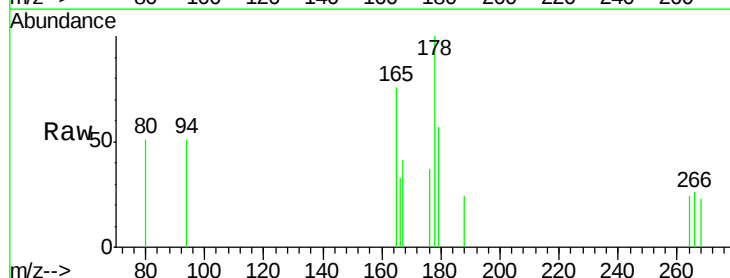

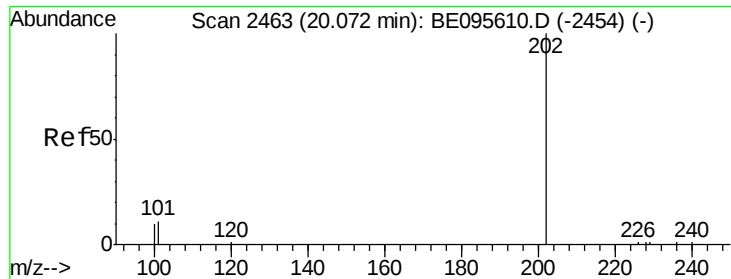

#17
 Pvrene
 Concen: 0.061 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095612.D
 Acq: 9 Feb 2018 17:47

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:202 Resp: 1271
 Ion Ratio Lower Upper
 202 100
 101 152.2 18.2 27.4#
 100 896.9 15.6 23.4#

