

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095614.D
 Acq On : 9 Feb 2018 18:59
 Operator : SJ/JU
 Sample : J1339-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 10 00:57:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1727	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4983	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3295	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7433	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7005	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	355972	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2644	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7132	0.25	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	106	0.074	ng/ul	95
12) Phenanthrene	17.75	178	520	0.021	ng/ul#	51
17) Pyrene	20.07	202	2277	0.097	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095614.D
Acq On : 9 Feb 2018 18:59
Operator : SJ/JU
Sample : J1339-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 10 00:57:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration




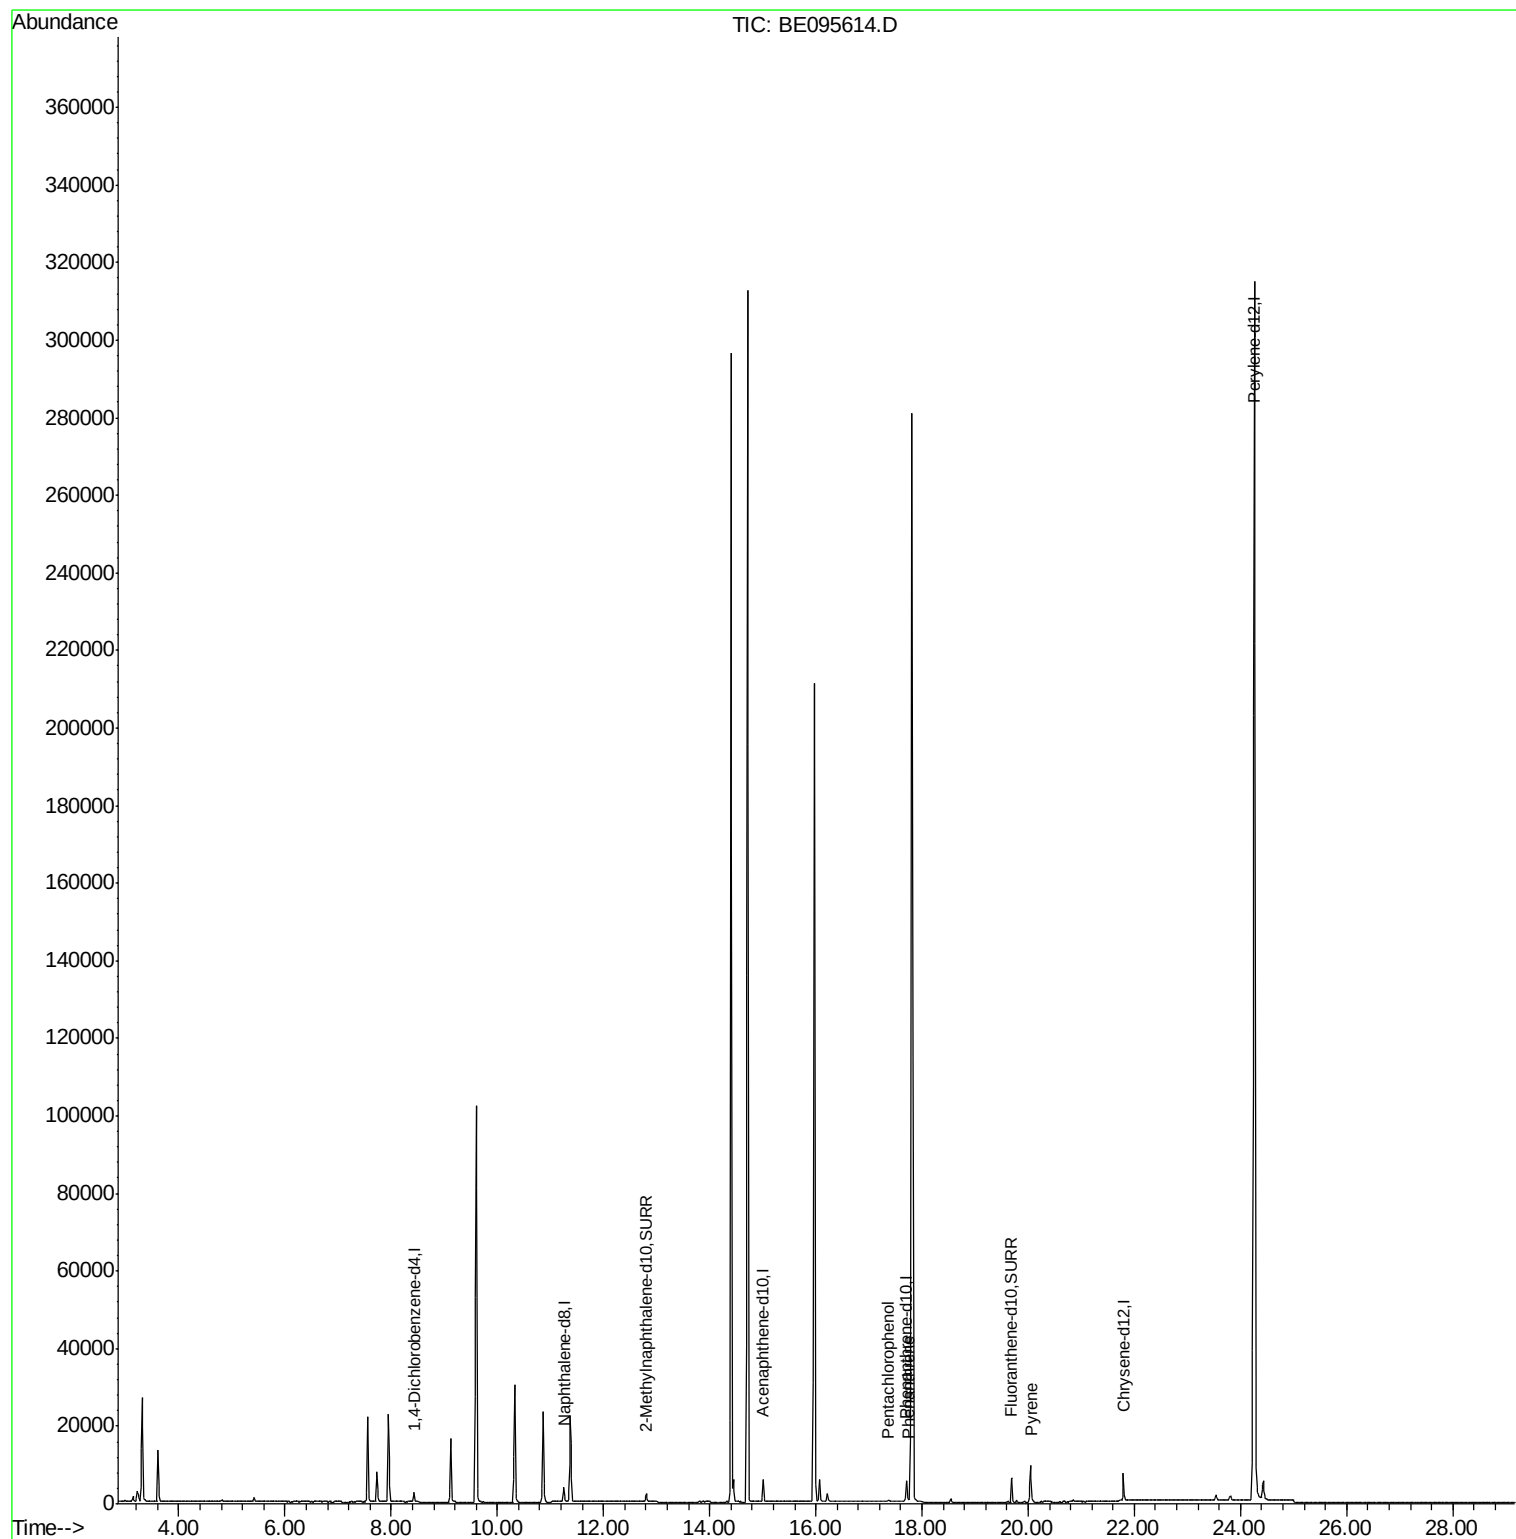


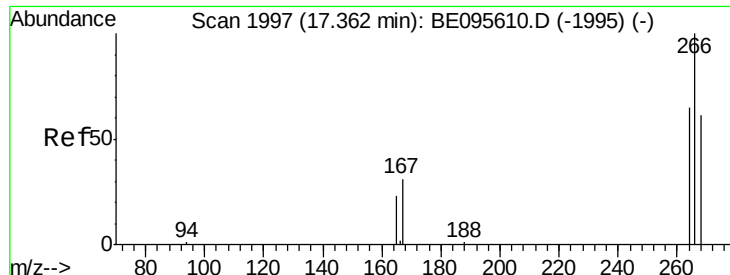

#11
 Pentachlorophenol
 Concen: 0.074 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095614.D
 Acq: 9 Feb 2018 18:59




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:266 Resp: 106
 Ion Ratio Lower Upper
 266 100
 264 67.9 47.9 71.9
 268 62.3 49.8 74.8

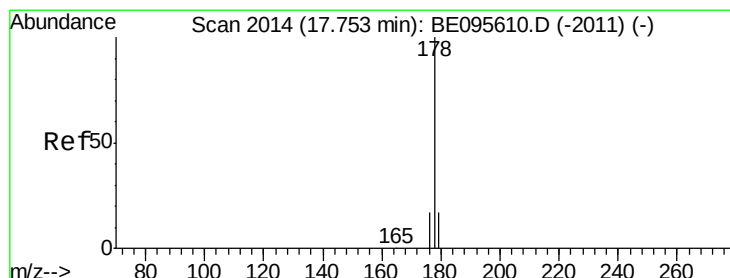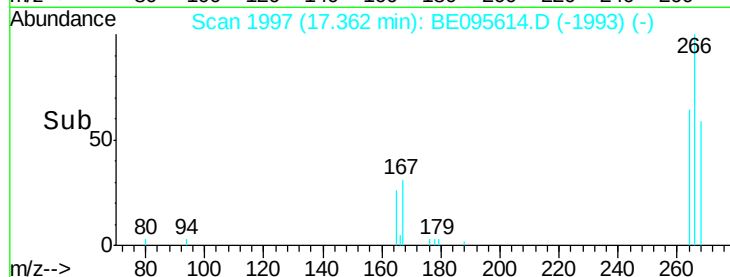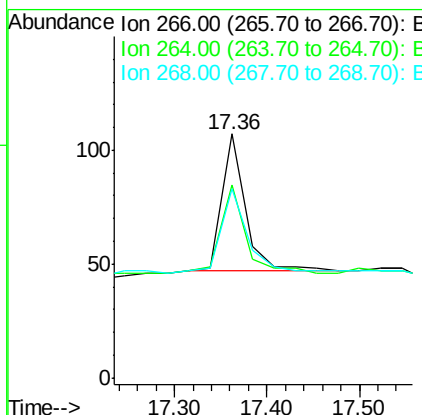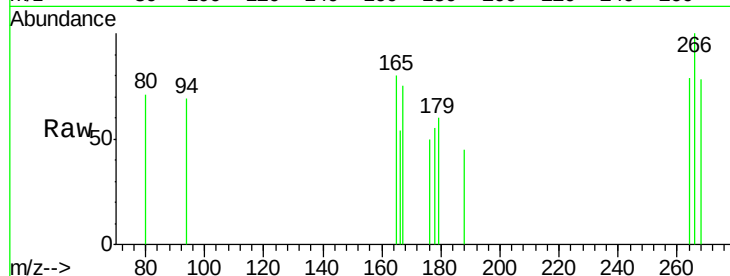

#12
 Phenanthrene
 Concen: 0.021 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095614.D
 Acq: 9 Feb 2018 18:59

Tgt Ion:178 Resp: 520
 Ion Ratio Lower Upper
 178 100
 179 46.6 18.4 27.6#
 176 38.9 13.6 20.4#

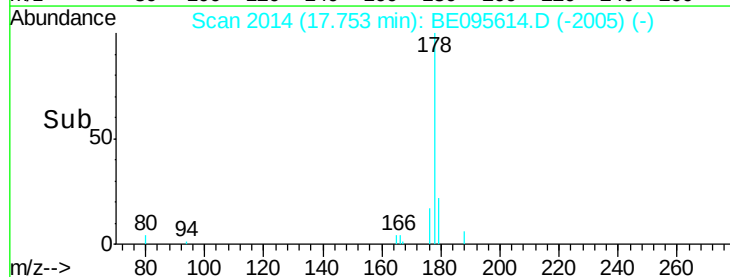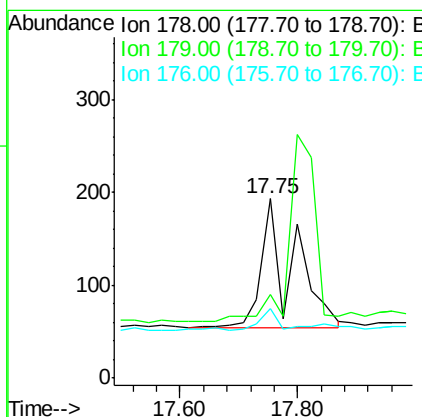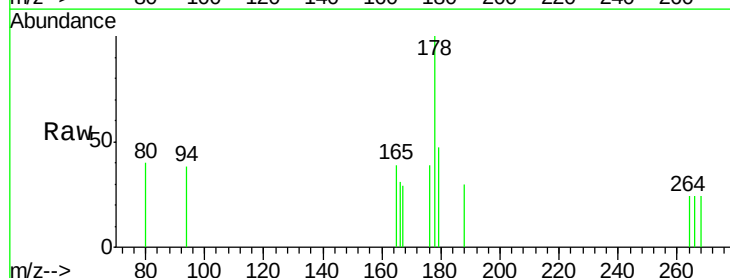

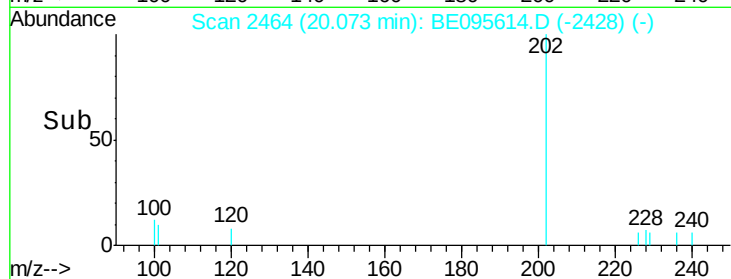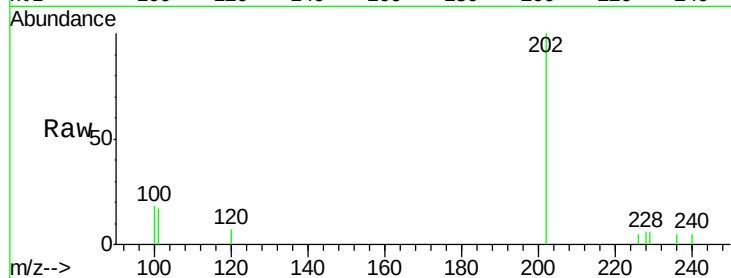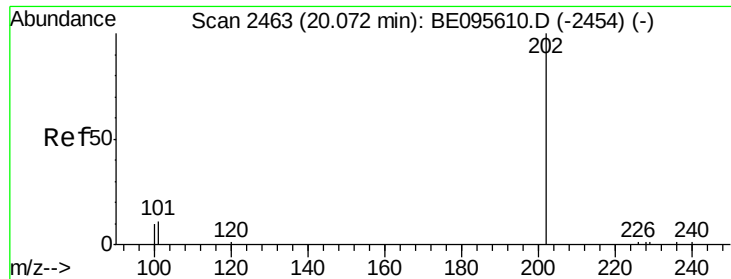

#17

Pvrene

Concen: 0.097 ng/ul

RT: 20.07 min Scan# 2464

Delta R.T. 0.00 min

Lab File: BE095614.D

Acq: 9 Feb 2018 18:59

Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 2277

Ion Ratio Lower Upper

202 100

101 17.3 18.2 27.4#

100 18.4 15.6 23.4

