

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095619.D
 Acq On : 9 Feb 2018 21:58
 Operator : SJ/JU
 Sample : J1339-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 10 00:58:12 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1722	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4932	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3304	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7676	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7068	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	381594	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.80	152	2755	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7688	0.26	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	2287	1.538	ng/ul	97
12) Phenanthrene	17.75	178	635	0.025	ng/ul#	60
17) Pyrene	20.05	202	1245	0.052	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095619.D
Acq On : 9 Feb 2018 21:58
Operator : SJ/JU
Sample : J1339-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 10 00:58:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

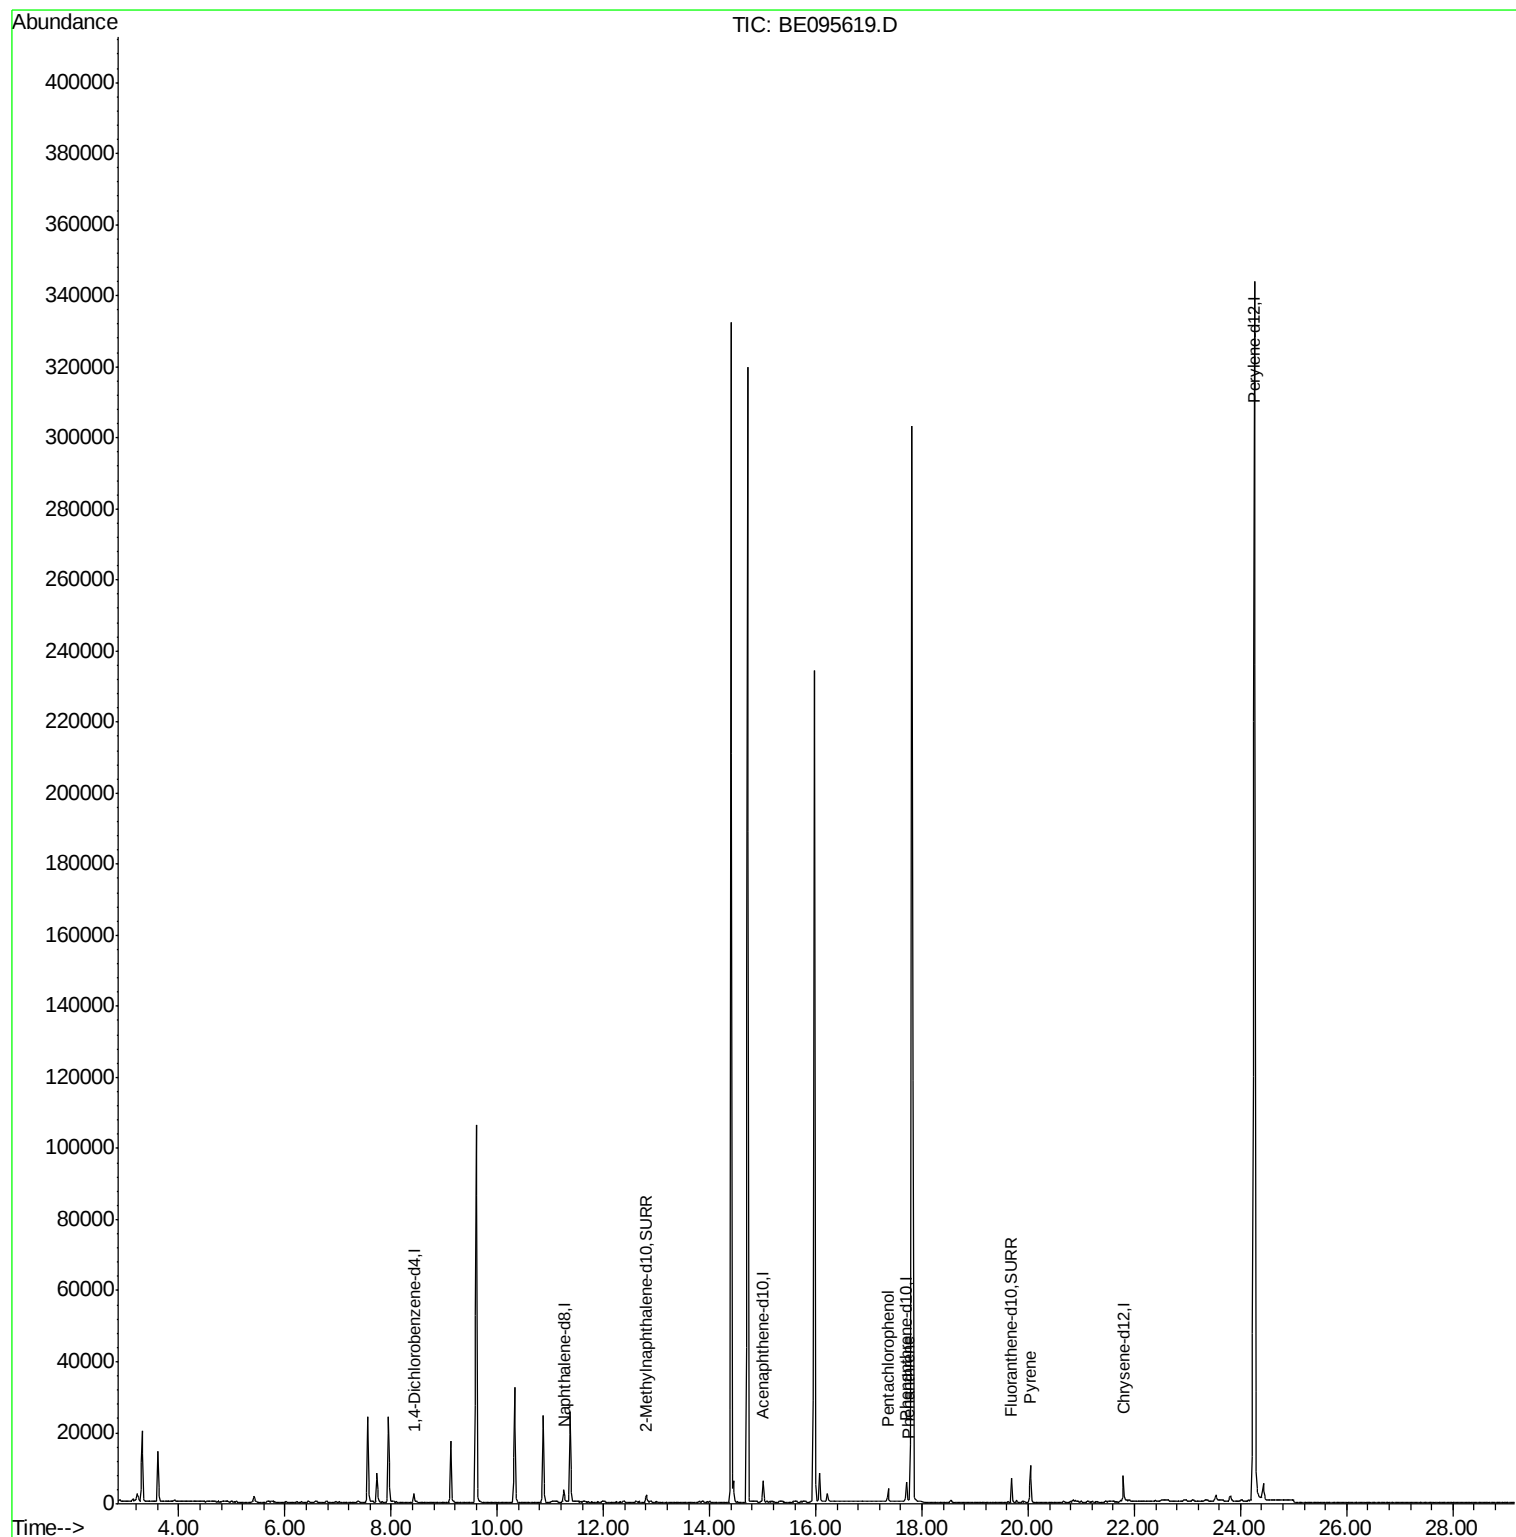


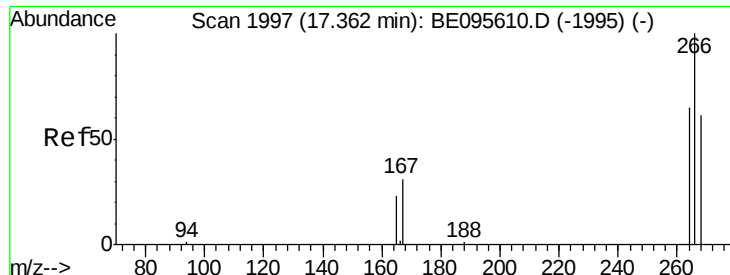




#11
 Pentachlorophenol
 Concen: 1.538 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095619.D
 Acq: 9 Feb 2018 21:58

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 2287
 Ion Ratio Lower Upper
 266 100
 264 62.5 47.9 71.9
 268 63.8 49.8 74.8

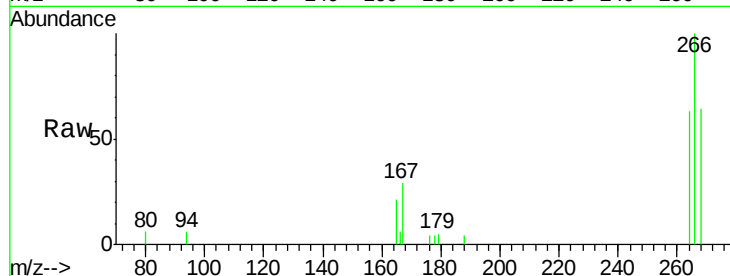


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

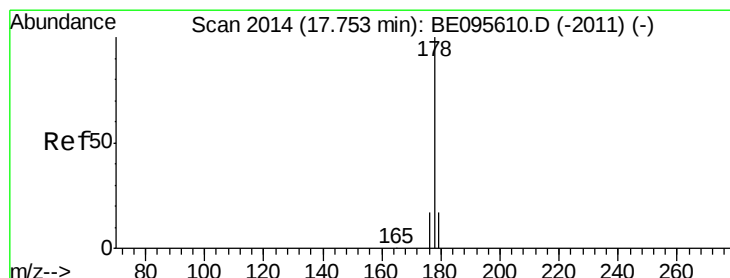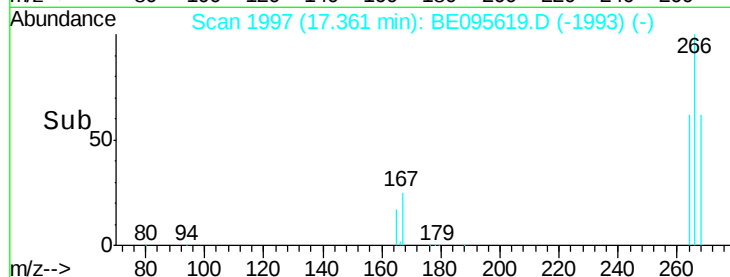
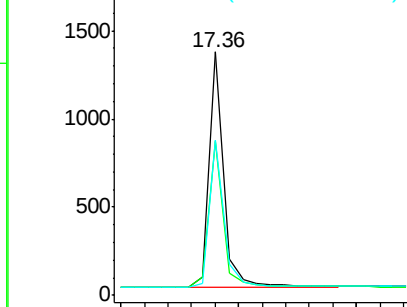





#12
 Phenanthrene
 Concen: 0.025 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095619.D
 Acq: 9 Feb 2018 21:58

Tgt Ion:178 Resp: 635
 Ion Ratio Lower Upper
 178 100
 179 41.2 18.4 27.6#
 176 35.4 13.6 20.4#

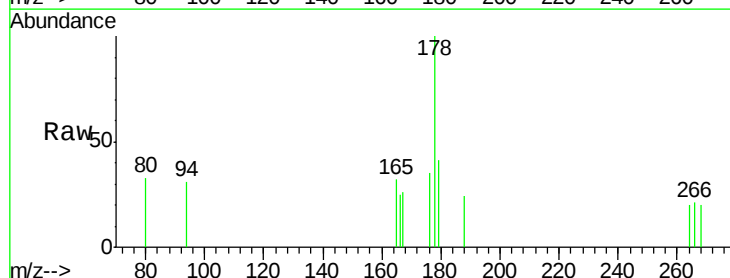

Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

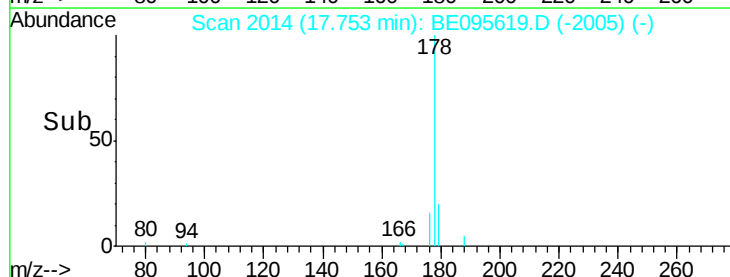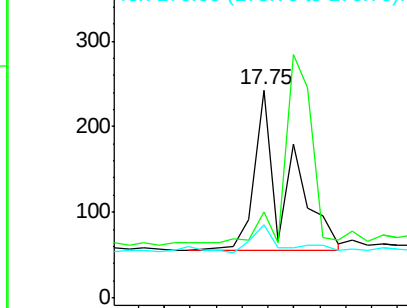

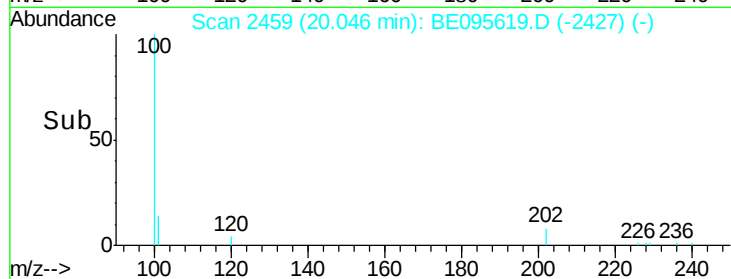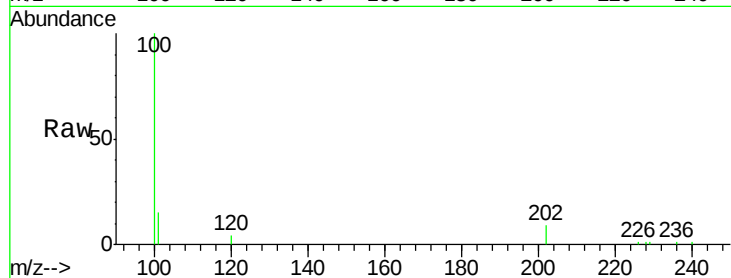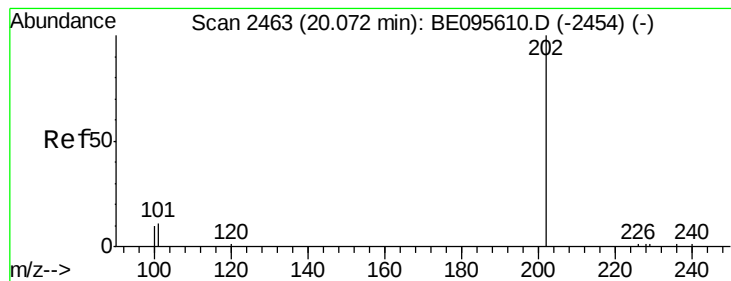

#17

Pvrene

Concen: 0.052 ng/ul

RT: 20.05 min Scan# 2459

Delta R.T. -0.03 min

Lab File: BE095619.D

Acq: 9 Feb 2018 21:58

Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 1245

Ion Ratio Lower Upper

202 100

101 174.9 18.2 27.4#

100 1142.3 15.6 23.4#

