

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095623.D
 Acq On : 10 Feb 2018 00:21
 Operator : SJ/JU
 Sample : J1339-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 10 02:01:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1697	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5043	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3337	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7560	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6998	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	468366	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3328	0.41	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9065	0.31	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	265	0.181	ng/ul	96
12) Phenanthrene	17.75	178	756	0.030	ng/ul#	70
17) Pyrene	20.07	202	2942	0.125	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095623.D
Acq On : 10 Feb 2018 00:21
Operator : SJ/JU
Sample : J1339-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 10 02:01:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration




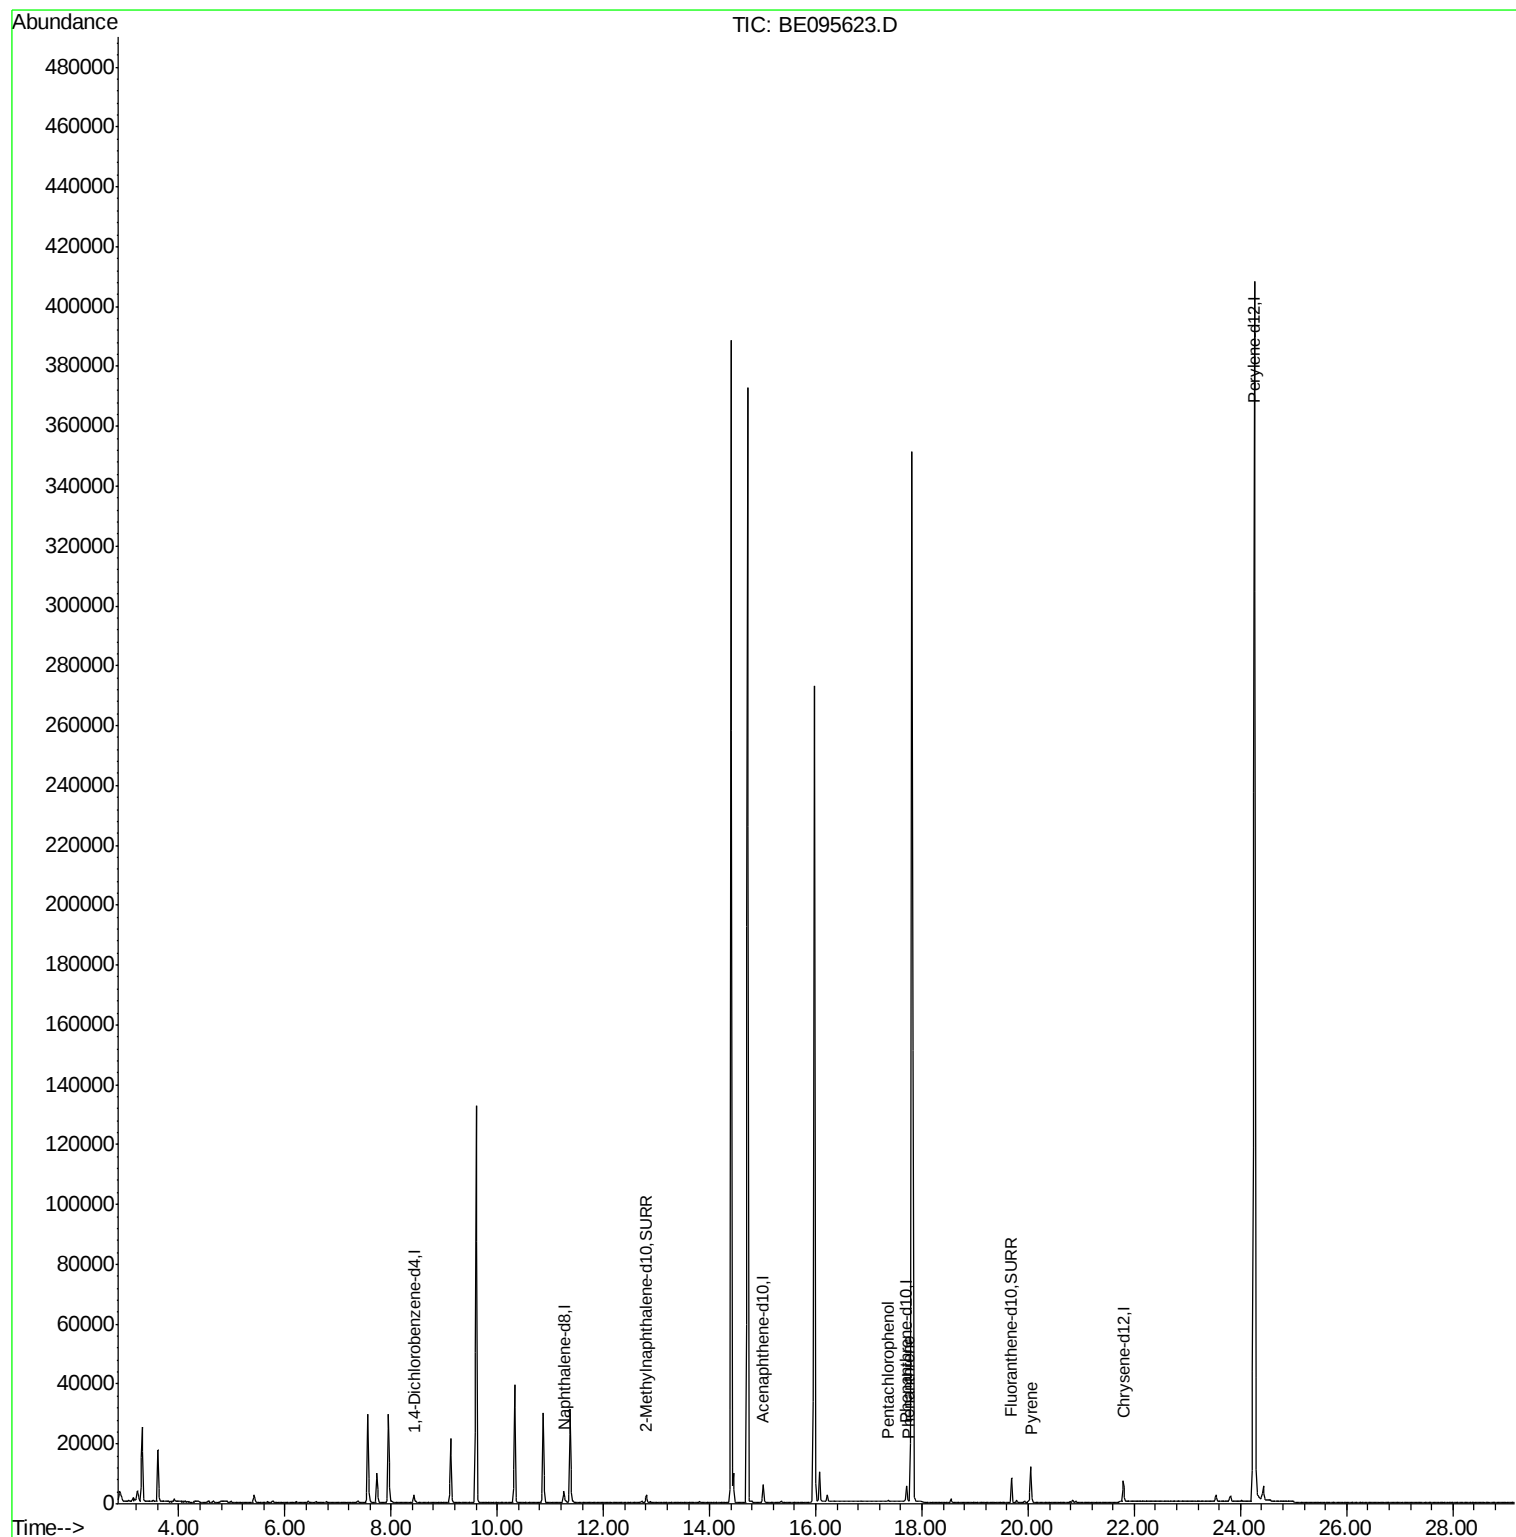


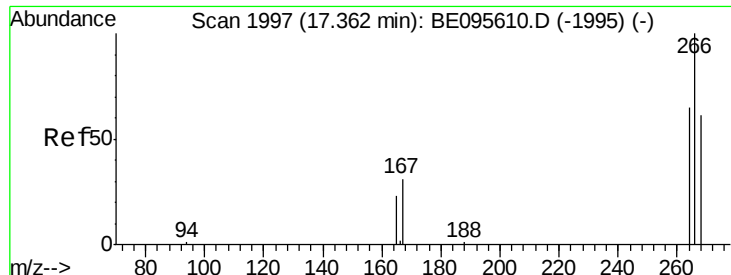

#11
 Pentachlorophenol
 Concen: 0.181 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095623.D
 Acq: 10 Feb 2018 00:21




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 265
 Ion Ratio Lower Upper
 266 100
 264 62.3 47.9 71.9
 268 65.3 49.8 74.8

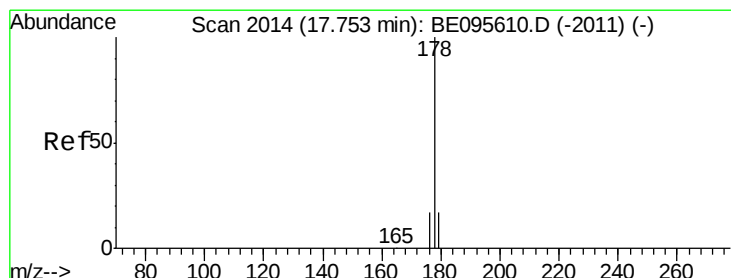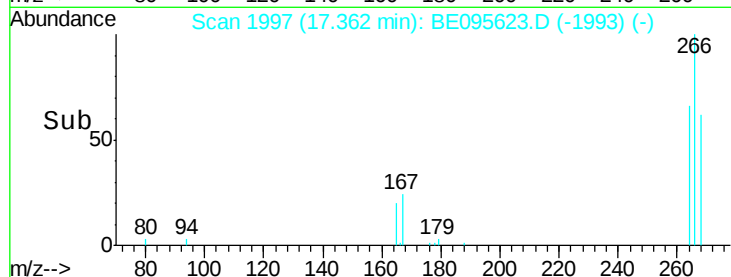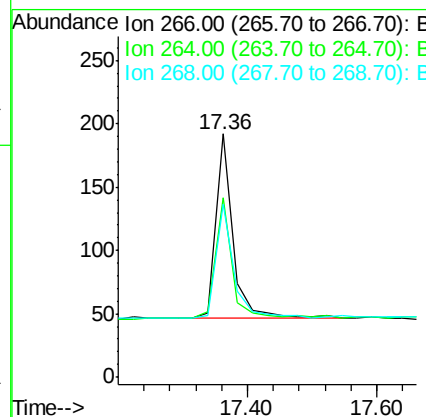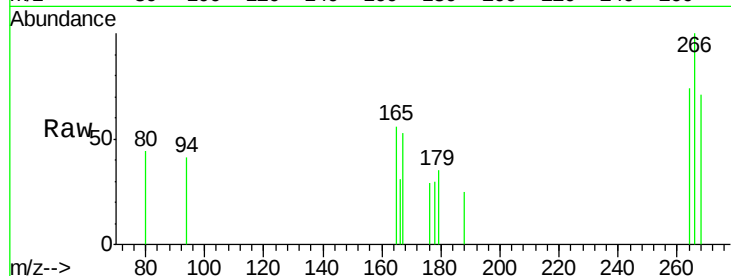

#12
 Phenanthrene
 Concen: 0.030 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095623.D
 Acq: 10 Feb 2018 00:21

Tgt Ion:178 Resp: 756
 Ion Ratio Lower Upper
 178 100
 179 36.5 18.4 27.6#
 176 30.9 13.6 20.4#

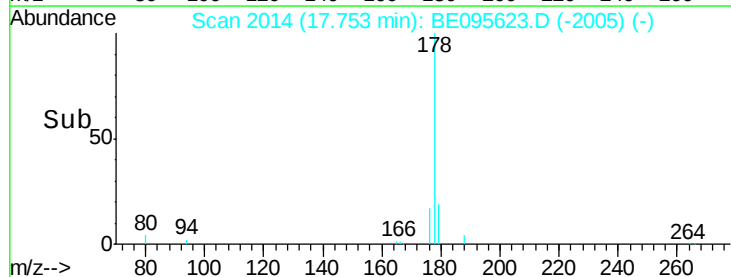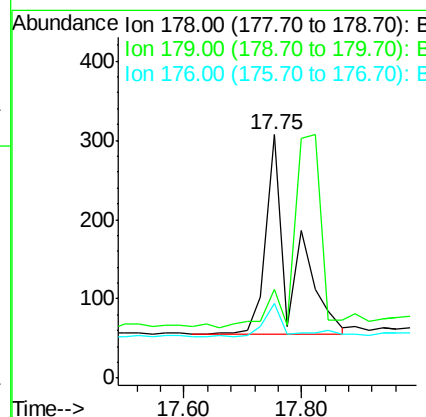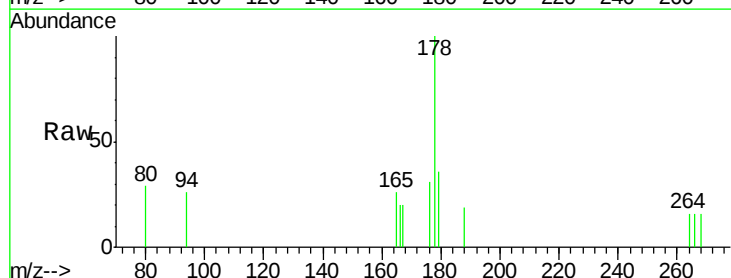

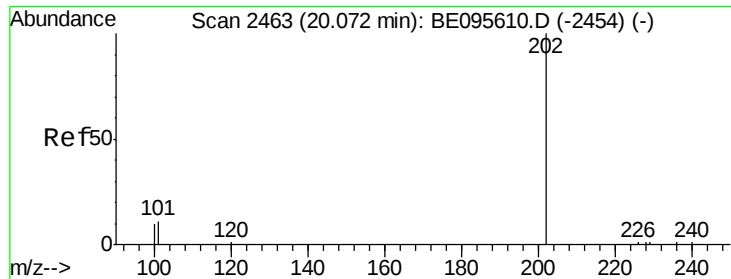

#17
 Pvrene
 Concen: 0.125 ng/ul
 RT: 20.07 min Scan# 2463
 Delta R.T. -0.00 min
 Lab File: BE095623.D
 Acq: 10 Feb 2018 00:21

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	18.8	18.2	27.4
100	22.9	15.6	23.4

