

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095624.D
 Acq On : 10 Feb 2018 00:57
 Operator : SJ/JU
 Sample : J1339-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 10 02:01:12 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1878	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5510	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3558	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8492	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7648	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	370669	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2696	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7288	0.22	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	124003	75.391	ng/ul	97
17) Pyrene	20.05	202	1573	0.061	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095624.D
Acq On : 10 Feb 2018 00:57
Operator : SJ/JU
Sample : J1339-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 10 02:01:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration




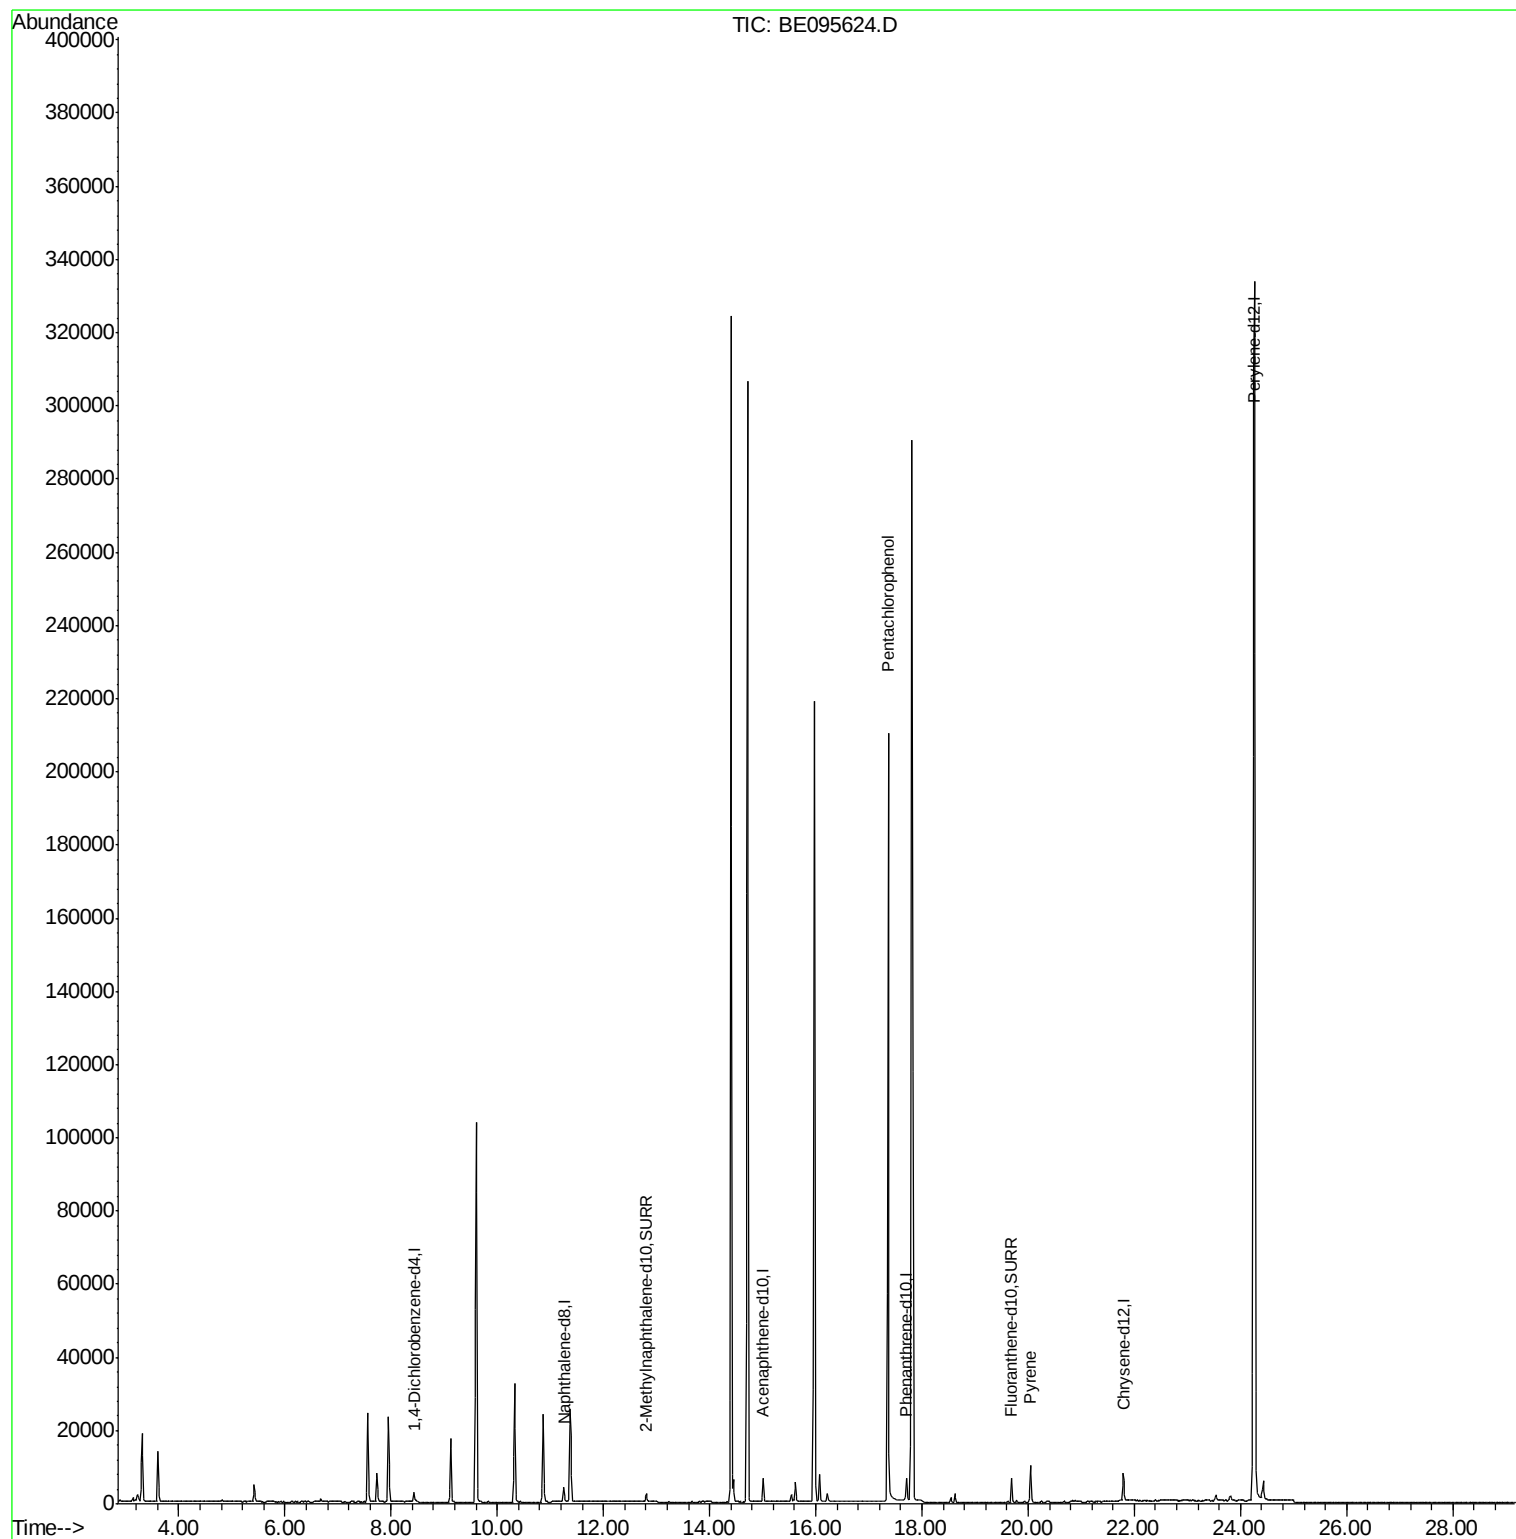


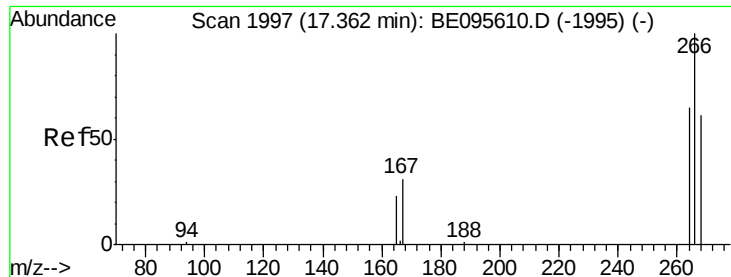

#11
 Pentachlorophenol
 Concen: 75.391 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095624.D
 Acq: 10 Feb 2018 00:57

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 124003
 Ion Ratio Lower Upper
 266 100
 264 63.6 47.9 71.9
 268 61.8 49.8 74.8

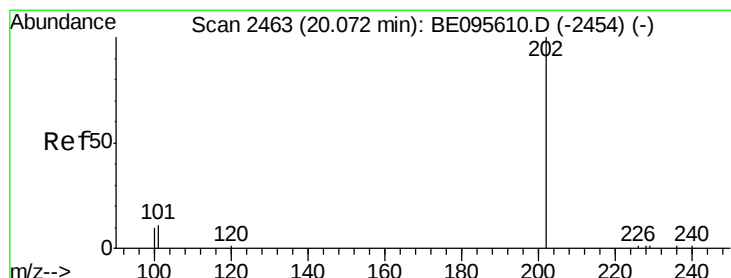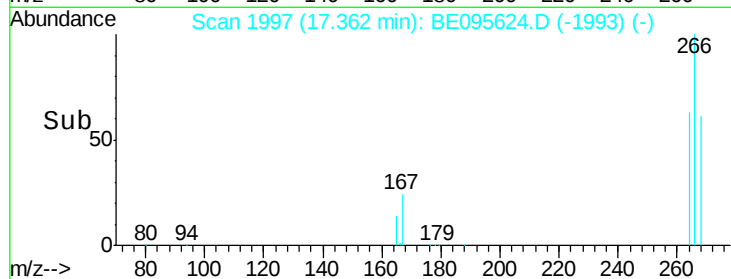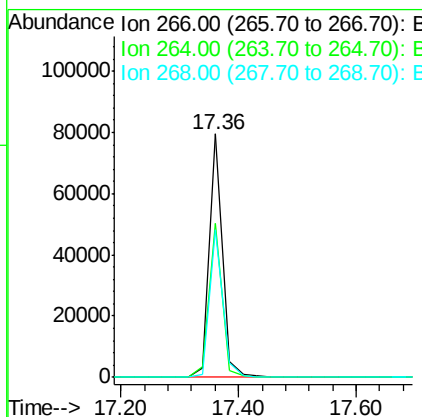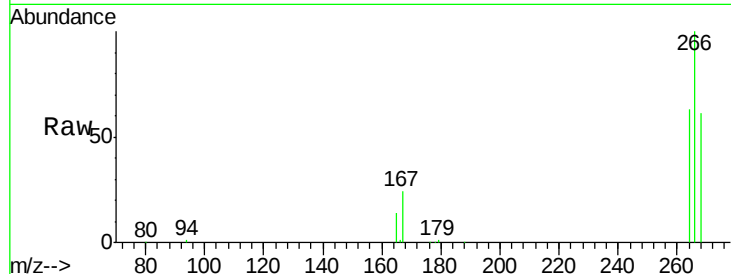

#17
 Pyrene
 Concen: 0.061 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095624.D
 Acq: 10 Feb 2018 00:57

Tgt Ion:202 Resp: 1573
 Ion Ratio Lower Upper
 202 100
 101 149.0 18.2 27.4#
 100 887.5 15.6 23.4#

