

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095627.D
 Acq On : 10 Feb 2018 2:59
 Operator : SJ/JU
 Sample : J1339-07DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 10 03:39:27 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1734	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4969	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3116	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7537	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7336	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7361	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	438	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	1245	0.04	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	16.03	166	492	0.041	ng/ul#	91
11) Pentachlorophenol	17.36	266	10598	7.260	ng/ul	98
12) Phenanthrene	17.85	178	1435	0.057	ng/ul	95
13) Anthracene	17.85	178	1414	0.061	ng/ul	96
15) Fluoranthene	19.72	202	12872	0.392	ng/ul	83
17) Pyrene	20.07	202	11347	0.461	ng/ul#	79
18) Benzo(a)anthracene	21.78	228	2525	0.110	ng/ul#	87
19) Chrysene	21.78	228	2525	0.106	ng/ul	98
21) Benzo(b)fluoranthene	23.62	252	2604	0.100	ng/ul	96
22) Benzo(k)fluoranthene	23.62	252	2604	0.110	ng/ul#	94
23) Benzo(a)pyrene	24.31	252	816	0.035	ng/ul#	86
26) Benzo(g,h,i)perylene	28.11	276	431	0.020	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095627.D
Acq On : 10 Feb 2018 2:59
Operator : SJ/JU
Sample : J1339-07DL 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 10 03:39:27 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration




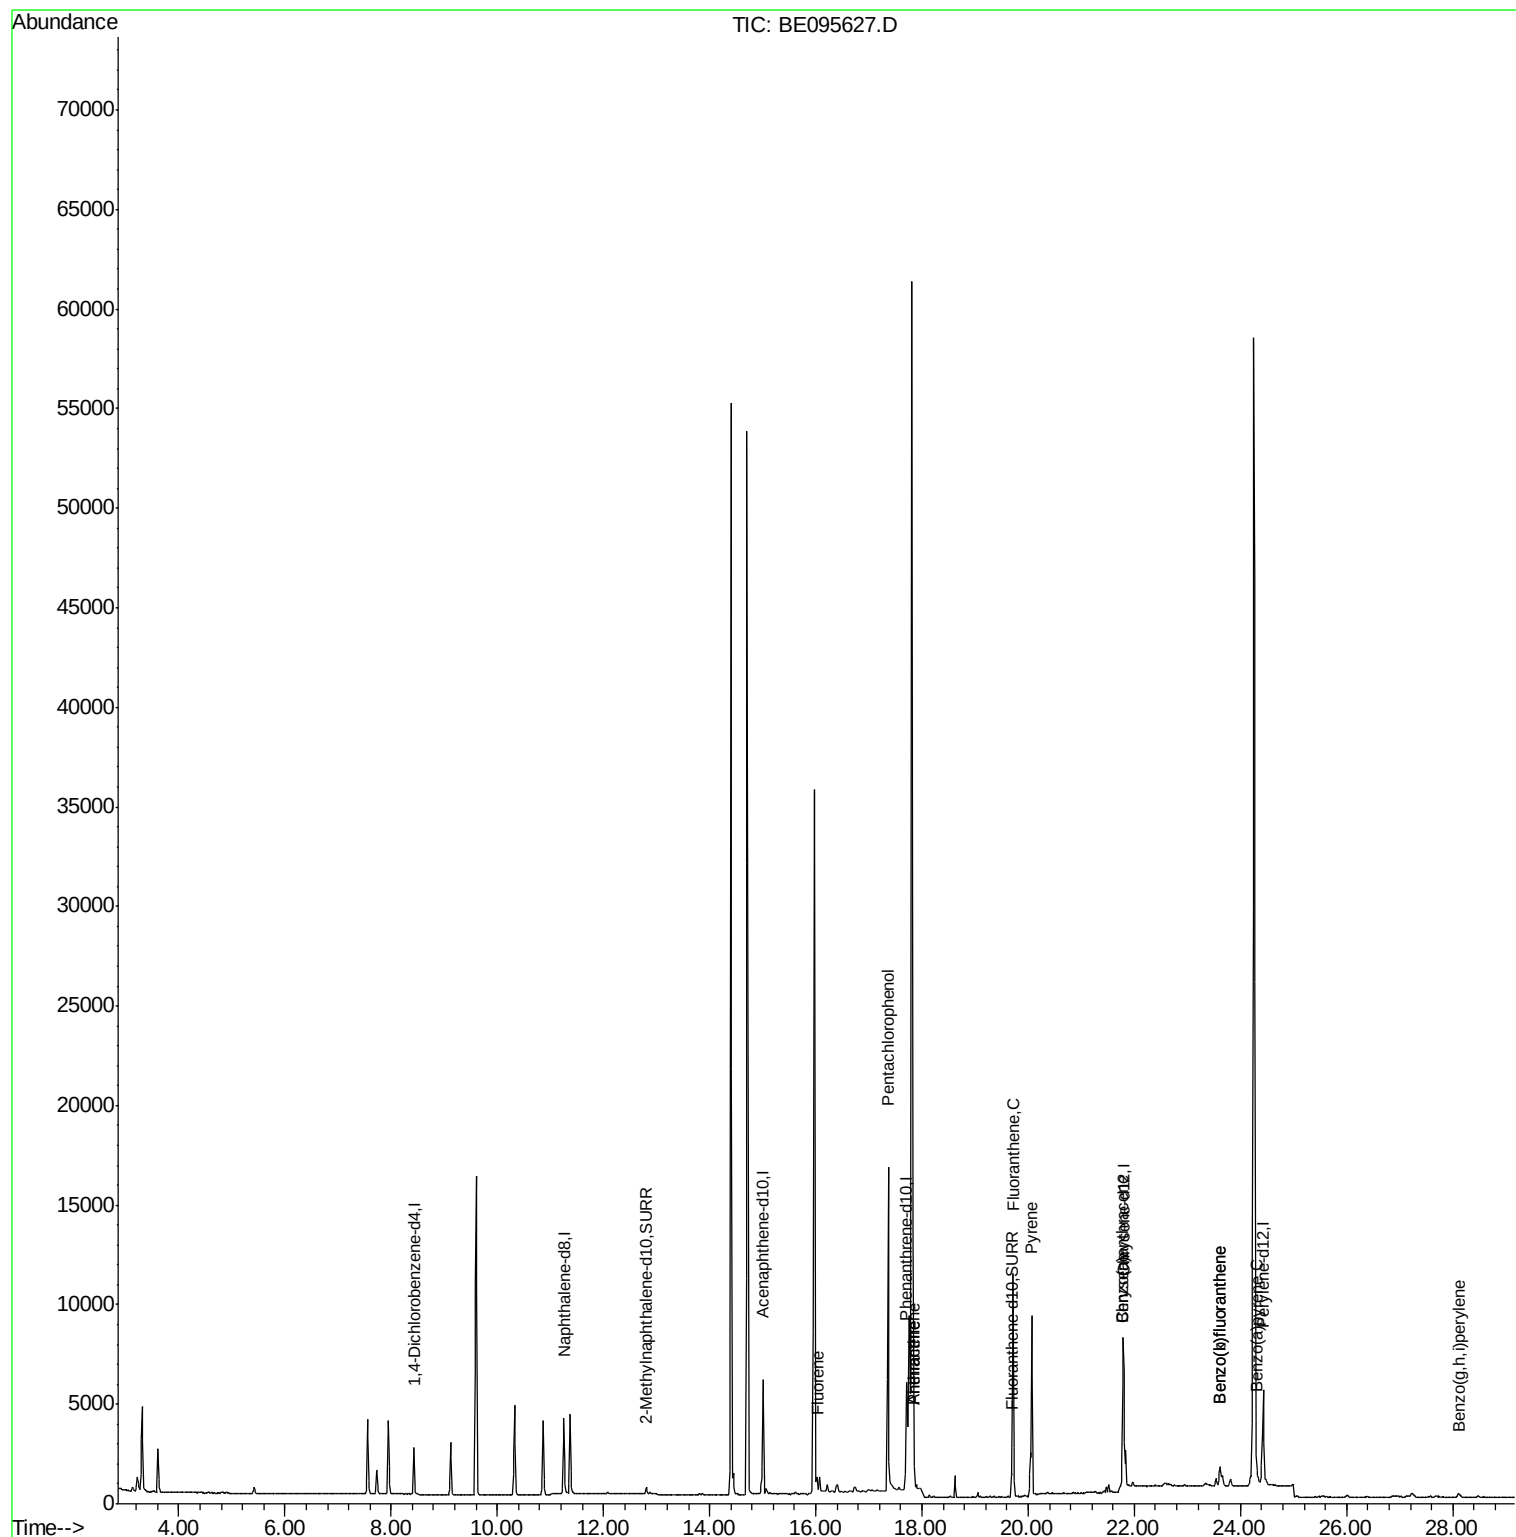


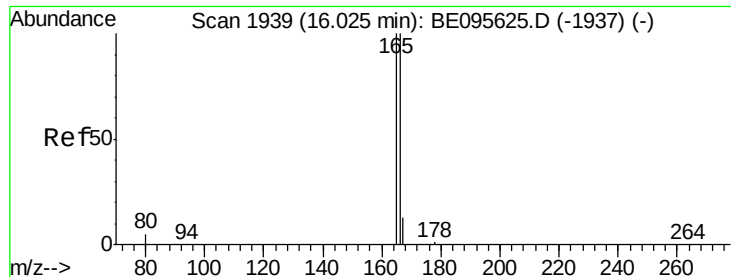

#9
Fluorene
 Concen: 0.041 ng/ul
 RT: 16.03 min Scan# 1939
 Delta R.T. 0.00 min
 Lab File: BE095627.D
 Acq: 10 Feb 2018 2:59




Instrument :
 BNA_E
 ClientSampled :


Tot Ion:166 Resp: 492
 Ion Ratio Lower Upper
 166 100
 165 100.3 73.4 110.2
 167 23.9 14.6 22.0#

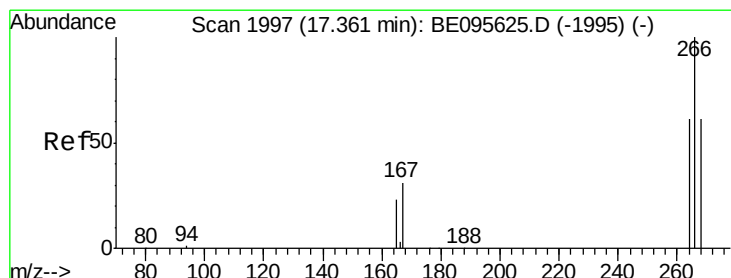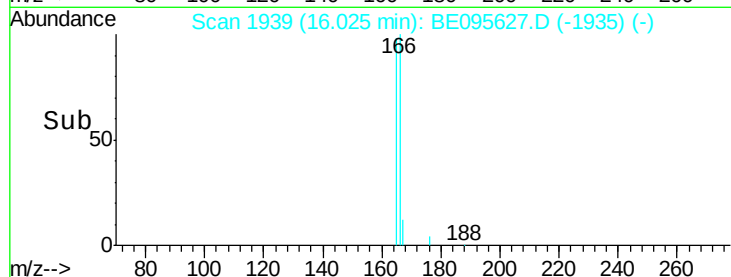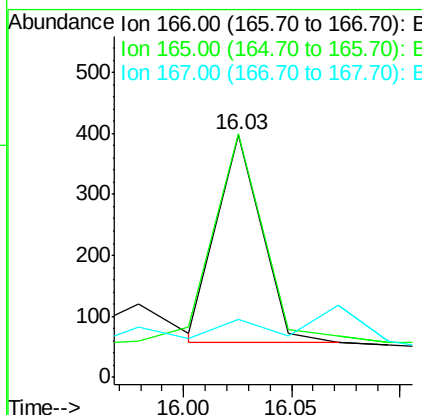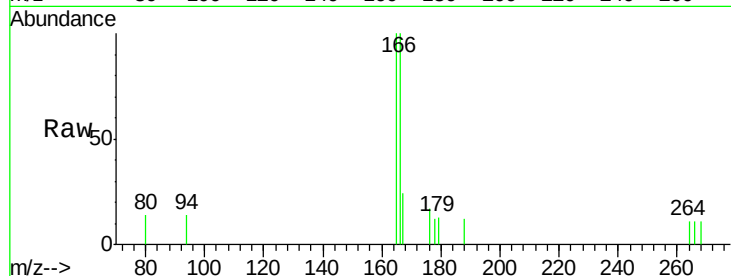

#11
Pentachlorophenol
 Concen: 7.260 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095627.D
 Acq: 10 Feb 2018 2:59

Tgt Ion:266 Resp: 10598
 Ion Ratio Lower Upper
 266 100
 264 61.4 47.9 71.9
 268 63.9 49.8 74.8

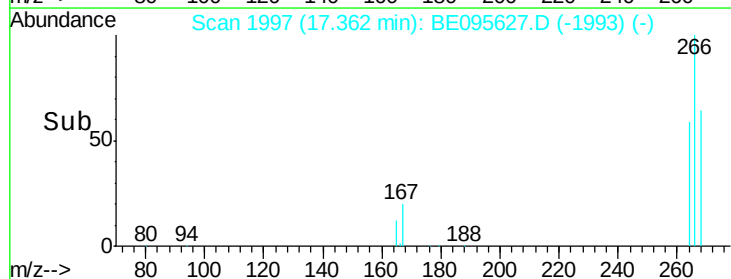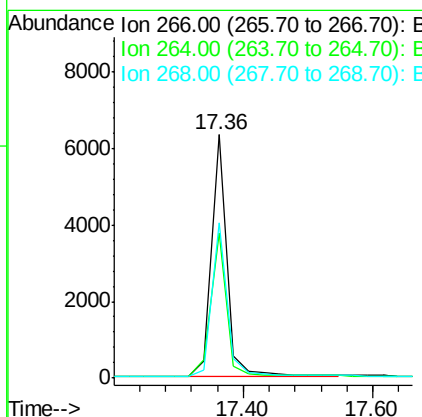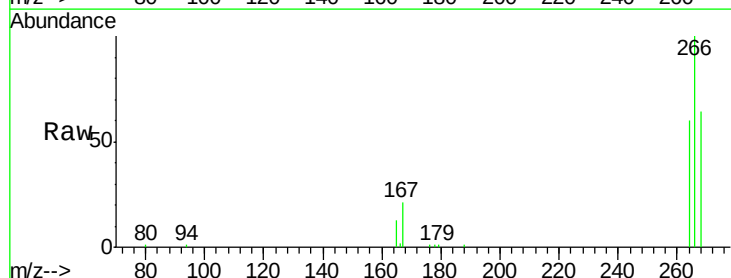

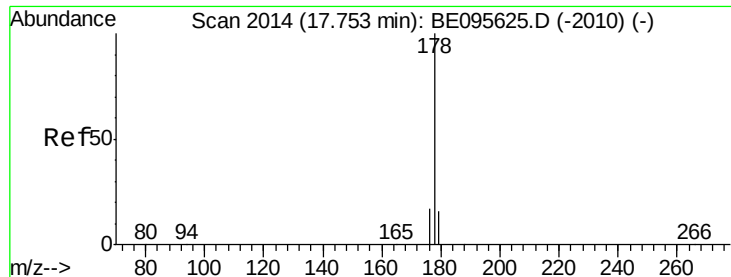

#12

Phenanthrene

Concen: 0.057 ng/ul

RT: 17.85 min Scan# 2018

Delta R.T. 0.09 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 1435

Ion Ratio Lower Upper

178 100

179 24.7 18.4 27.6




176 20.2 13.6 20.4

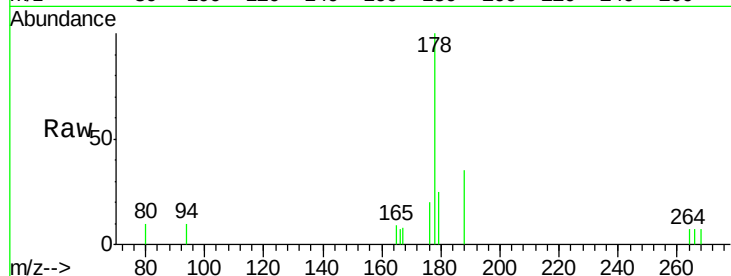

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

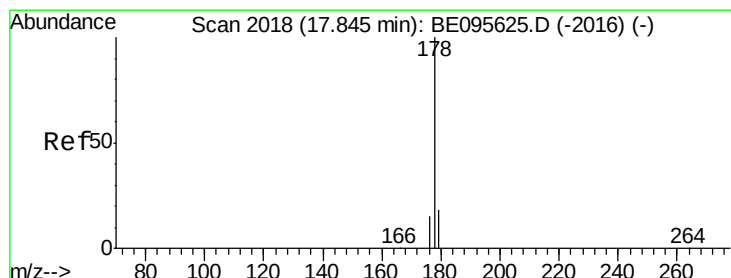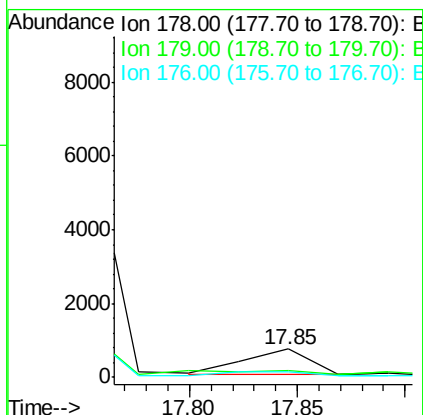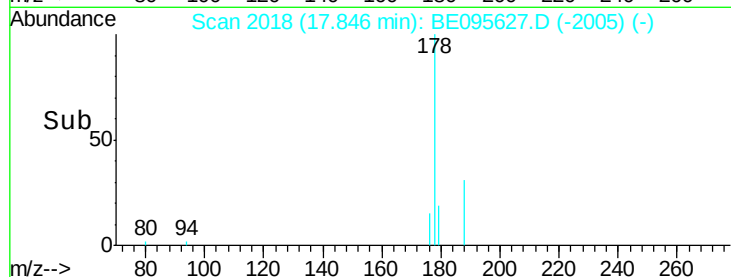

#13

Anthracene

Concen: 0.061 ng/ul

RT: 17.85 min Scan# 2018

Delta R.T. 0.00 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59


Tgt Ion:178 Resp: 1414

Ion Ratio Lower Upper

178 100

179 24.7 18.1 27.1



176 20.2 14.7 22.1

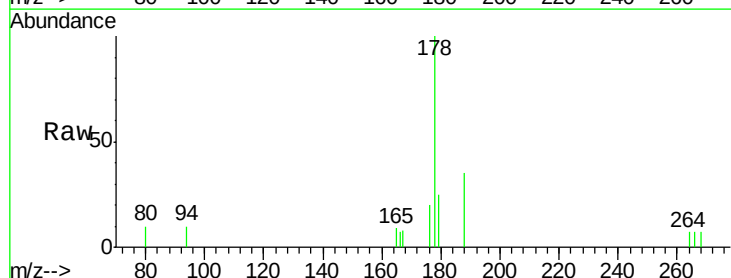


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

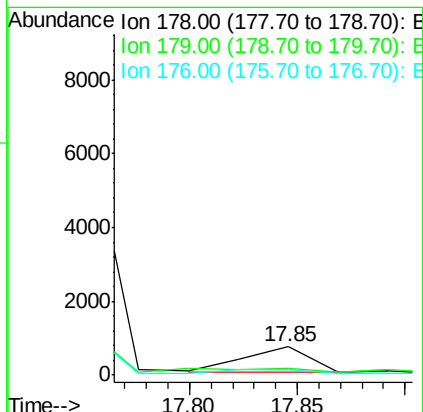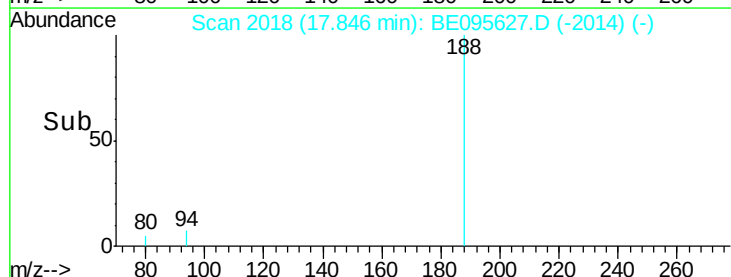

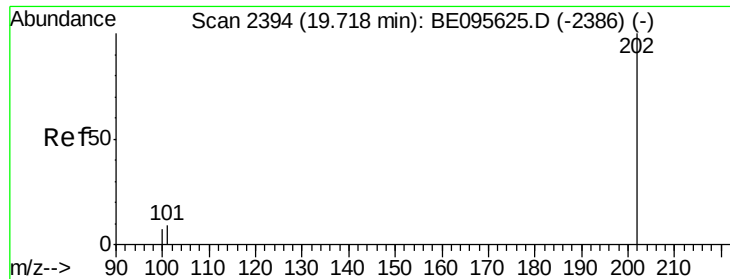

#15

Fluoranthene

Concen: 0.392 ng/ul

RT: 19.72 min Scan# 2394

Delta R.T. 0.00 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 12872

Ion Ratio Lower Upper

202 100

101 9.5 0.0 30.3




100 7.9 0.0 39.5

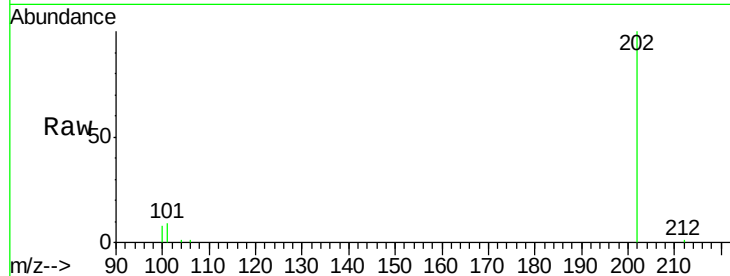

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

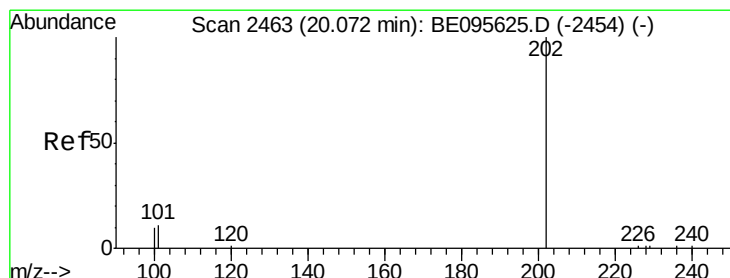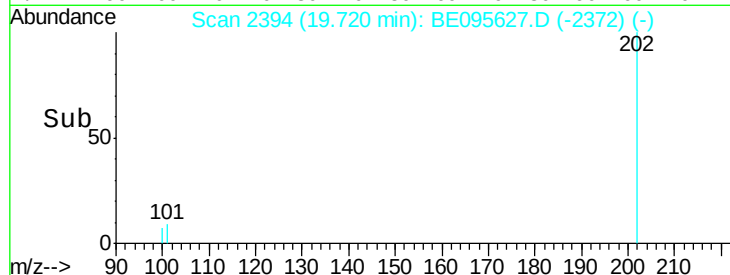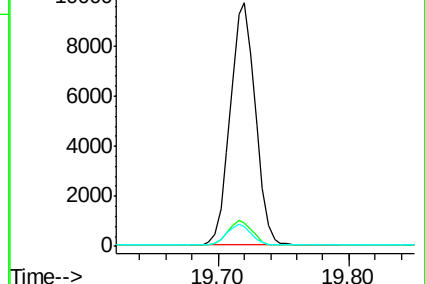

#17

Pyrene

Concen: 0.461 ng/ul

RT: 20.07 min Scan# 2463

Delta R.T. -0.00 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59


Tgt Ion:202 Resp: 11347

Ion Ratio Lower Upper

202 100

101 11.9 18.2 27.4#



100 10.7 15.6 23.4#

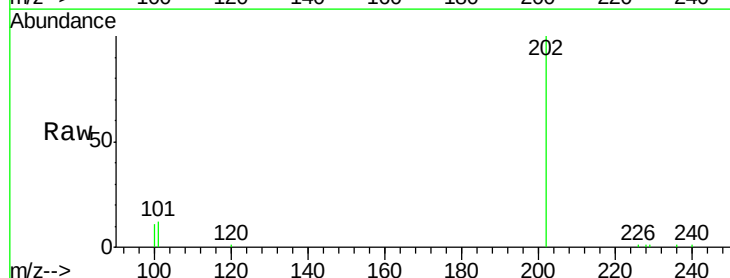


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

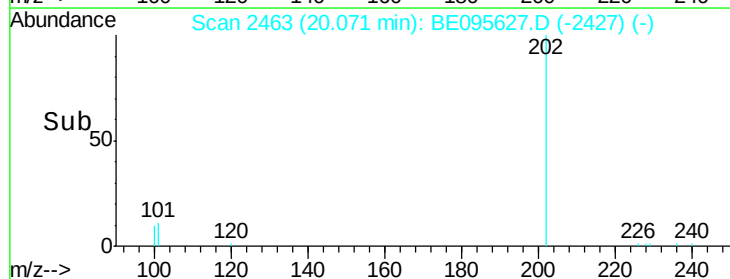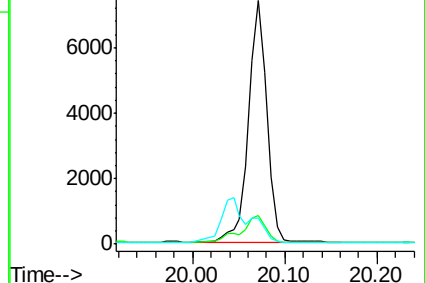

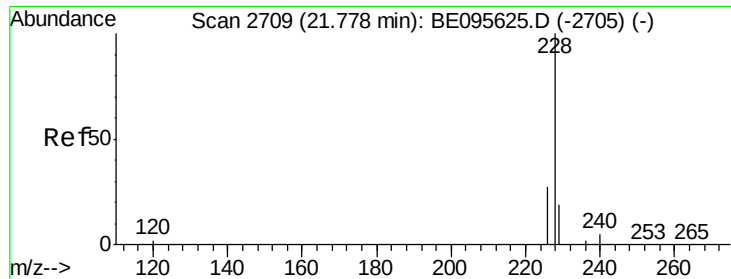

#18

Benzo(a)anthracene

Concen: 0.110 ng/ul

RT: 21.78 min Scan# 2709

Delta R.T. 0.00 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59

Instrument :

BNA_E

ClientSampleId :





Tot Ion:228 Resp: 2525

Ion Ratio Lower Upper

228 100

229 23.7 22.8 34.2

226 29.7 17.0 25.6#

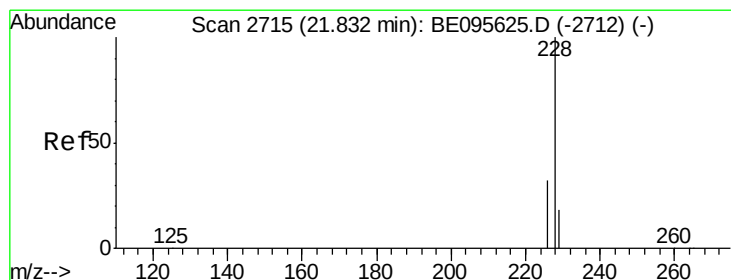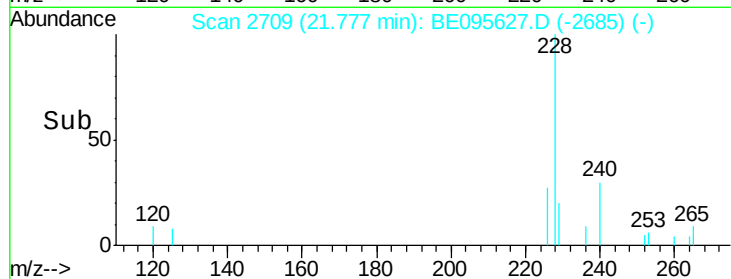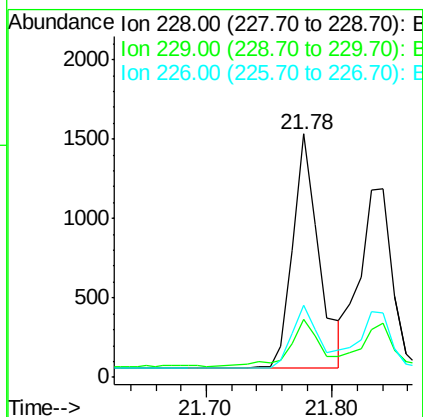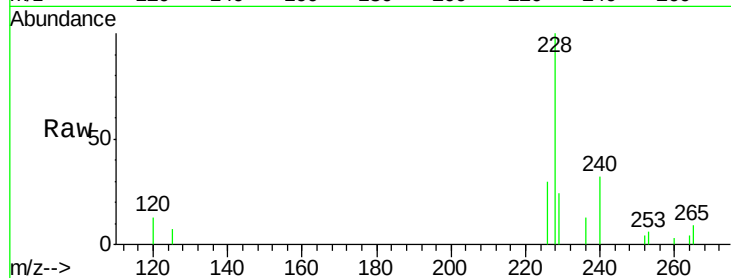

#19

Chrysene

Concen: 0.106 ng/ul

RT: 21.78 min Scan# 2709

Delta R.T. -0.06 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59




Tgt Ion:228 Resp: 2525


Ion Ratio Lower Upper

228 100

226 29.7 23.4 35.0

229 23.7 17.7 26.5

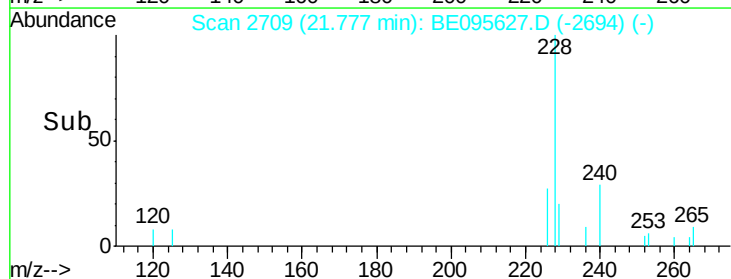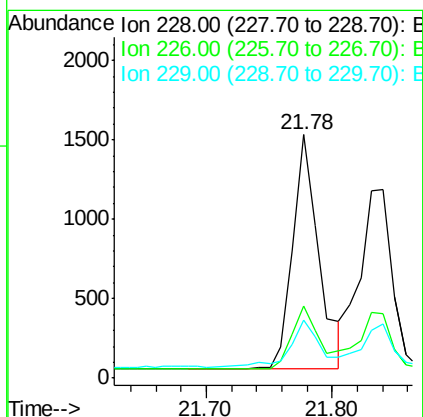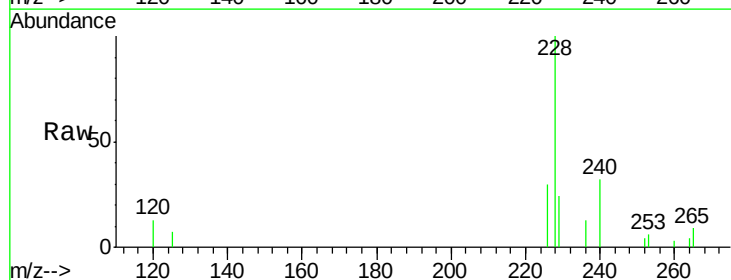

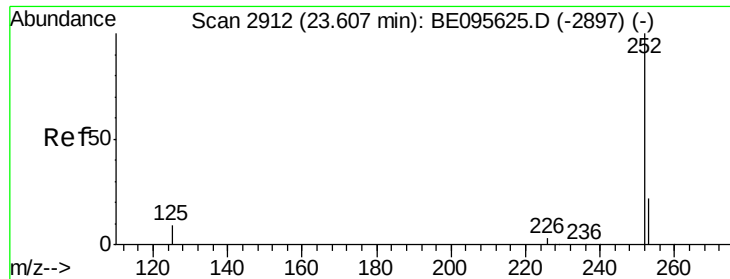

#21

Benzo(b)fluoranthene

Concen: 0.100 ng/ul

RT: 23.62 min Scan# 2913

Delta R.T. 0.01 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 2604

Ion Ratio Lower Upper

252 100

253 32.1 0.0 64.2




125 22.1 0.0 35.0

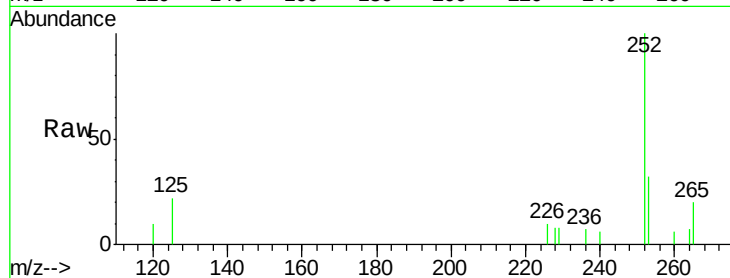

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

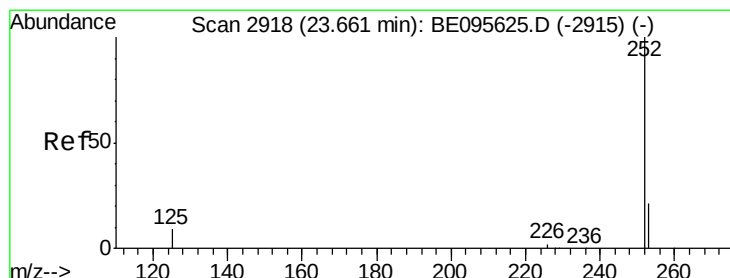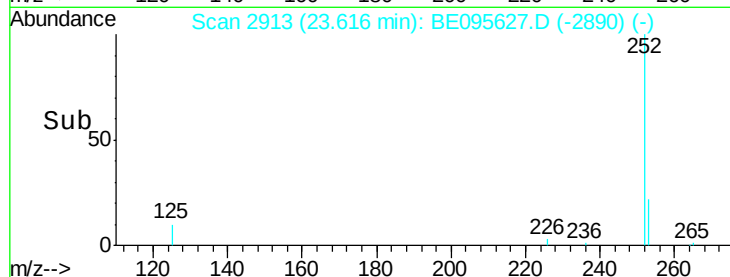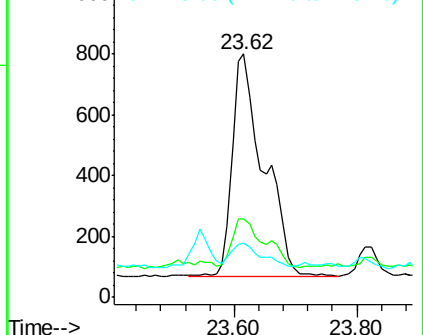

#22

Benzo(k)fluoranthene

Concen: 0.110 ng/ul

RT: 23.62 min Scan# 2913

Delta R.T. -0.04 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59


Tgt Ion:252 Resp: 2604

Ion Ratio Lower Upper

252 100

253 32.1 24.5 36.7



125 22.1 13.7 20.5#

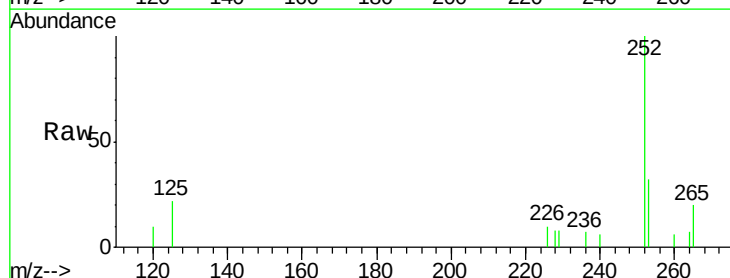


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

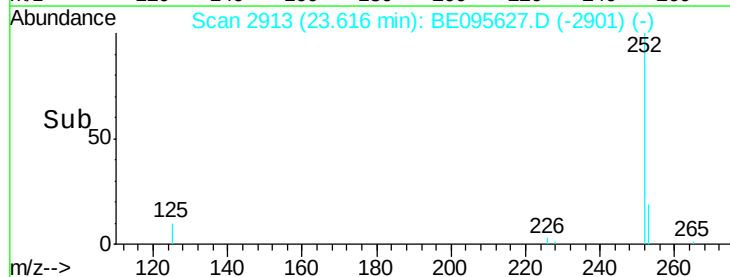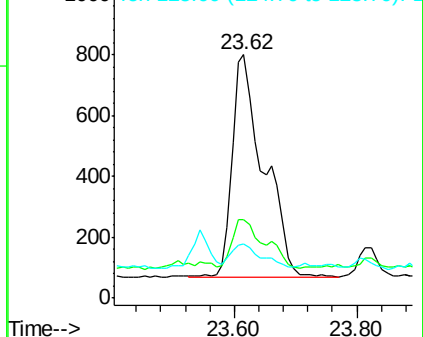

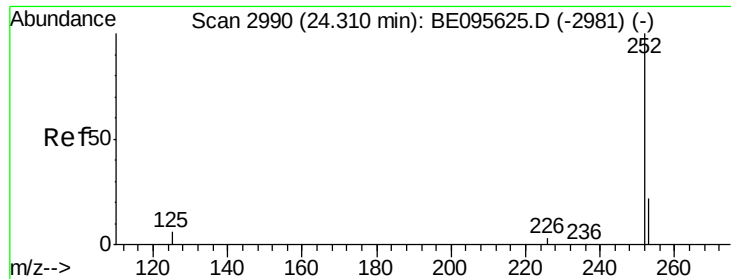

#23

Benzo(a)pyrene

Concen: 0.035 ng/ul

RT: 24.31 min Scan# 2990

Delta R.T. 0.00 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 816

Ion Ratio Lower Upper




252 100

253 41.4 28.5 42.7

125 32.4 18.1 27.1#

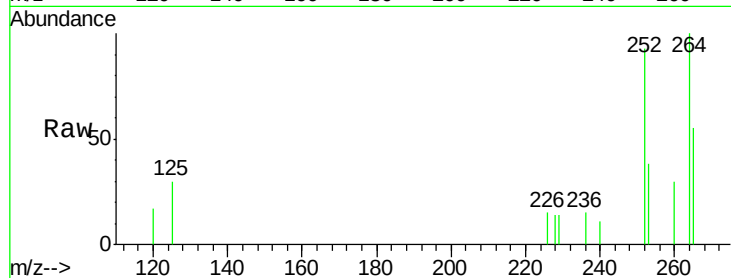

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

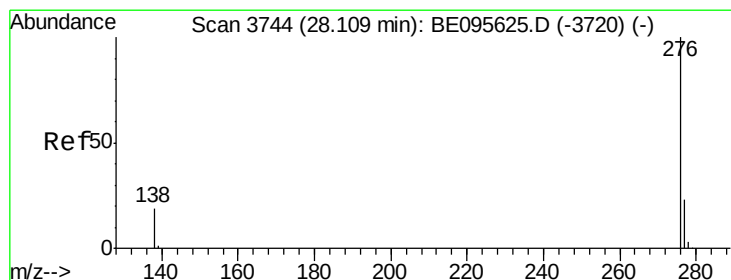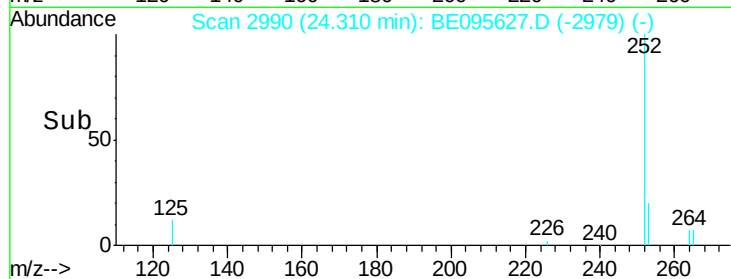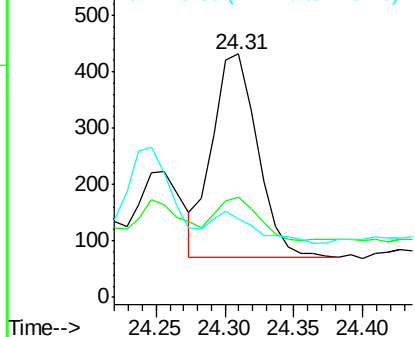

#26

Benzo(g,h,i)perylene

Concen: 0.020 ng/ul

RT: 28.11 min Scan# 3745

Delta R.T. 0.00 min

Lab File: BE095627.D

Acq: 10 Feb 2018 2:59


Tgt Ion:276 Resp: 431

Ion Ratio Lower Upper

276 100

138 49.4 21.8 32.8#

277 48.1 20.5 30.7#

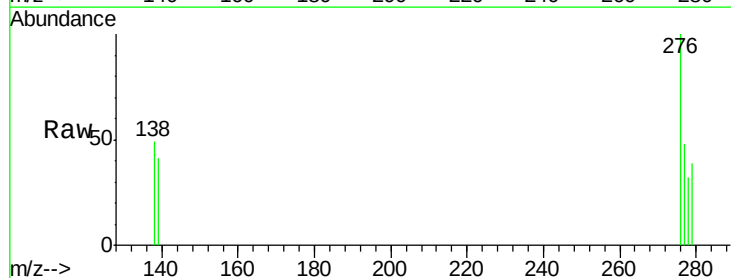

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

