

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095632.D
 Acq On : 10 Feb 2018 5:58
 Operator : SJ/JU
 Sample : J1339-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 12 00:20:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 02:59:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1742	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5143	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3328	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7824	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7263	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	381917	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2879	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7790	0.26	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	59	0.039	ng/ul#	87
17) Pyrene	20.05	202	1229	0.050	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095632.D
Acq On : 10 Feb 2018 5:58
Operator : SJ/JU
Sample : J1339-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 12 00:20:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration




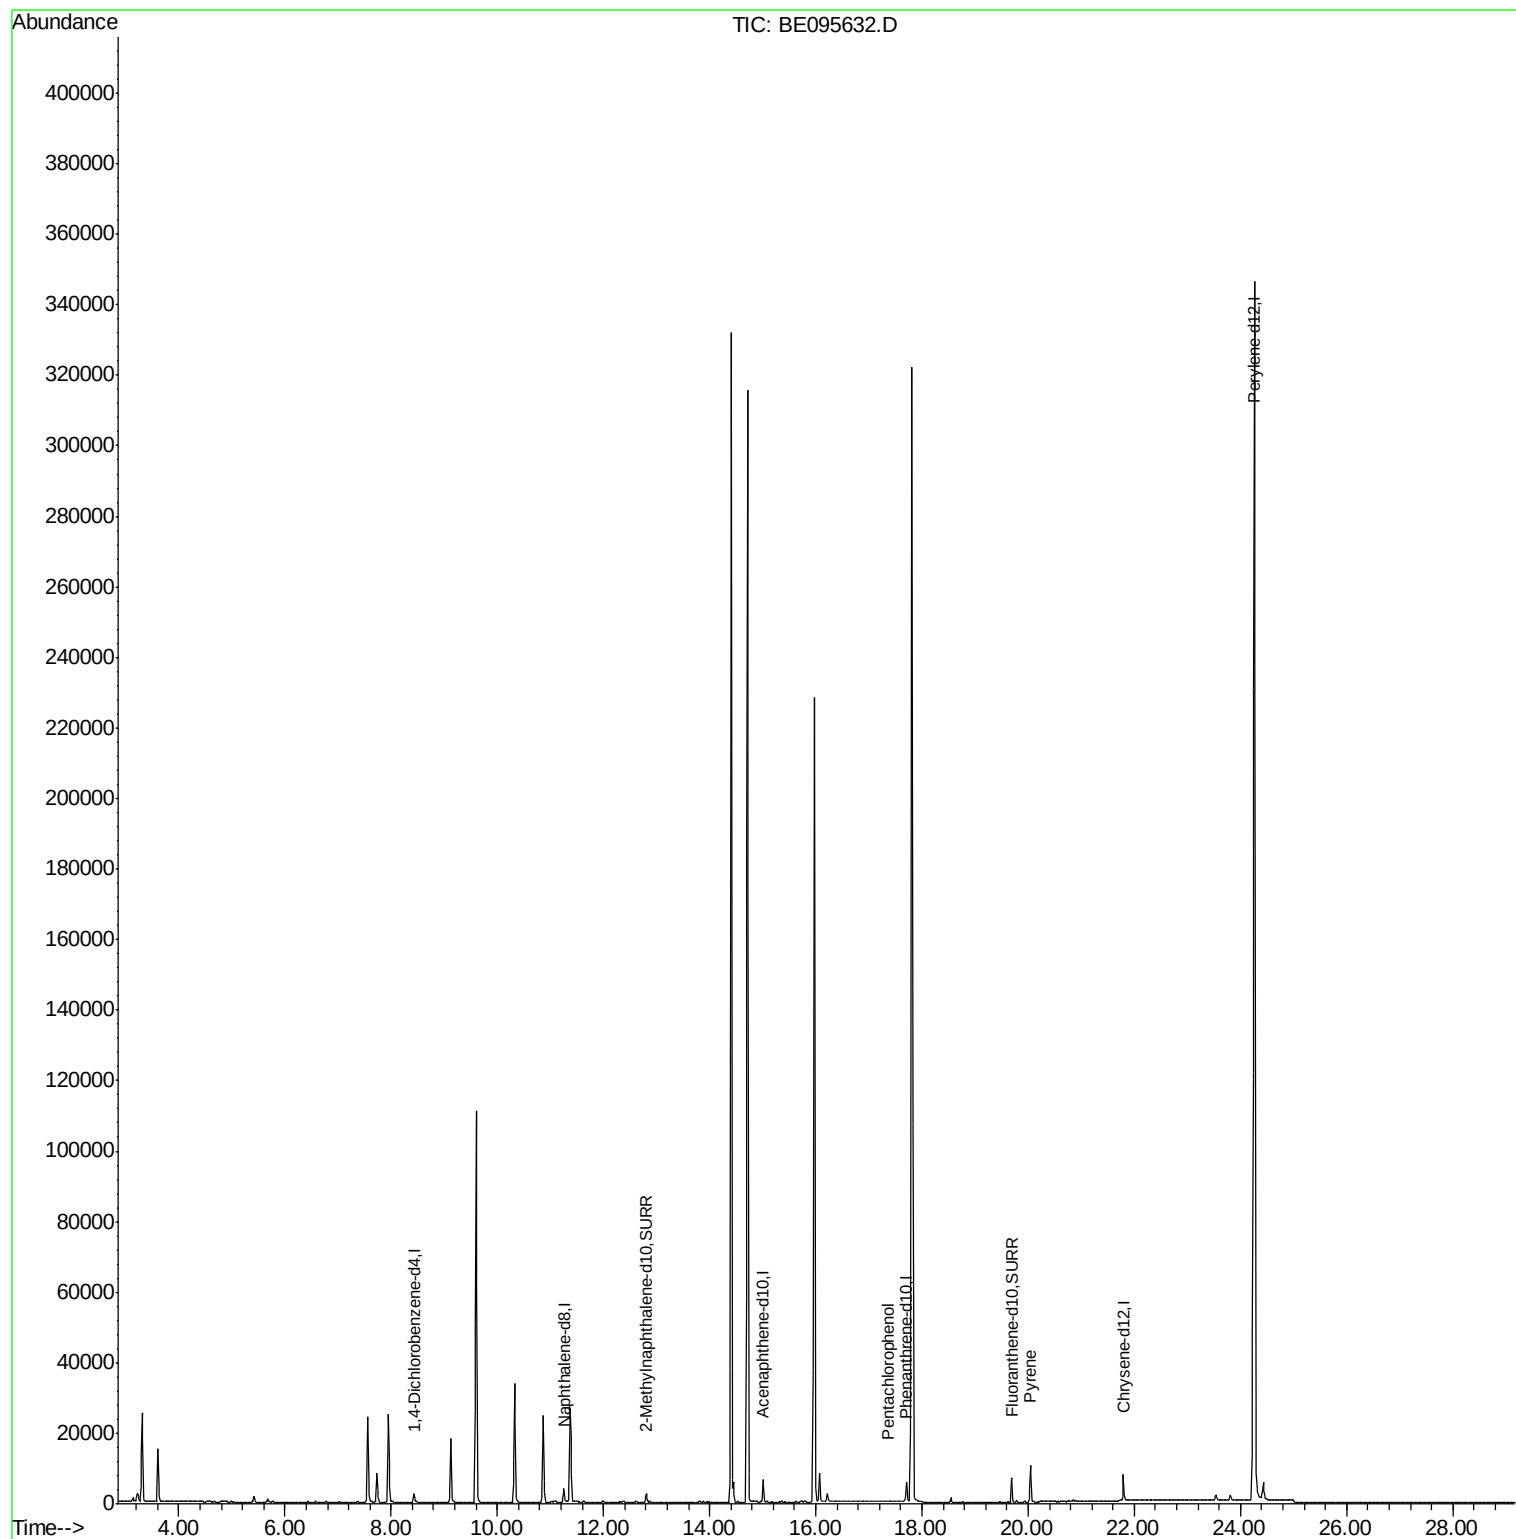


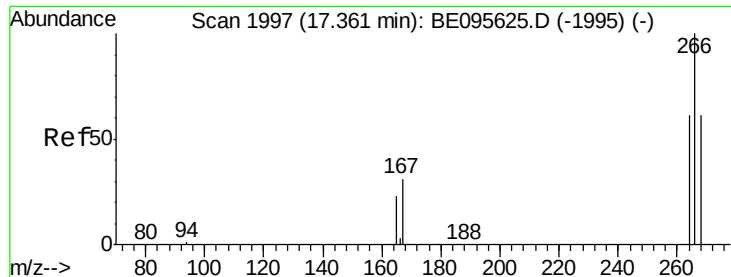

#11
 Pentachlorophenol
 Concen: 0.039 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095632.D
 Acq: 10 Feb 2018 5:58

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 59
 Ion Ratio Lower Upper
 266 100
 264 78.0 47.9 71.9#
 268 61.0 49.8 74.8

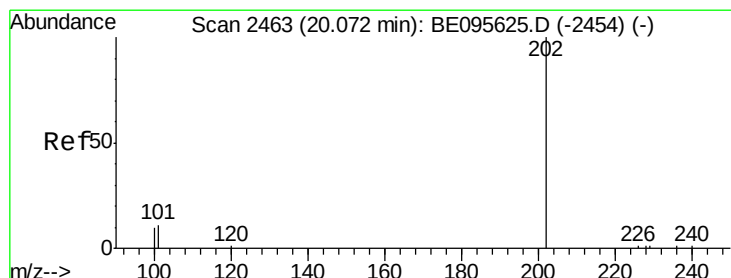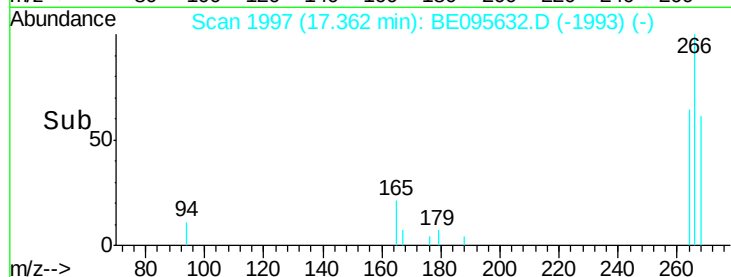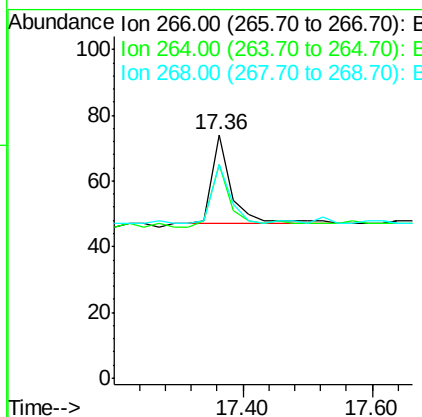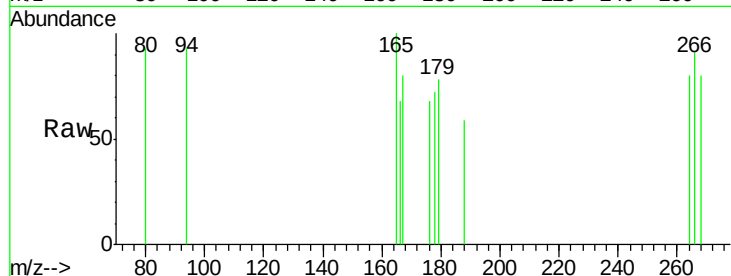

#17
 Pyrene
 Concen: 0.050 ng/ul
 RT: 20.05 min Scan# 2459
 Delta R.T. -0.03 min
 Lab File: BE095632.D
 Acq: 10 Feb 2018 5:58

Tgt Ion:202 Resp: 1229
 Ion Ratio Lower Upper
 202 100
 101 170.1 18.2 27.4#
 100 1162.7 15.6 23.4#

