

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095634.D
 Acq On : 10 Feb 2018 7:07
 Operator : SJ/JU
 Sample : J1339-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 12 00:20:20 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 02:59:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1973	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5834	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3902	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8900	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8152	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	503013	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3465	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9418	0.28	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	88488	51.332	ng/ul	98
12) Phenanthrene	17.75	178	805	0.027	ng/ul#	71
17) Pyrene	20.05	202	1337	0.049	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095634.D
Acq On : 10 Feb 2018 7:07
Operator : SJ/JU
Sample : J1339-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 12 00:20:20 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

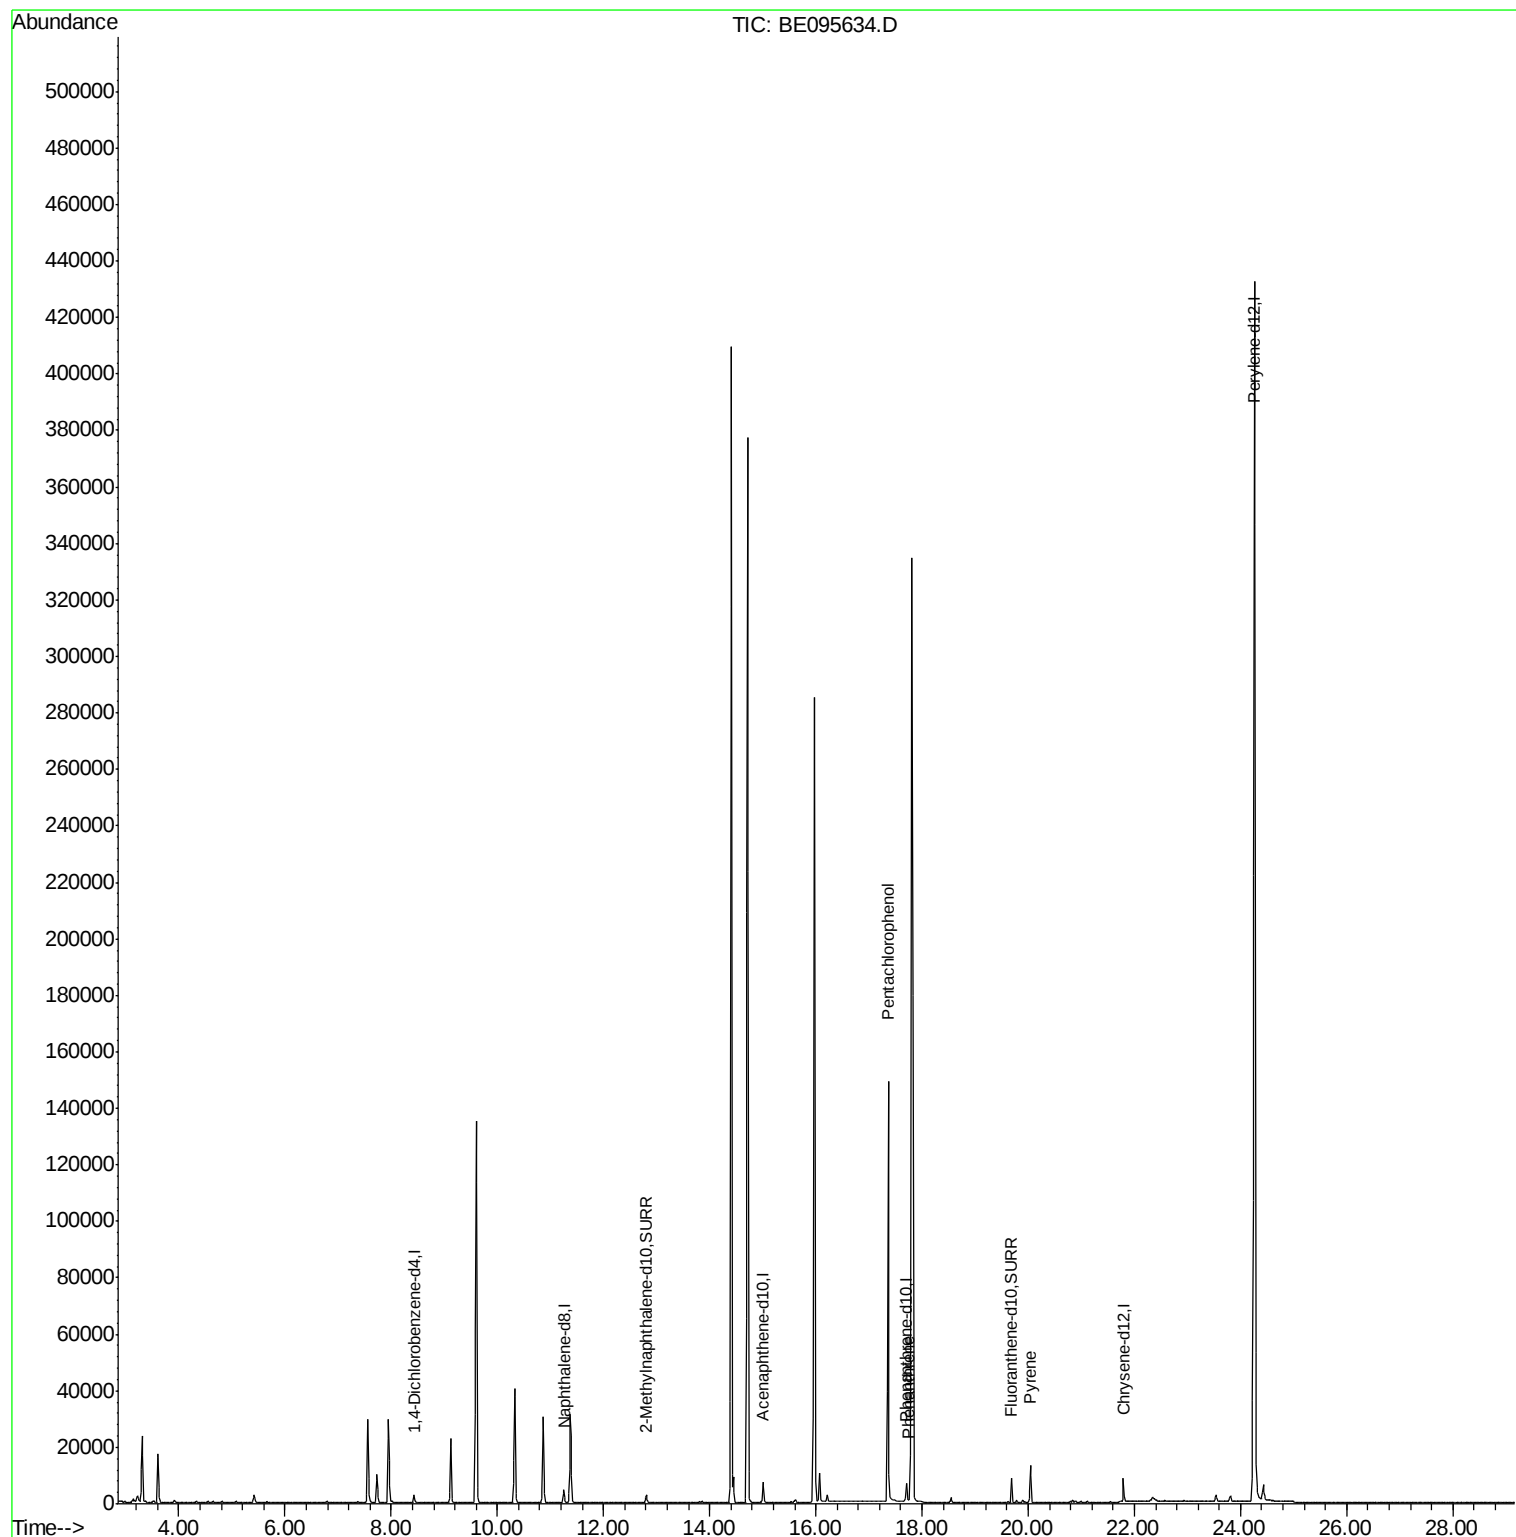


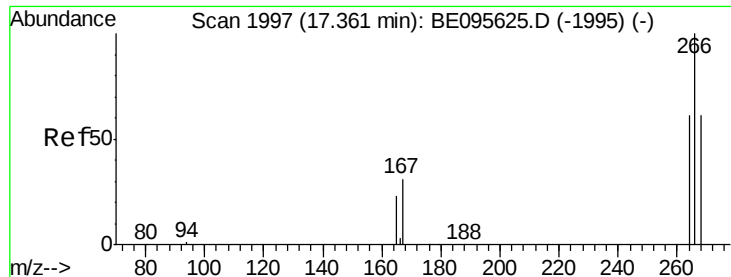




#11
 Pentachlorophenol
 Concen: 51.332 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095634.D
 Acq: 10 Feb 2018 7:07

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 88488
 Ion Ratio Lower Upper
 266 100
 264 62.6 47.9 71.9
 268 62.8 49.8 74.8

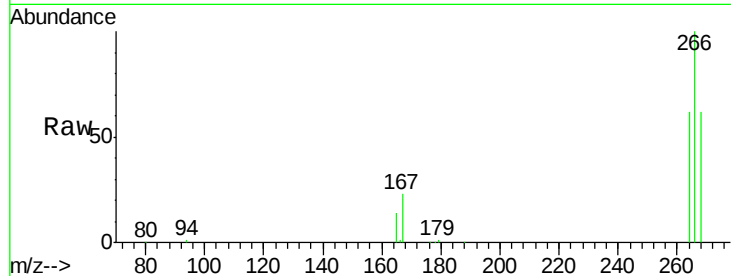


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

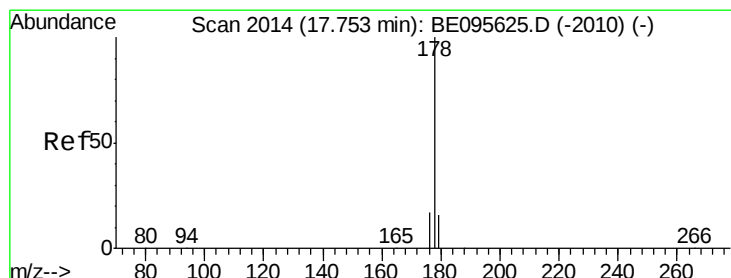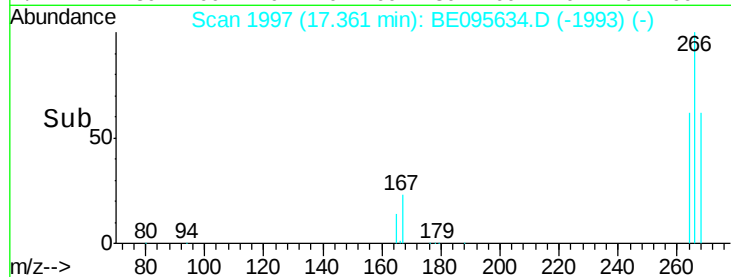
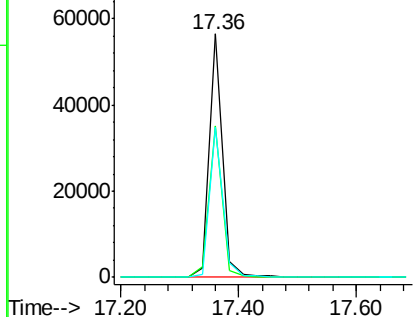





#12
 Phenanthrene
 Concen: 0.027 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095634.D
 Acq: 10 Feb 2018 7:07

Tgt Ion:178 Resp: 805
 Ion Ratio Lower Upper
 178 100
 179 35.6 18.4 27.6#
 176 31.2 13.6 20.4#

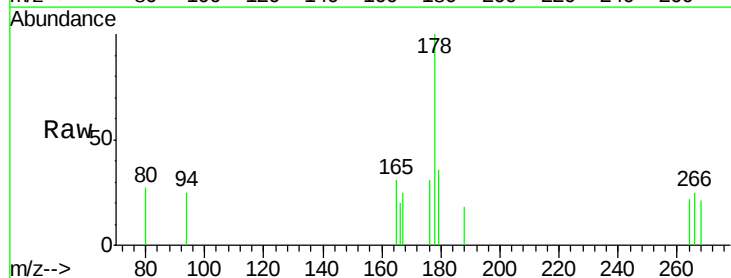

Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

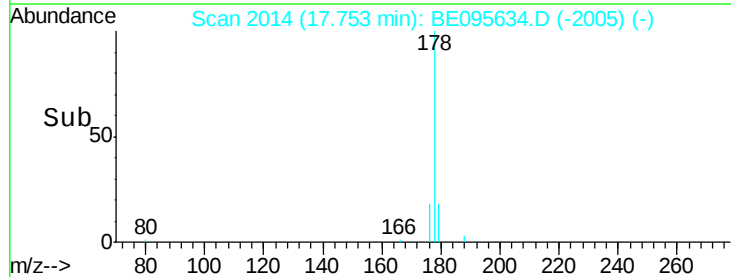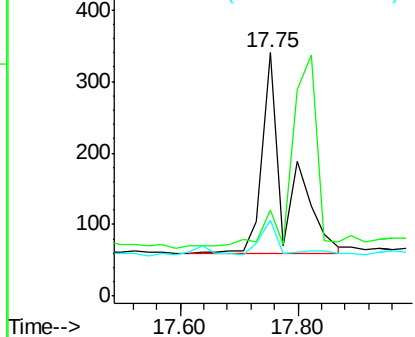

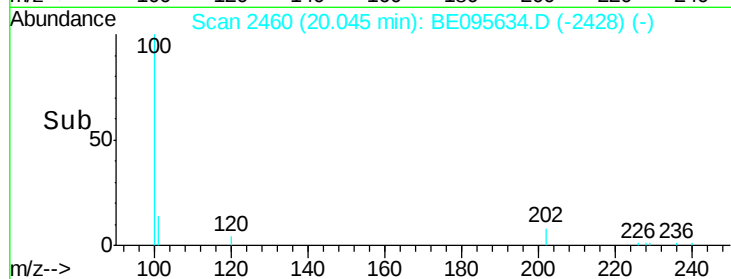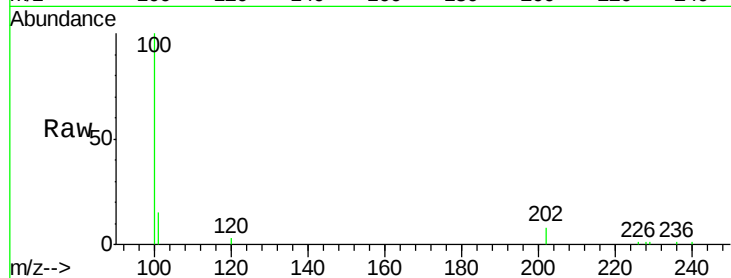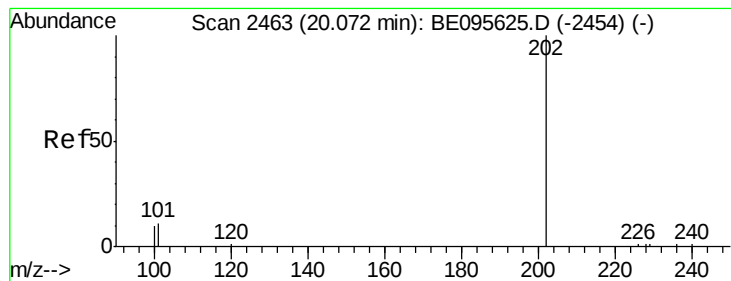

#17

Pvrene

Concen: 0.049 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095634.D

Acq: 10 Feb 2018 7:07

Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 1337

Ion Ratio Lower Upper

202 100

101 175.2 18.2 27.4#

100 1204.8 15.6 23.4#

