

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095643.D
 Acq On : 10 Feb 2018 13:05
 Operator : SJ/JU
 Sample : J1355-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 12 01:58:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 12 01:48:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2129	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	6344	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4216	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9852	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8775	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	626816	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.80	152	4379	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	11733	0.31	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	278	0.146	ng/ul	91
12) Phenanthrene	17.75	178	1265	0.038	ng/ul#	86
17) Pyrene	20.05	202	2276	0.077	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095643.D
Acq On : 10 Feb 2018 13:05
Operator : SJ/JU
Sample : J1355-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 12 01:58:56 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 01:48:13 2018
Response via : Initial Calibration




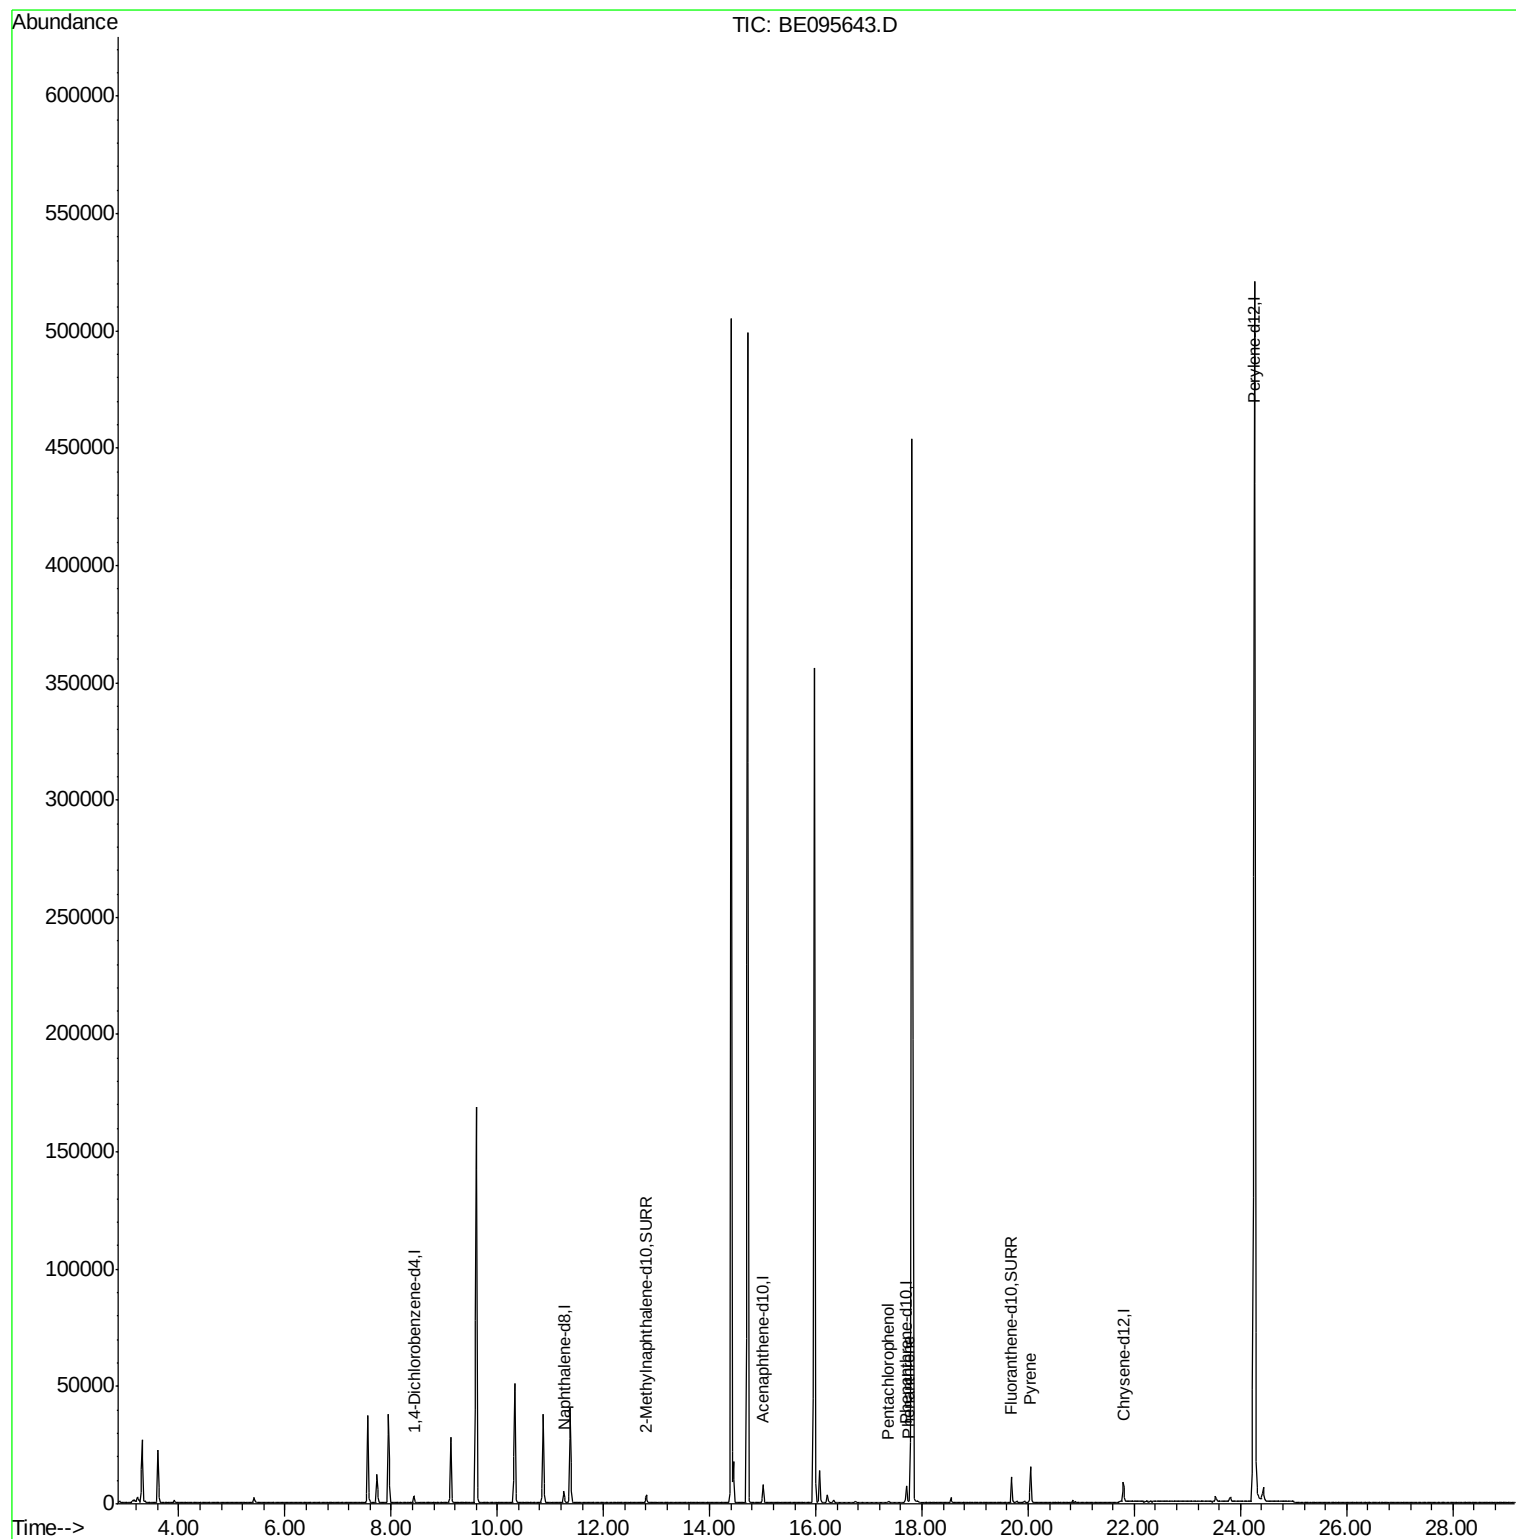


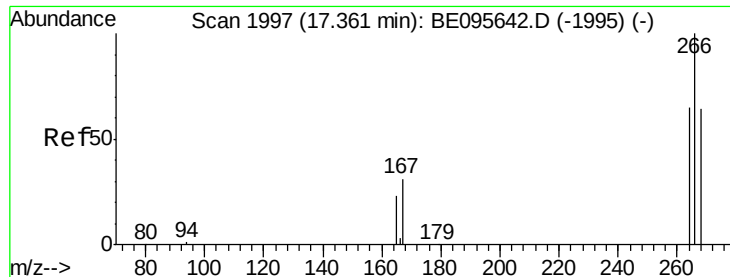

#11
 Pentachlorophenol
 Concen: 0.146 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095643.D
 Acq: 10 Feb 2018 13:05




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:266 Resp: 278
 Ion Ratio Lower Upper
 266 100
 264 68.0 47.9 71.9
 268 67.3 49.8 74.8

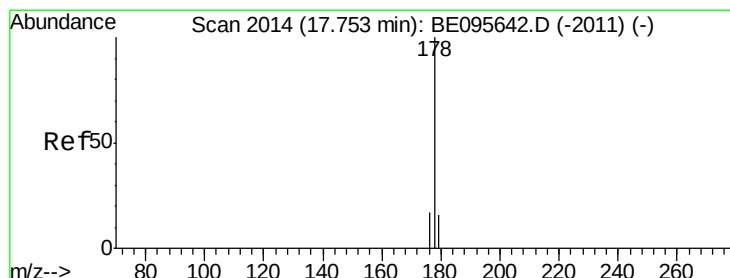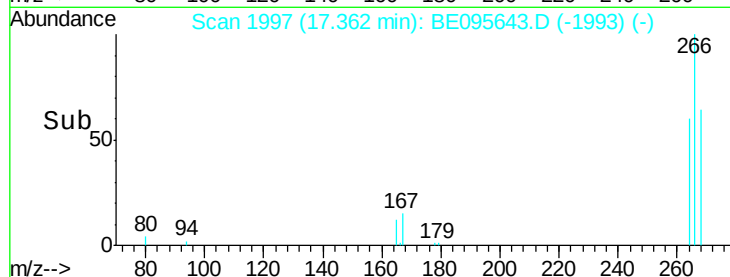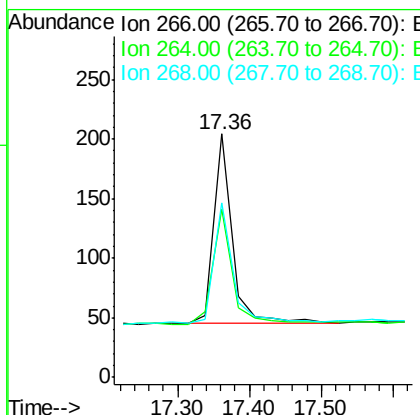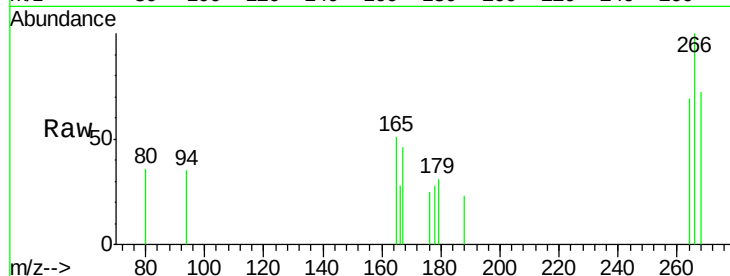

#12
 Phenanthrene
 Concen: 0.038 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095643.D
 Acq: 10 Feb 2018 13:05

Tgt Ion:178 Resp: 1265
 Ion Ratio Lower Upper
 178 100
 179 28.0 18.4 27.6#
 176 25.1 13.6 20.4#

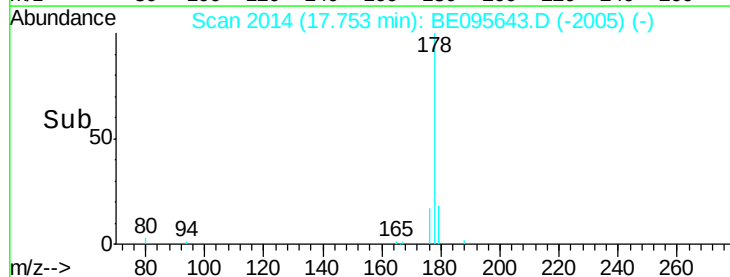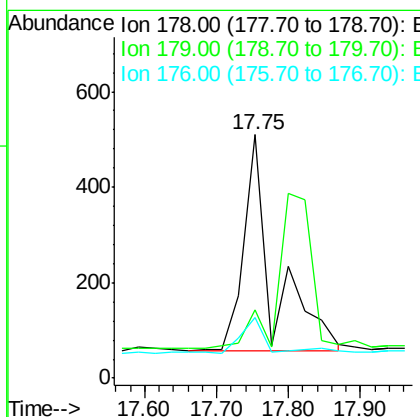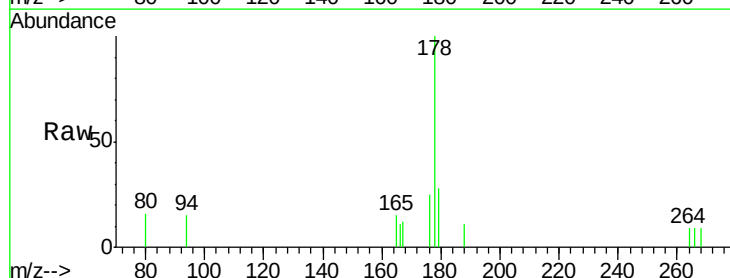

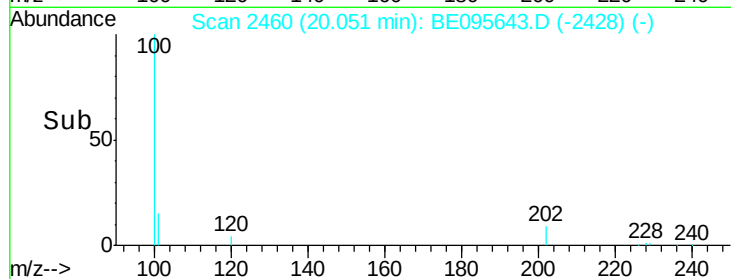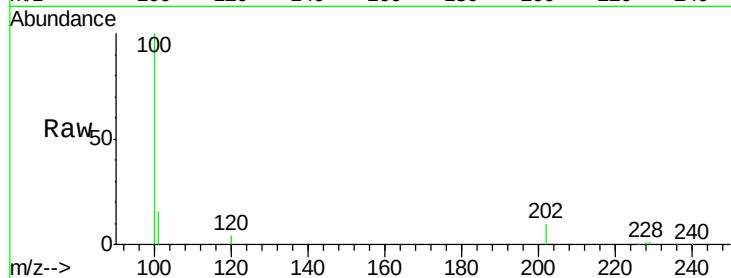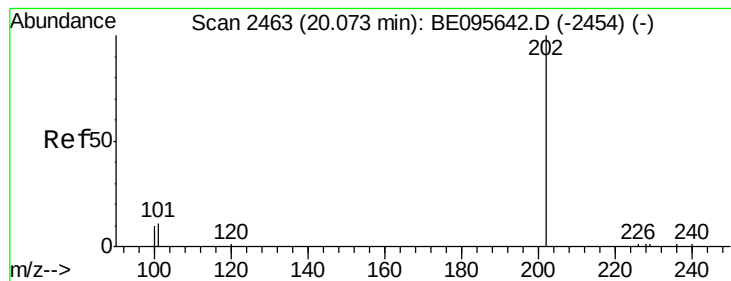

#17

Pvrene

Concen: 0.077 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.02 min

Lab File: BE095643.D

Acq: 10 Feb 2018 13:05

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 202 Resp: 2276

Ion Ratio Lower Upper

202 100

101 160.8 18.2 27.4#

100 1008.6 15.6 23.4#

