


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095601.D
Acq On : 9 Feb 2018 11:13
Operator : SJ/JU
Sample : J1317-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D02

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:23 AM

Quant Time: Feb 09 23:53:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

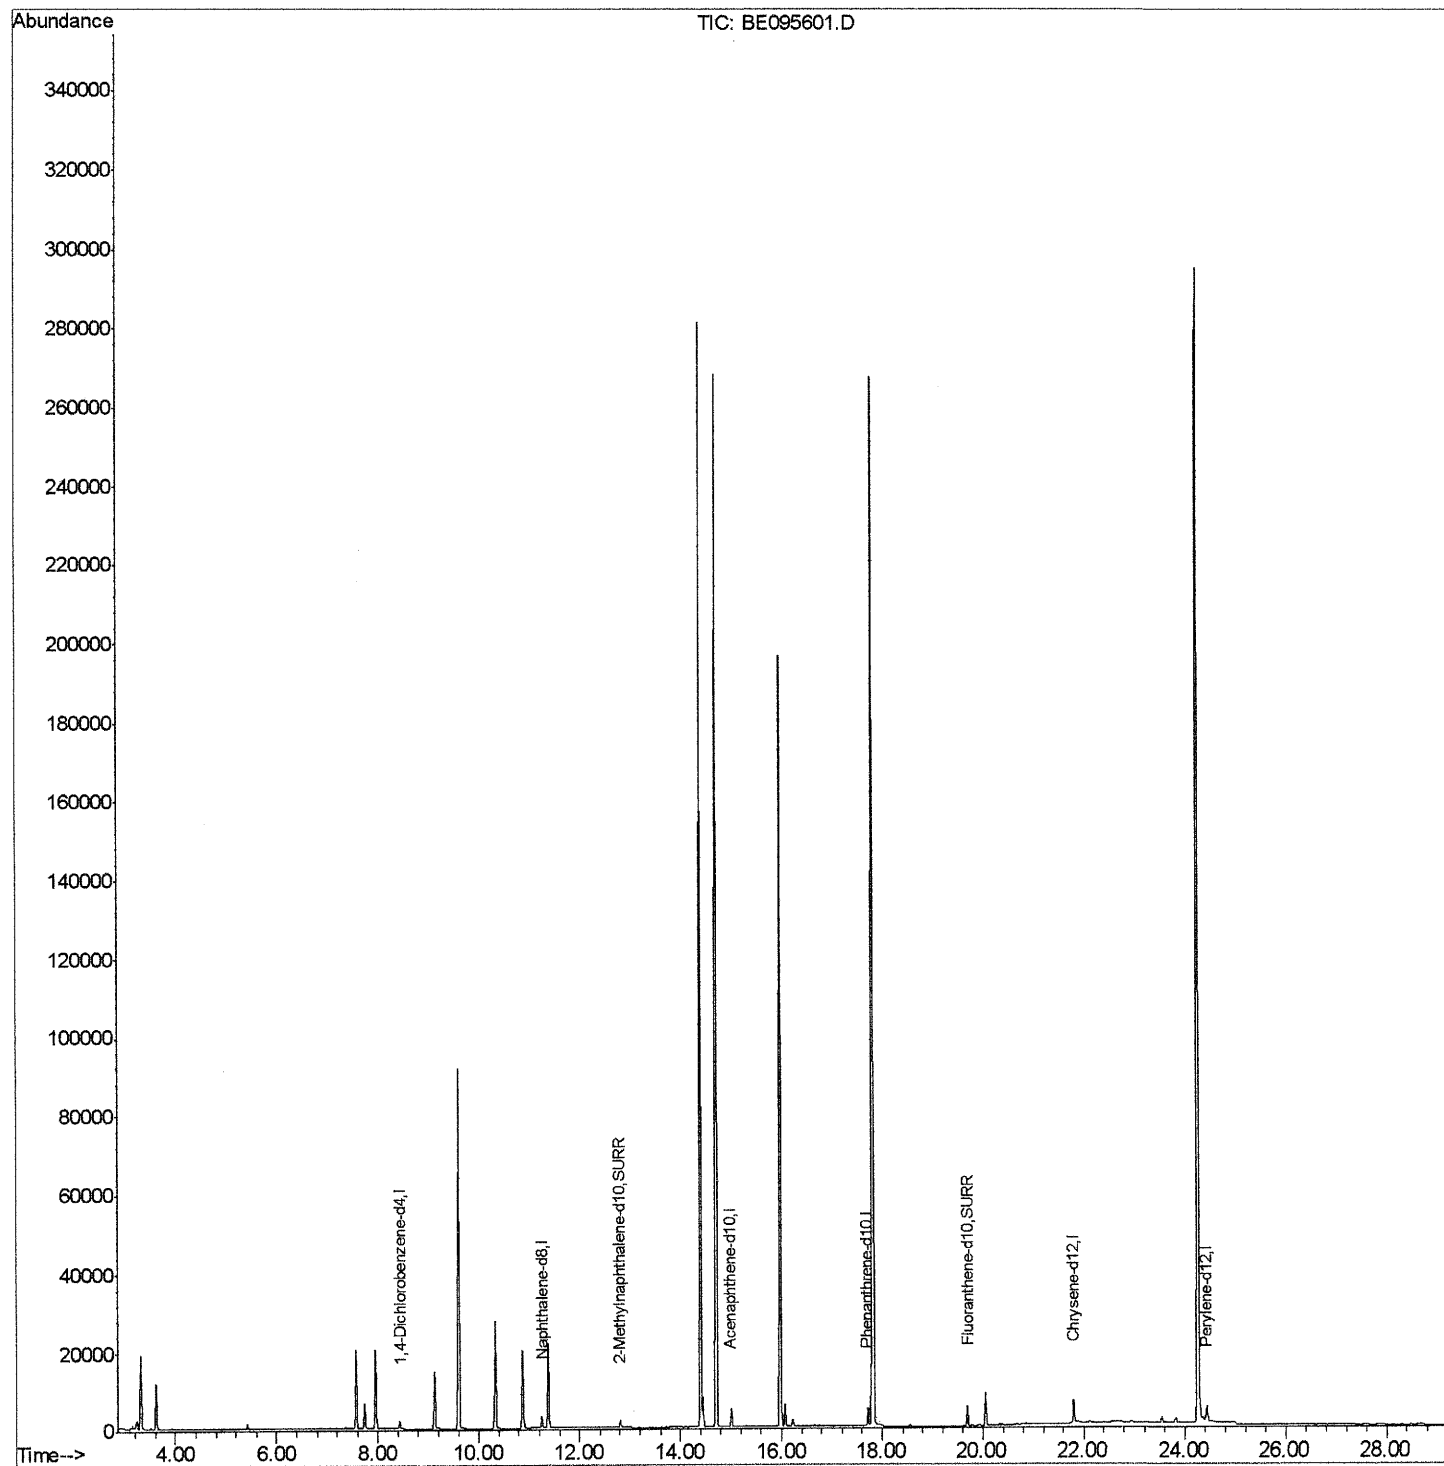

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095601.D
Acq On : 9 Feb 2018 11:13
Operator : SJ/JU
Sample : J1317-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D02

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:23 AM

Quant Time: Feb 09 23:40:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

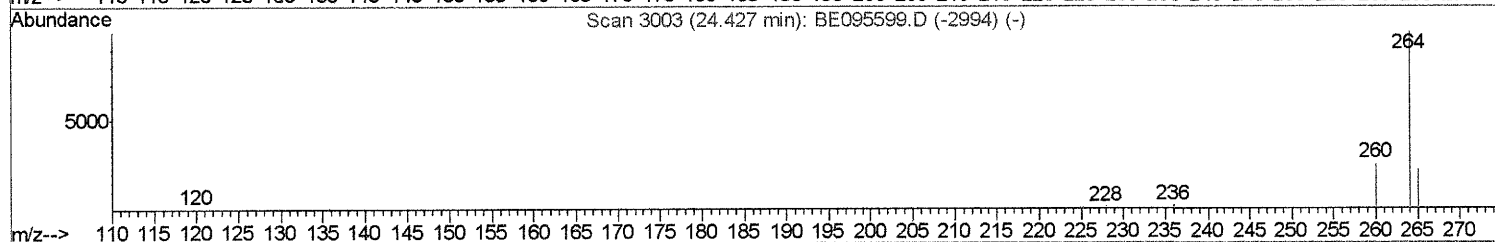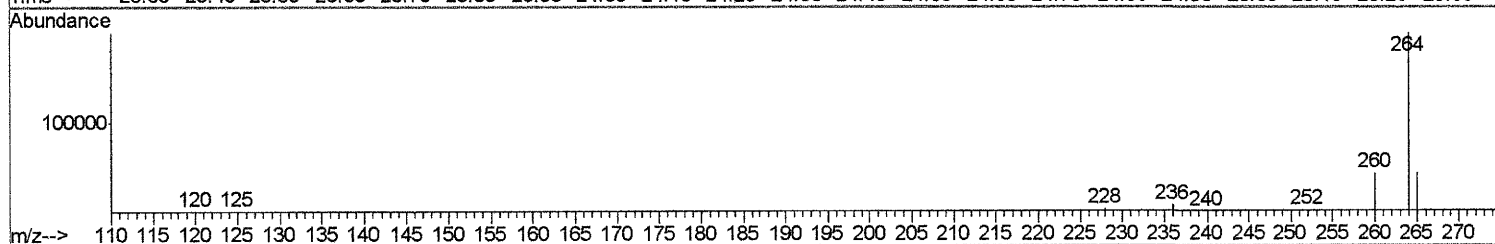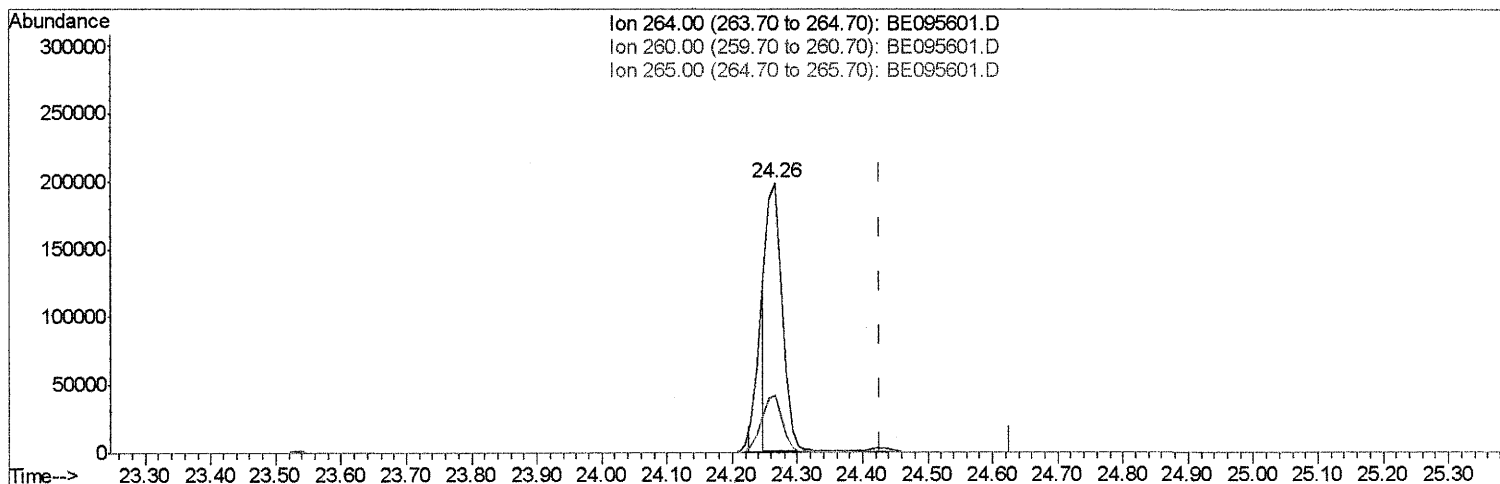

TIC: BE095601.D

(20) Perylene-d12 (I)

24.265min (-0.163) 0.40ng/ul

response 323822

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.96#
265.00	103.50	21.58#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095601.D
Acq On : 9 Feb 2018 11:13
Operator : SJ/JU
Sample : J1317-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D02

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:23 AM

Quant Time: Feb 09 23:40:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

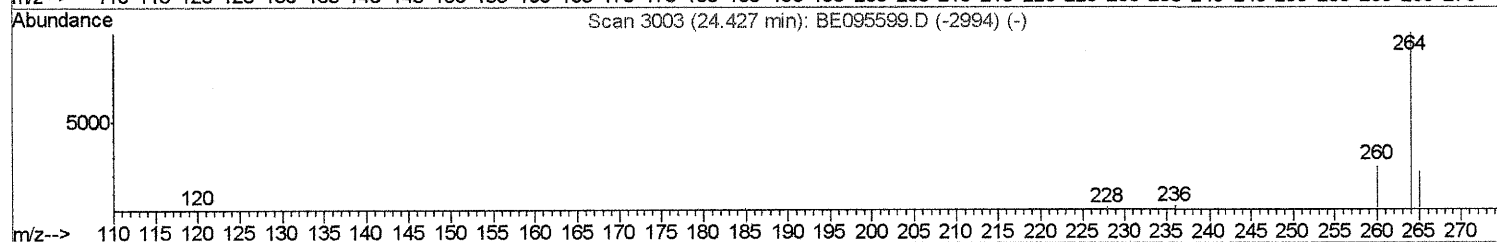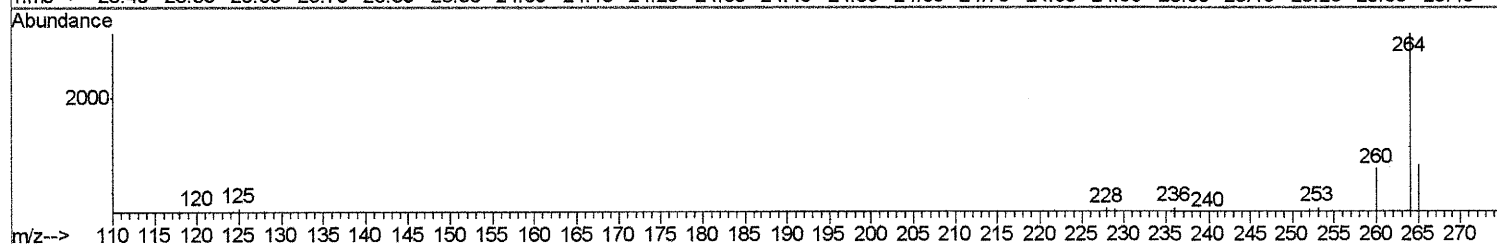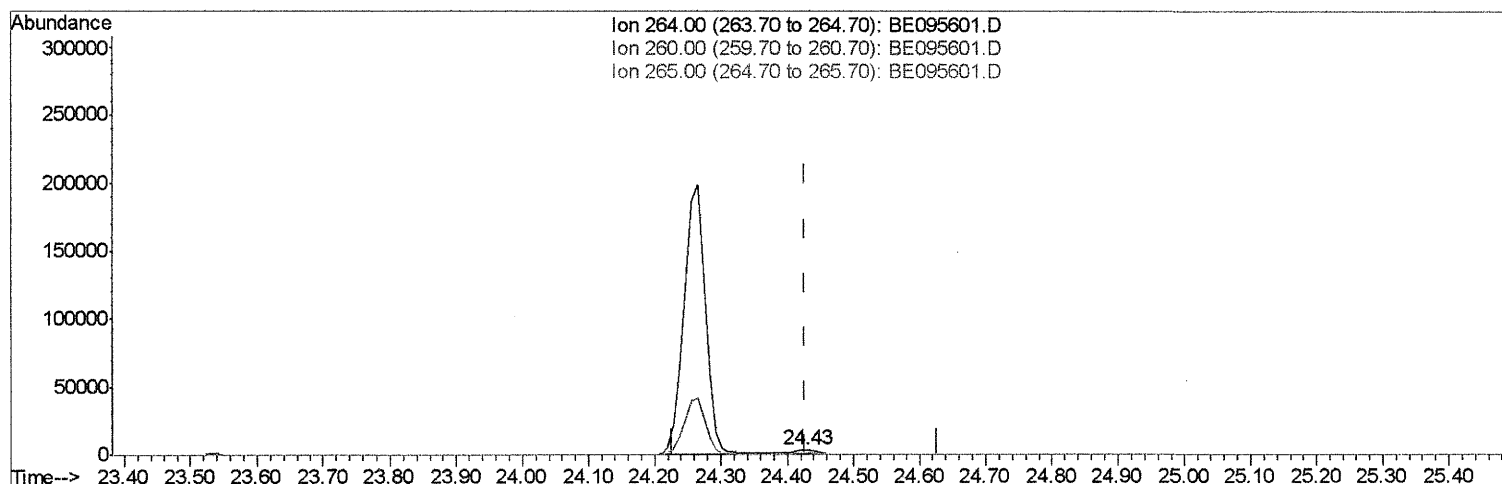

TIC: BE095601.D

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m> SJ 2/13/18

response 5680

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.59
265.00	103.50	27.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095601.D
Acq On : 9 Feb 2018 11:13
Operator : SJ/JU
Sample : J1317-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D02

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:23 AM

Quant Time: Feb 09 23:53:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1500	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4286	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2858	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6922	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6352	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	5680m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2345	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6563	0.25	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/13/18