


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095607.D
Acq On : 9 Feb 2018 14:48
Operator : SJ/JU
Sample : PB106255BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:40 AM

Quant Time: Feb 10 00:36:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

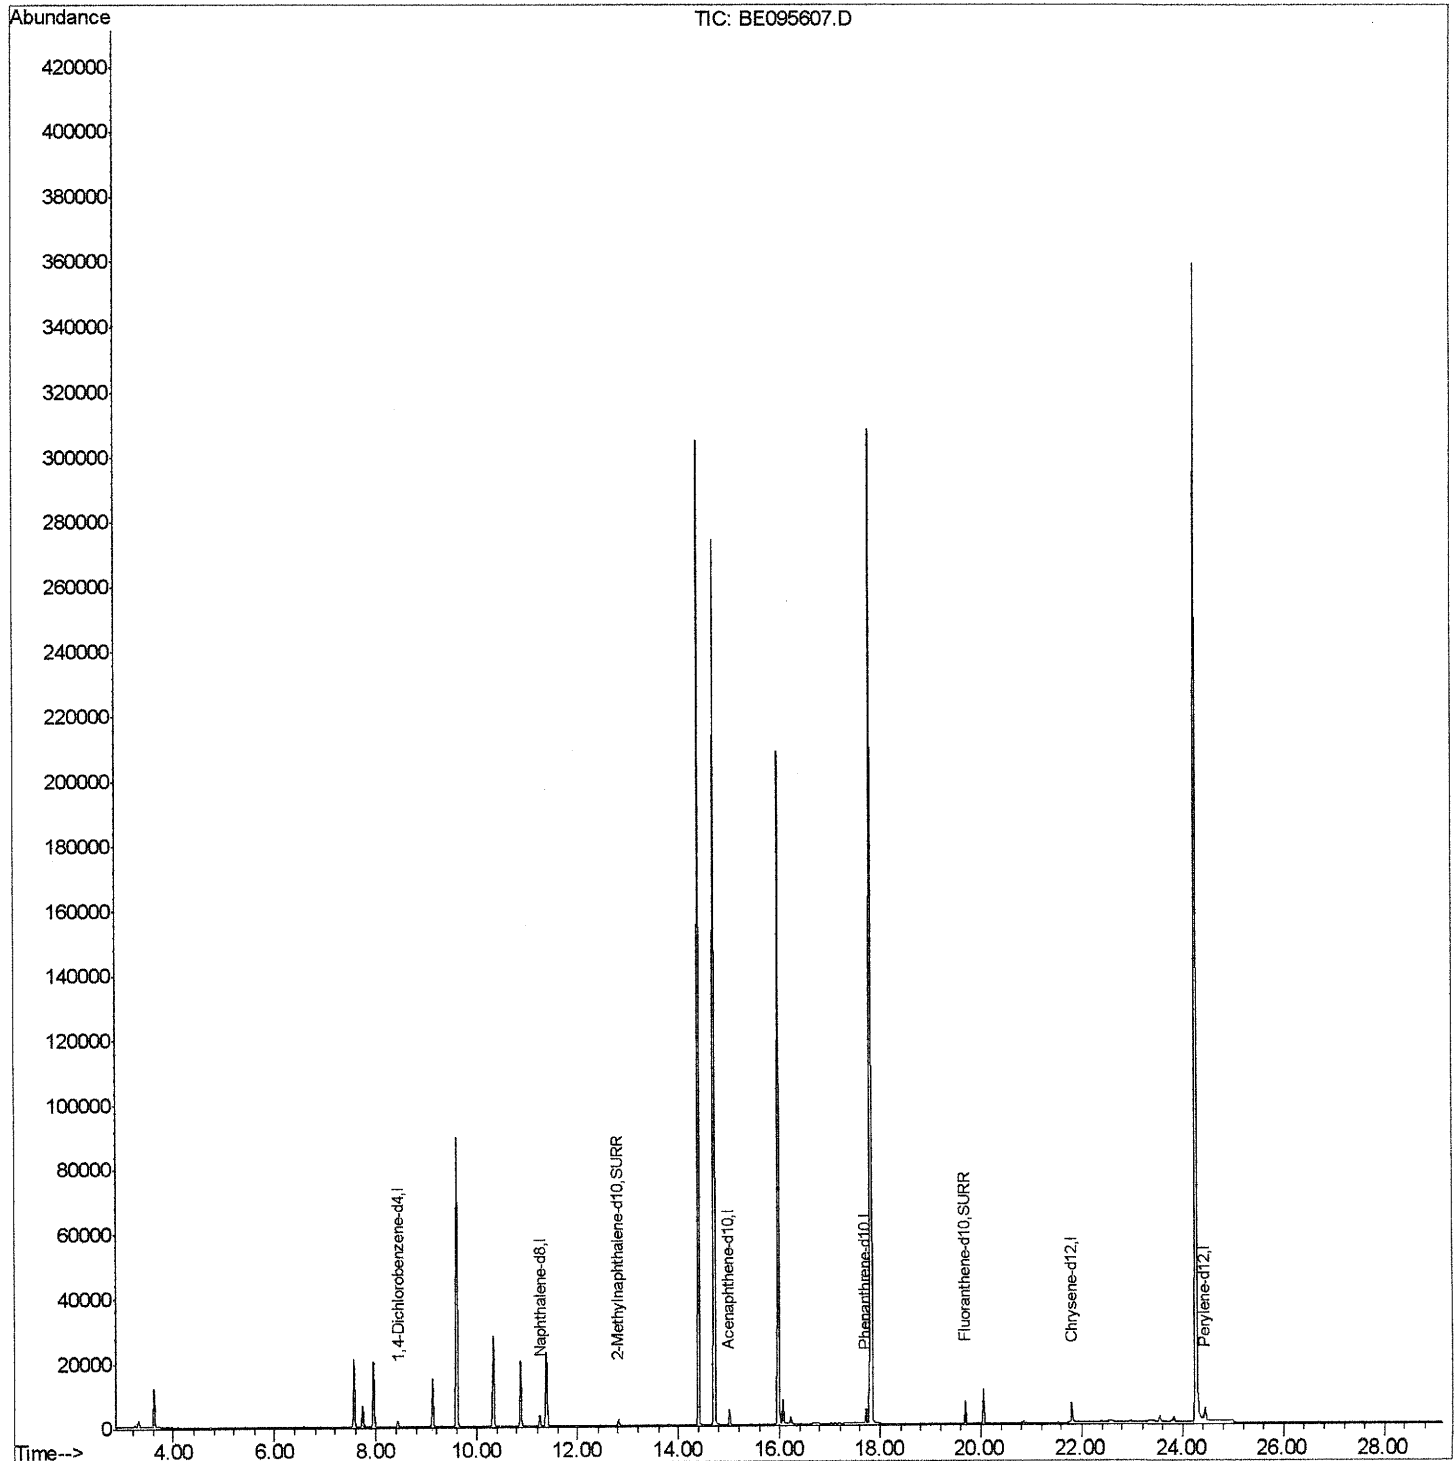

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095607.D
Acq On : 9 Feb 2018 14:48
Operator : SJ/JU
Sample : PB106255BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK55

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:40 AM

Quant Time: Feb 09 23:41:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

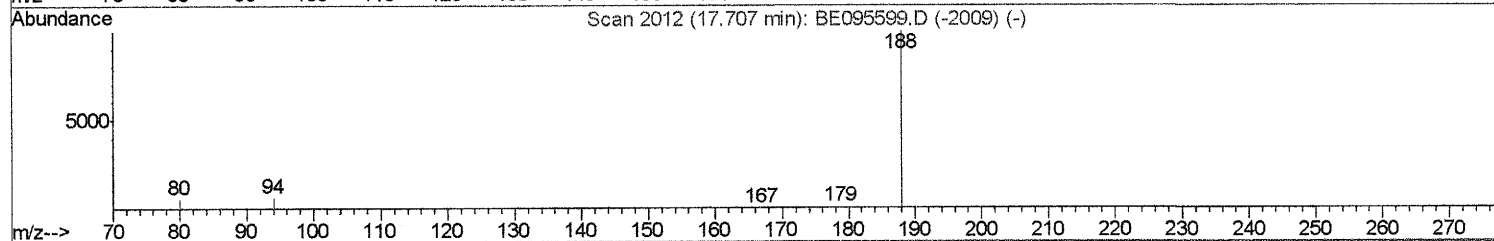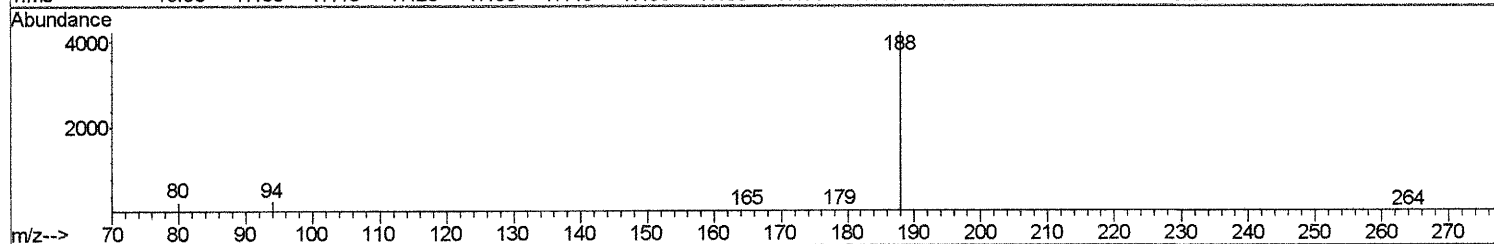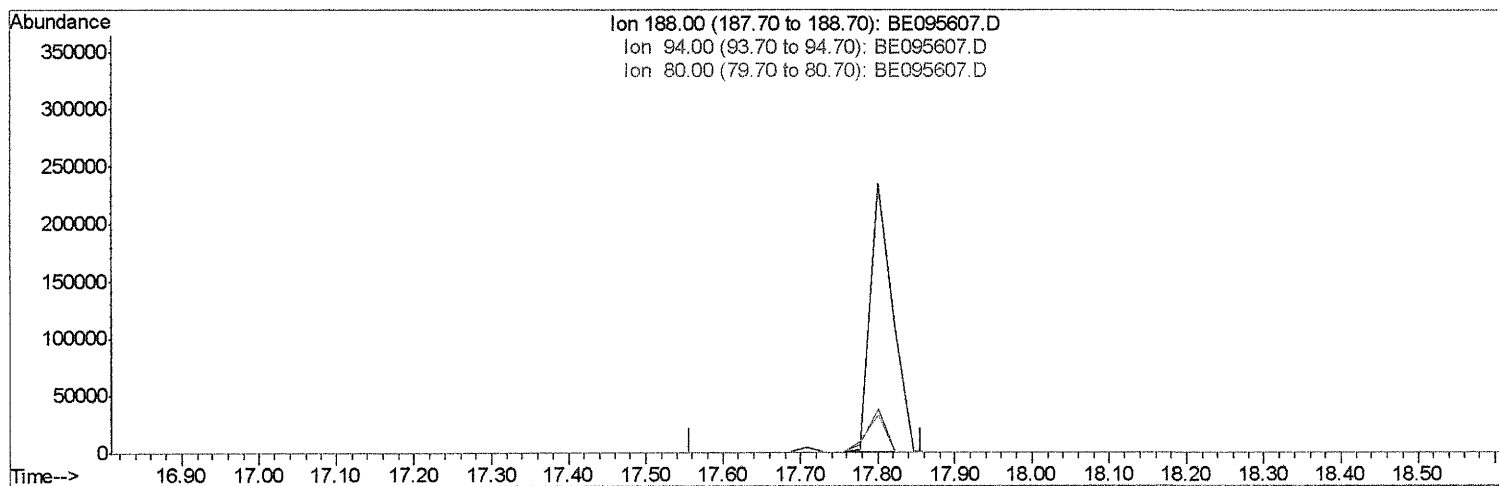

TIC: BE095607.D

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095607.D
 Acq On : 9 Feb 2018 14:48
 Operator : SJ/JU
 Sample : PB106255BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK55

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:40 AM

Quant Time: Feb 09 23:41:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 23:40:09 2018
 Response via : Initial Calibration

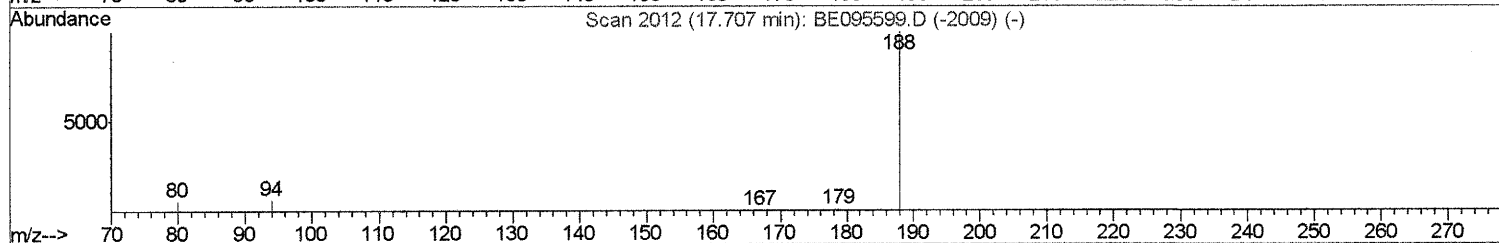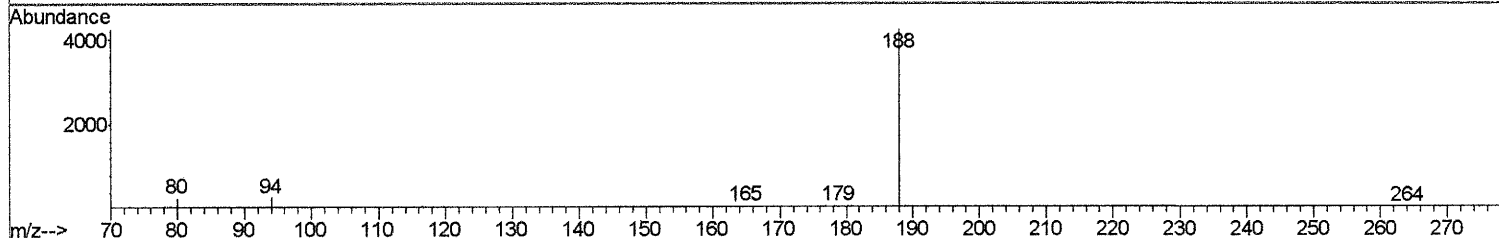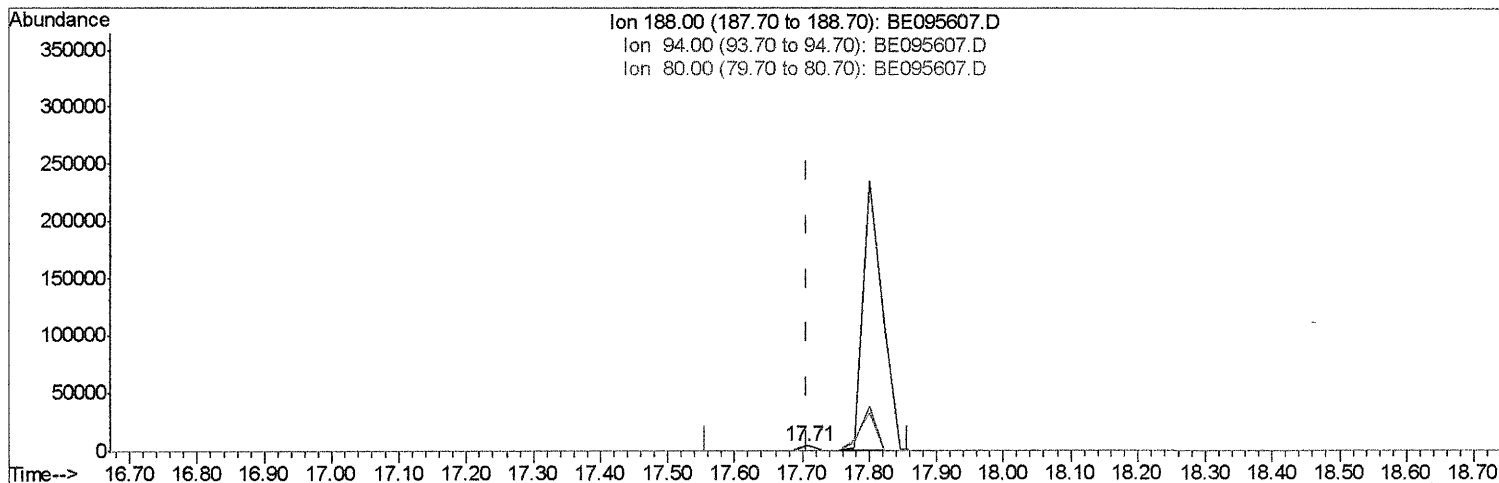

TIC: BE095607.D

(10) Phenanthrene-d10 (I)

17.708min (+0.001) 0.40ng/ul m> S1 2/13/18

response 6375

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.23#
80.00	11.80	5.92#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095607.D
 Acq On : 9 Feb 2018 14:48
 Operator : SJ/JU
 Sample : PB106255BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK55

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:40 AM

Quant Time: Feb 10 00:35:59 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 23:40:09 2018
 Response via : Initial Calibration

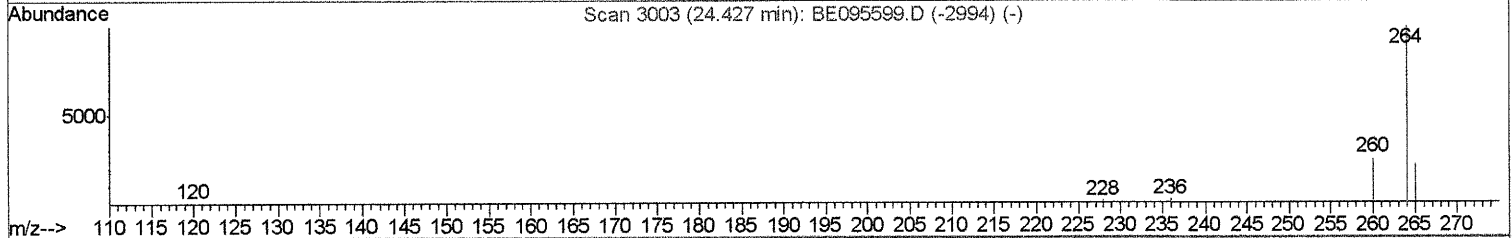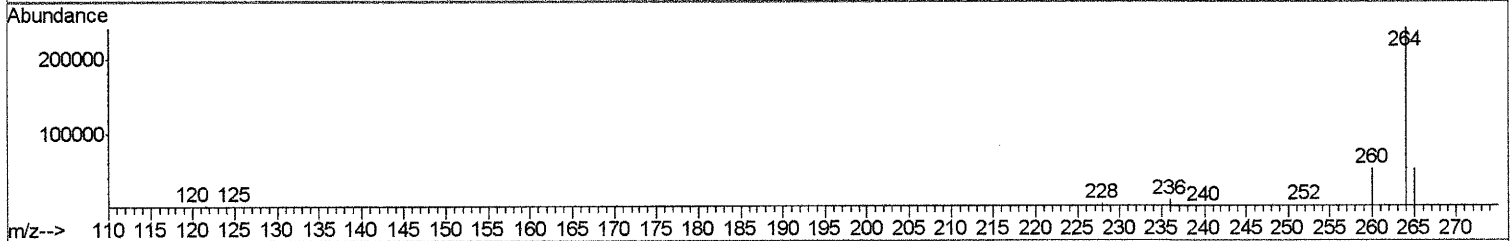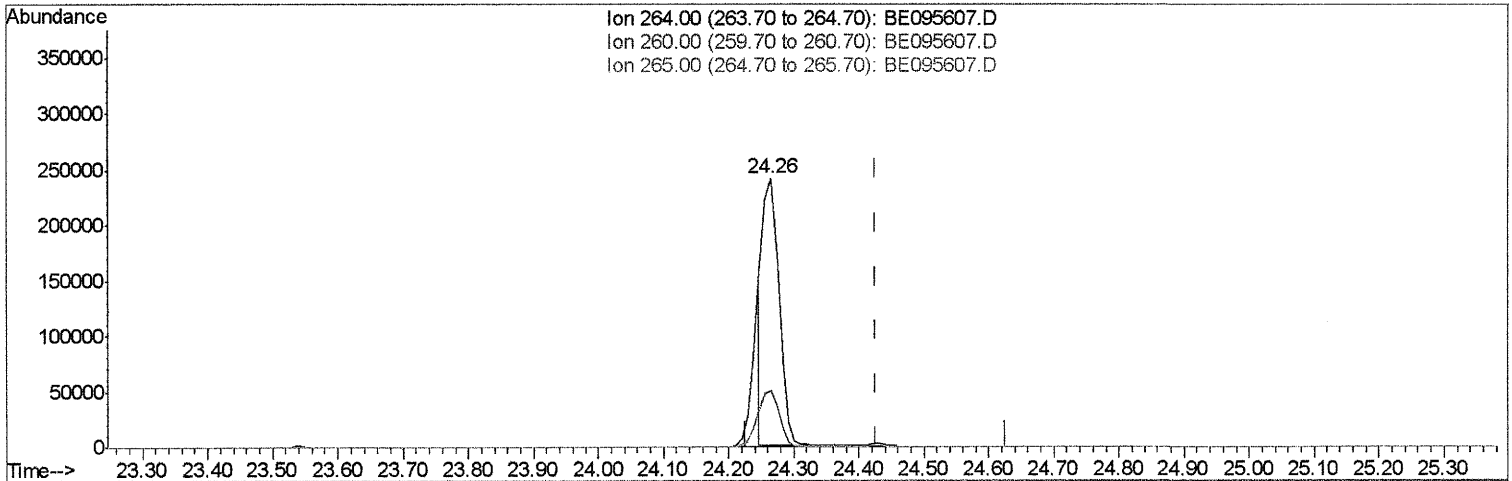

TIC: BE095607.D

(20) Perylene-d12 (I)

24.265min (-0.163) 0.40ng/ul

response 400041

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.07#
265.00	103.50	21.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095607.D
Acq On : 9 Feb 2018 14:48
Operator : SJ/JU
Sample : PB106255BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
SBLK55

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:40 AM

Quant Time: Feb 10 00:35:59 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

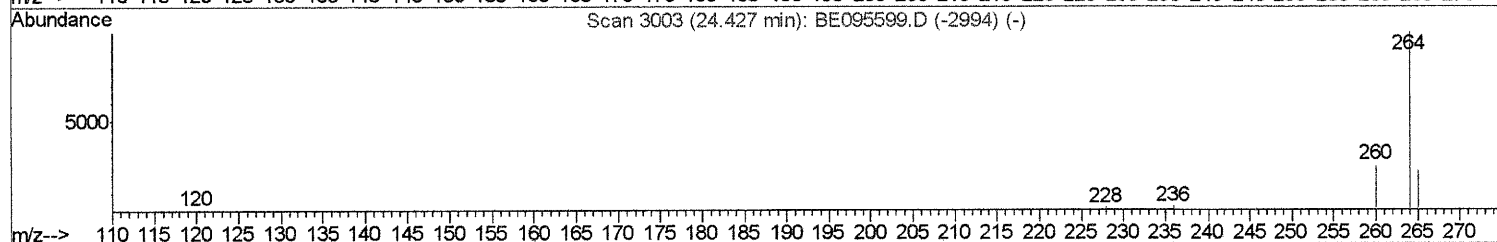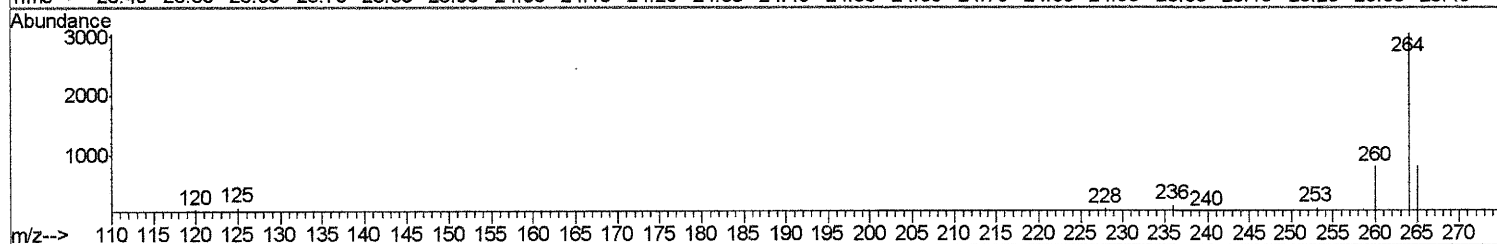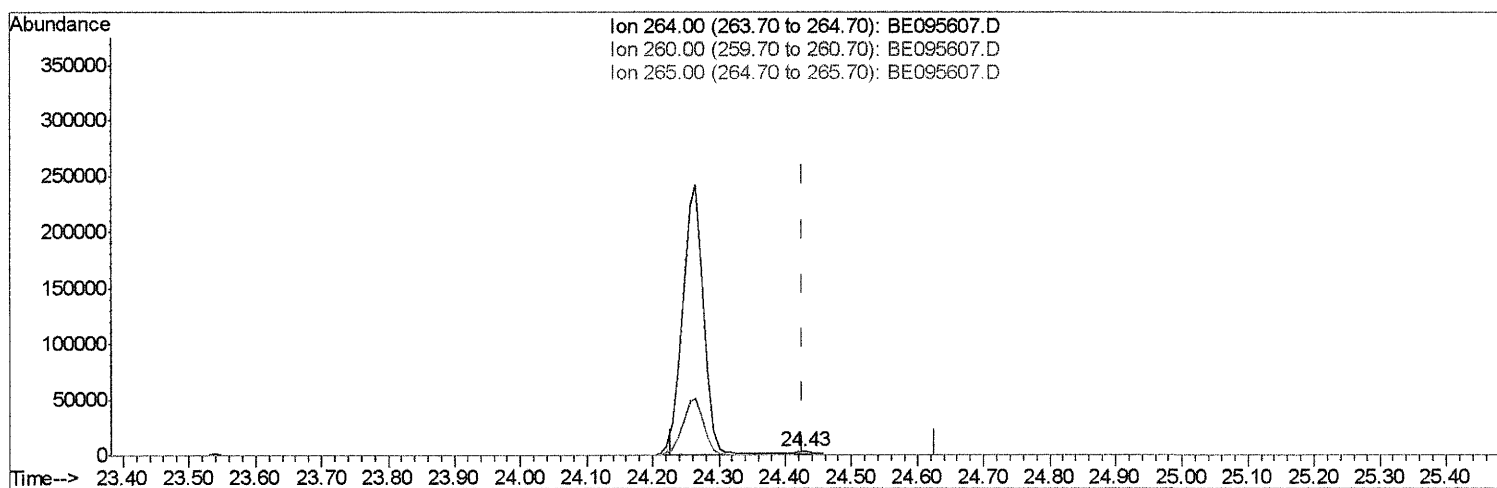

TIC: BE095607.D

(20) Perylene-d12 (I)

24.427min (-0.000) 0.40ng/ul m > 51 2/13/18

response 5514

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.83
265.00	103.50	26.23#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095607.D
Acq On : 9 Feb 2018 14:48
Operator : SJ/JU
Sample : PB106255BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:40 AM

Quant Time: Feb 10 00:36:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 23:40:09 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1506	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4125	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2701	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6375m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6082	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	5514m	0.40	ng/ul	0.00

} SJ 2/13/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2345	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7588	0.31	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed