


Data Path : Z:\HPCHEM1\BNA E\Data\BE020918\
Data File : BE095620.D
Acq On : 9 Feb 2018 22:34
Operator : SJ/JU
Sample : J1339-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D17

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:14 AM

Quant Time: Feb 10 01:52:13 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

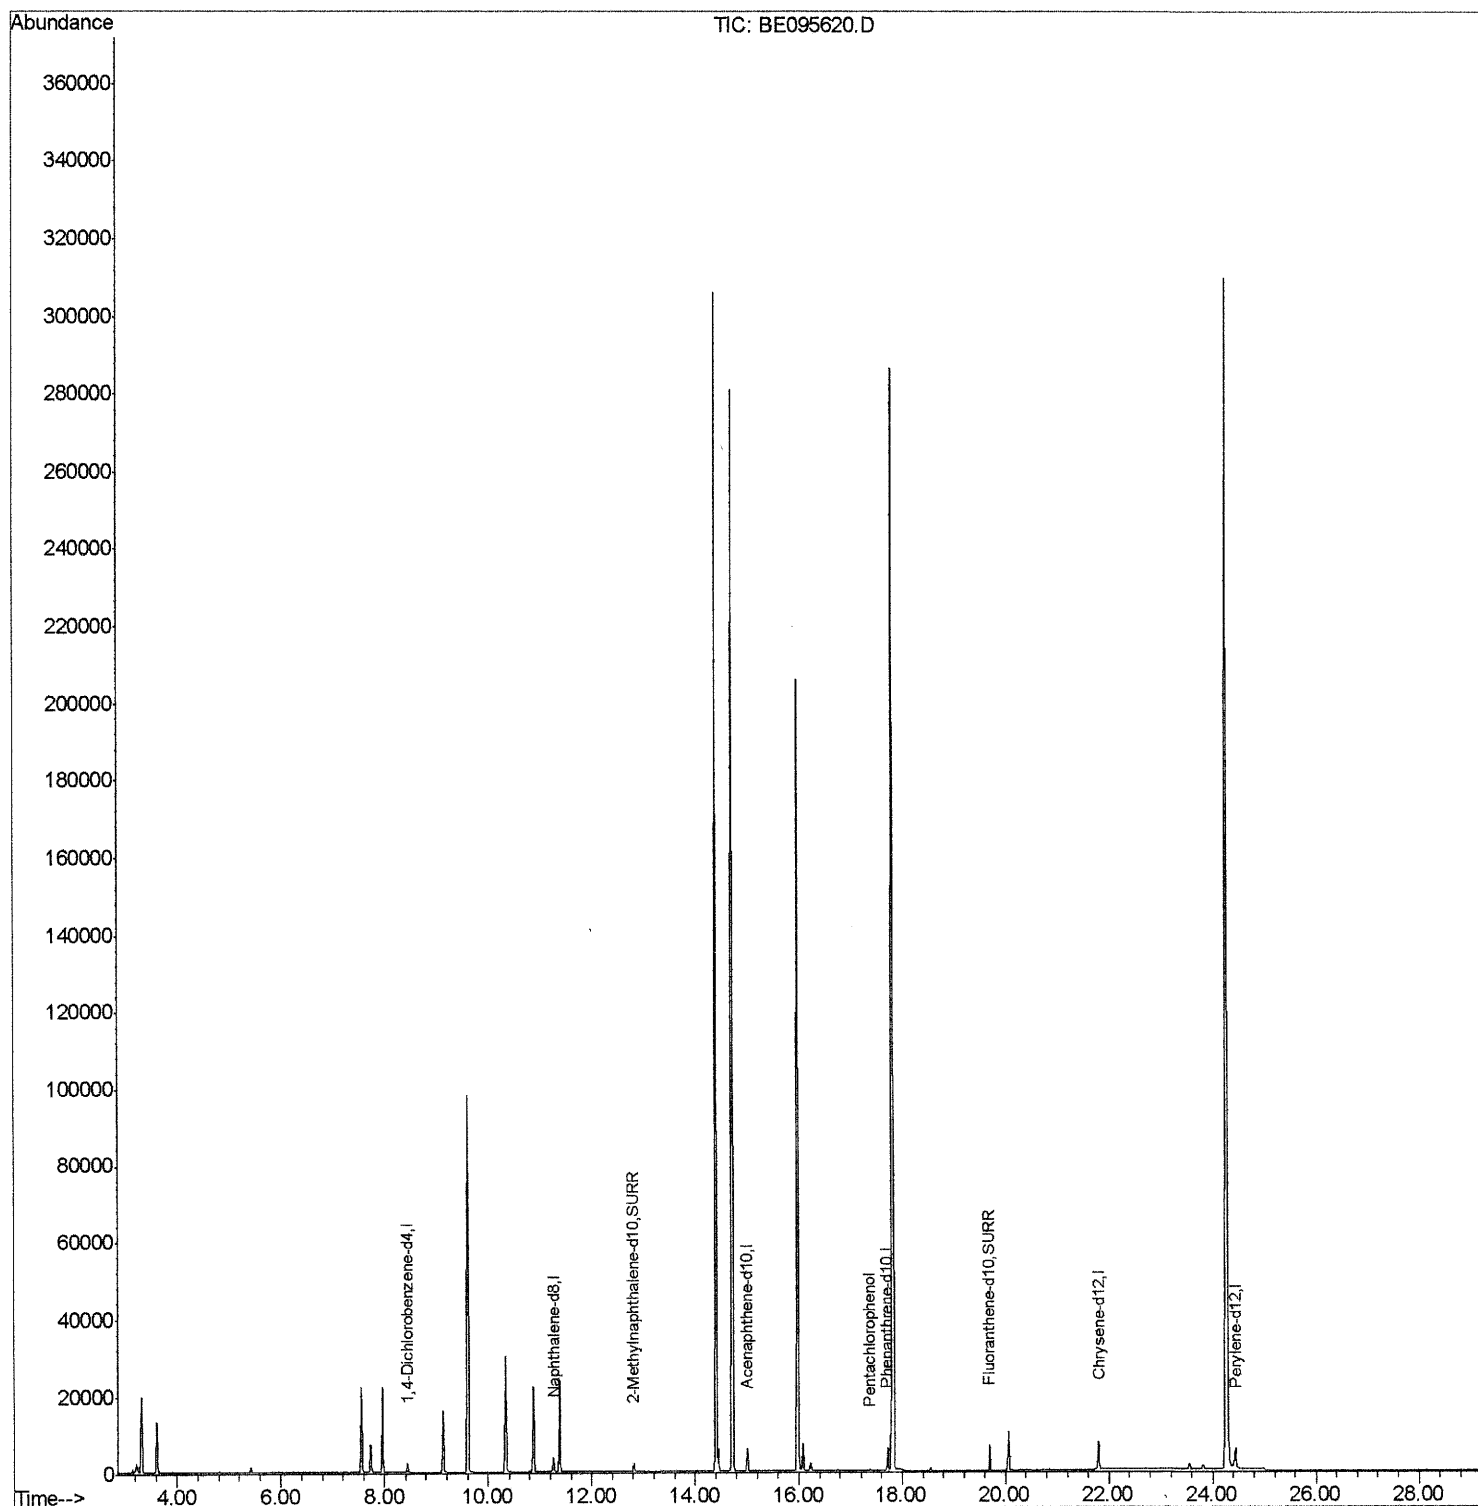




Data Path : Z:\HPCHEM1\BNA E\Data\BE020918\
Data File : BE095620.D
Acq On : 9 Feb 2018 22:34
Operator : SJ/JU
Sample : J1339-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D17

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:14 AM

Quant Time: Feb 10 00:58:19 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

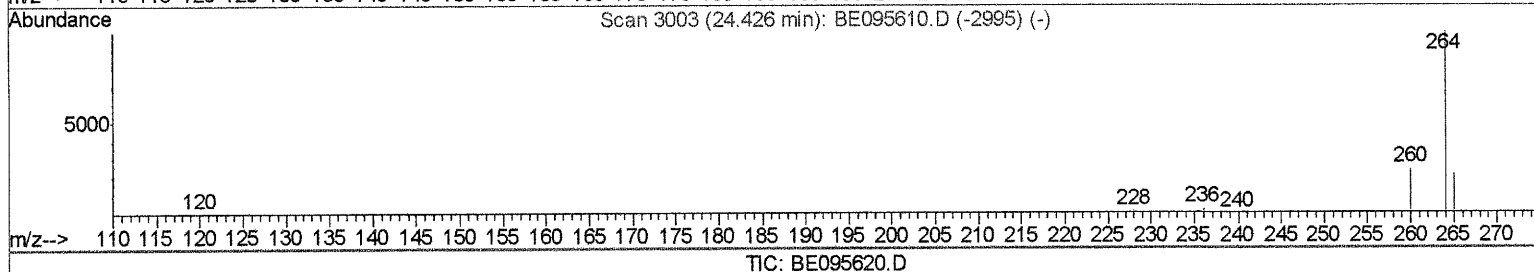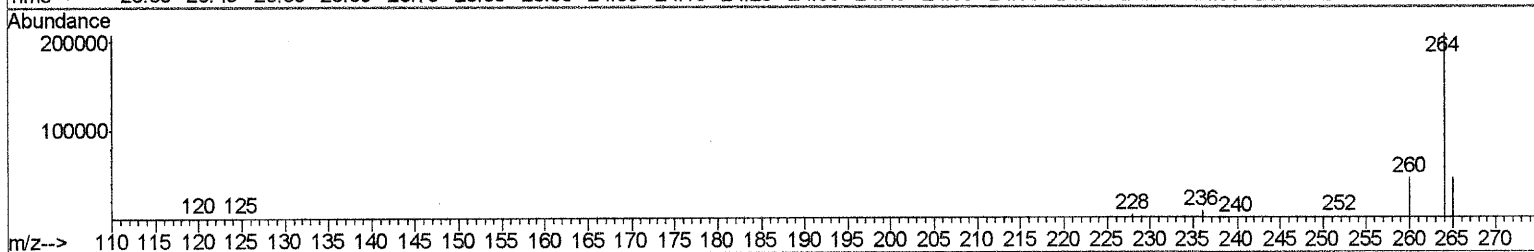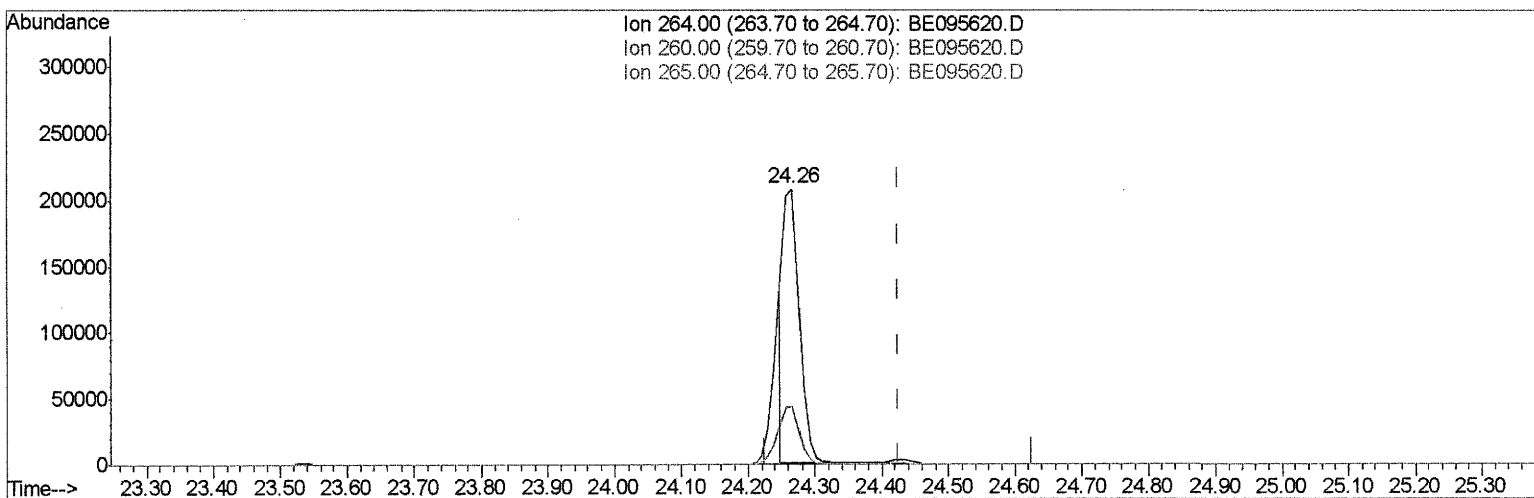

(20) Perylene-d12 (I)

24.265min (-0.161) 0.40ng/ul

response 345480

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.12#
265.00	103.50	21.50#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE020918\
Data File : BE095620.D
Acq On : 9 Feb 2018 22:34
Operator : SJ/JU
Sample : J1339-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6D17

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:14 AM

Quant Time: Feb 10 00:58:19 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

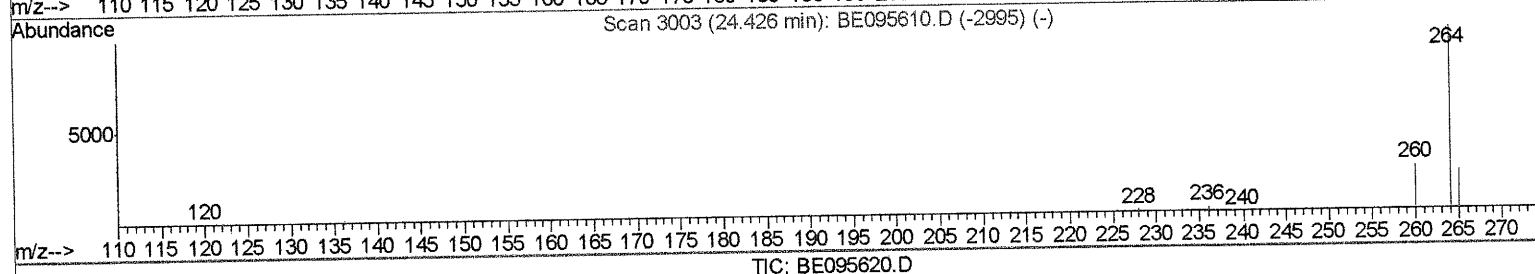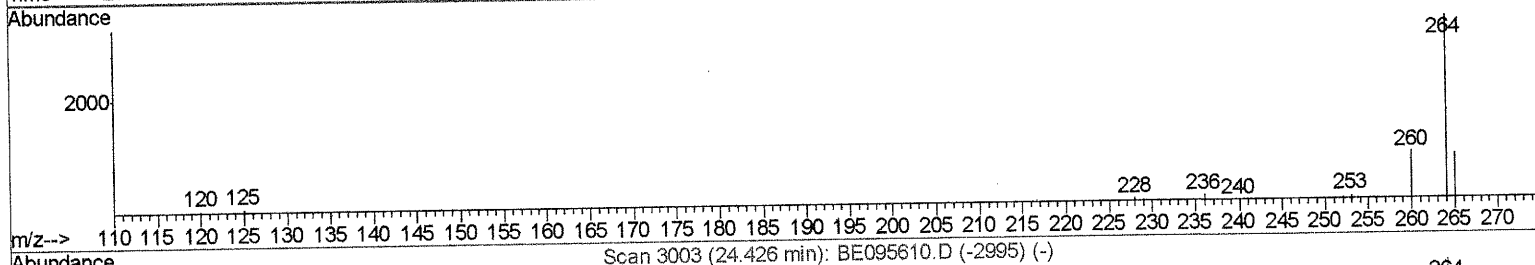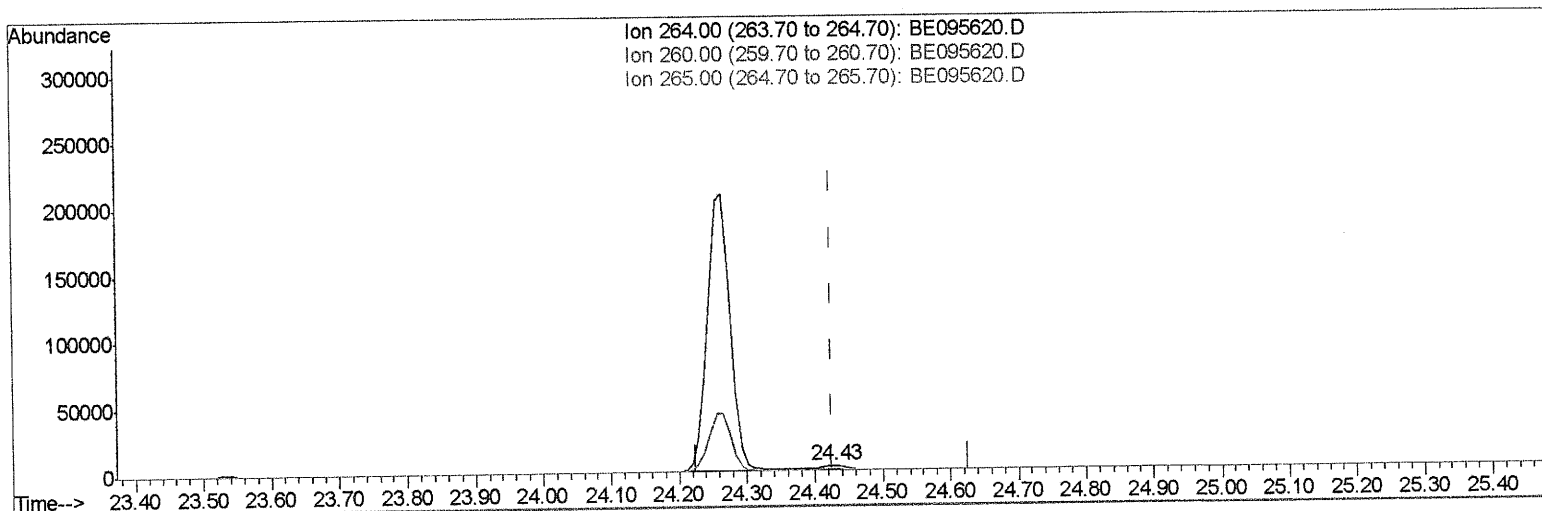

(20) Perylene-d12 (l)

24.427min (+0.001) 0.40ng/ul m

SJ 2/13/18

response 6284

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.21
265.00	103.50	25.35#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE020918\
 Data File : BE095620.D
 Acq On : 9 Feb 2018 22:34
 Operator : SJ/JU
 Sample : J1339-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D17

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:39:14 AM

Quant Time: Feb 10 01:52:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1708	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4810	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3156	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7412	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6826	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6284m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2546	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7020	0.25	ng/ul	0.00
Target Compounds						Ovalue
11) Pentachlorophenol	17.36	266	225	0.157	ng/ul	99

SI 2/13/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed