

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095624.D
Acq On : 10 Feb 2018 00:57
Operator : SJ/JU
Sample : J1339-13
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D22

Manual Integrations
APPROVED

Sohil

2/12/2018 11:39:25 AM

Quant Time: Feb 10 02:49:50 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

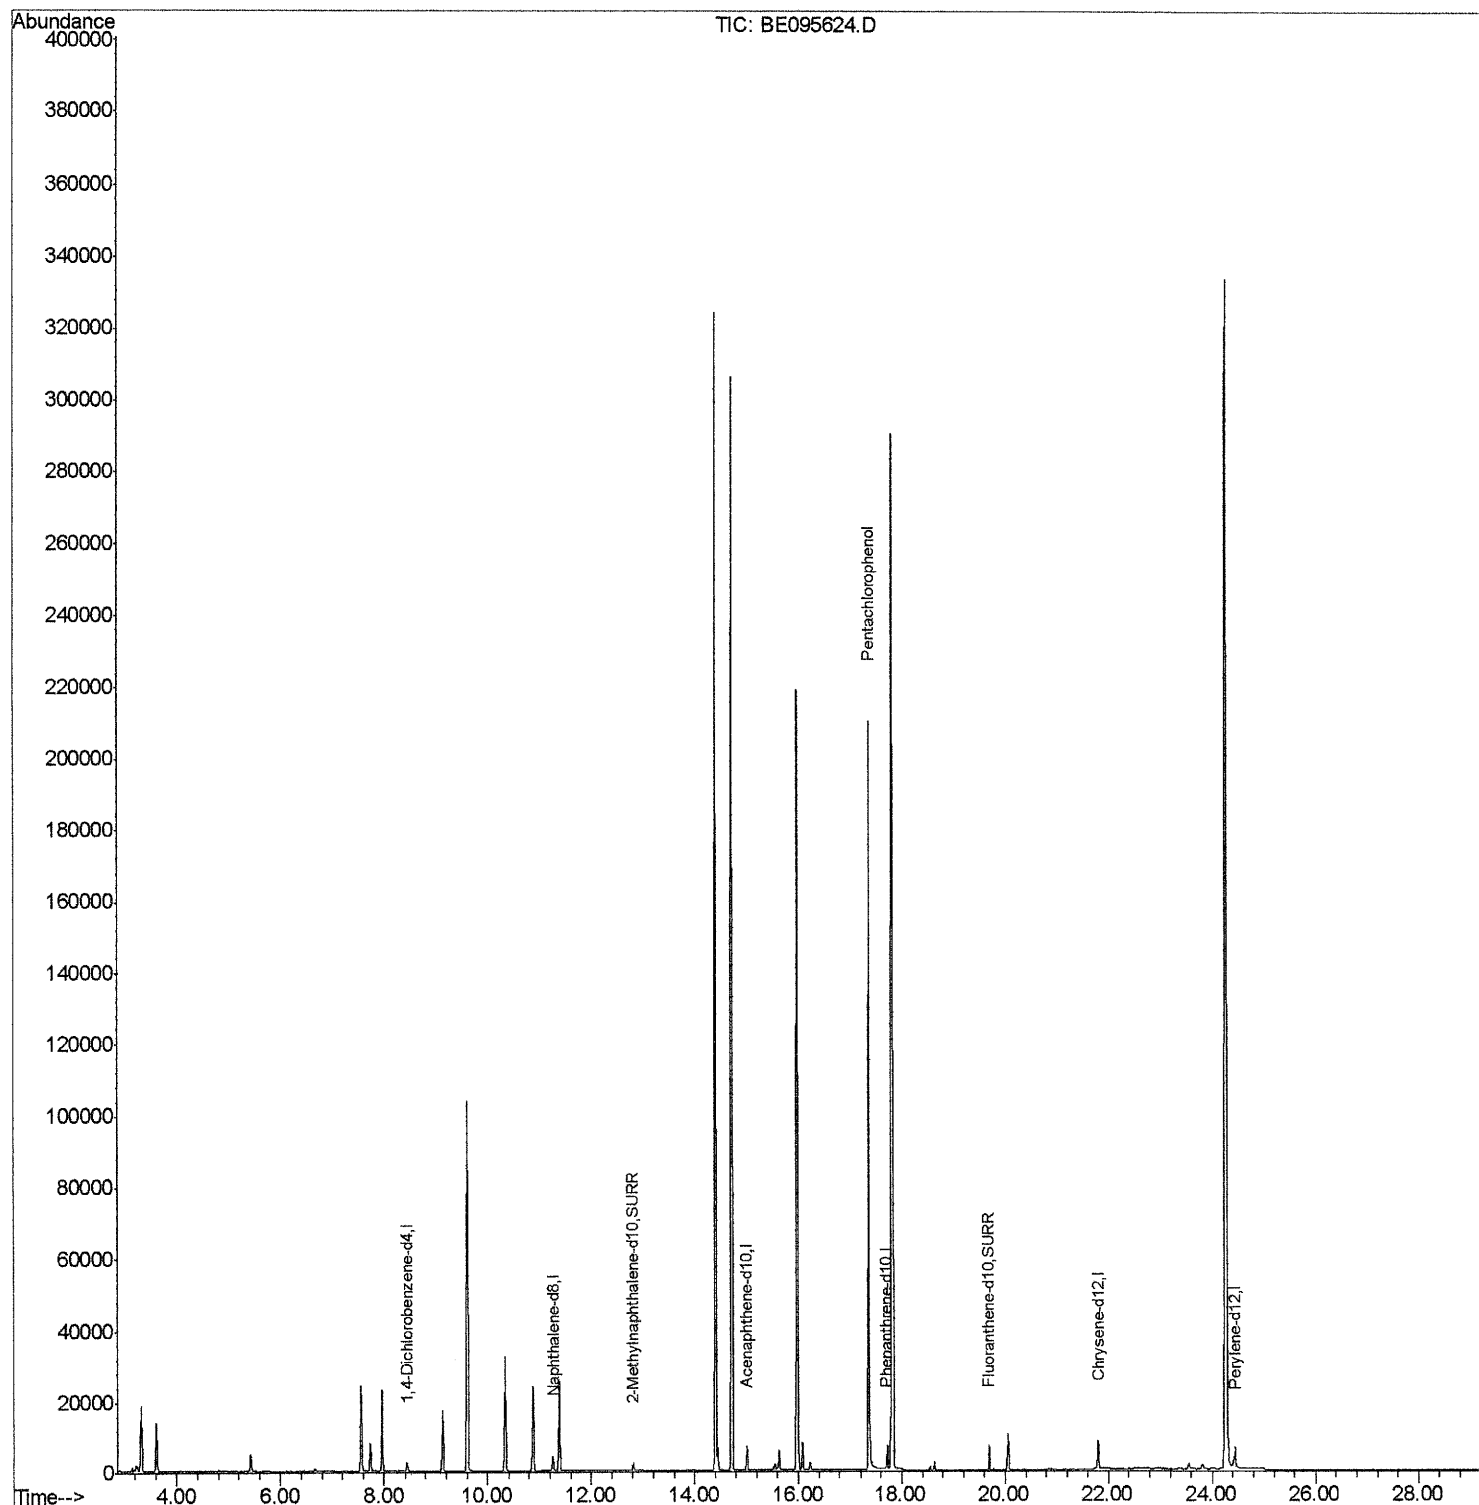

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095624.D
Acq On : 10 Feb 2018 00:57
Operator : SJ/JU
Sample : J1339-13
Misc :
ALS Vial : 26 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
F6D22

Manual Integrations
APPROVED

Sohil

2/12/2018 11:39:25 AM

Quant Time: Feb 10 02:01:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

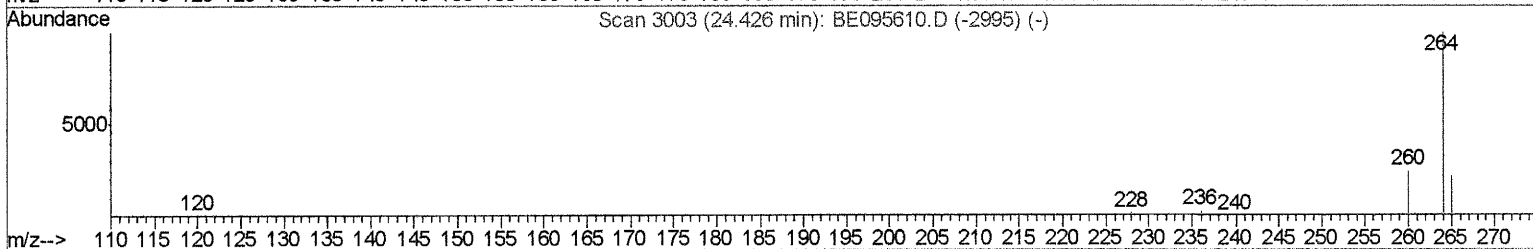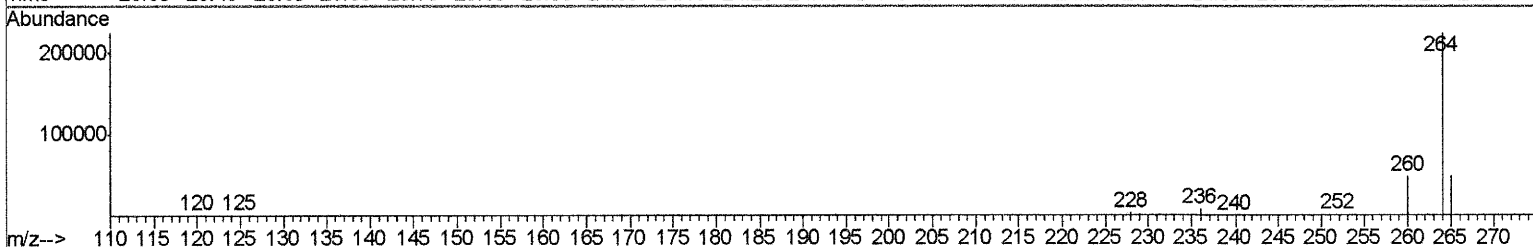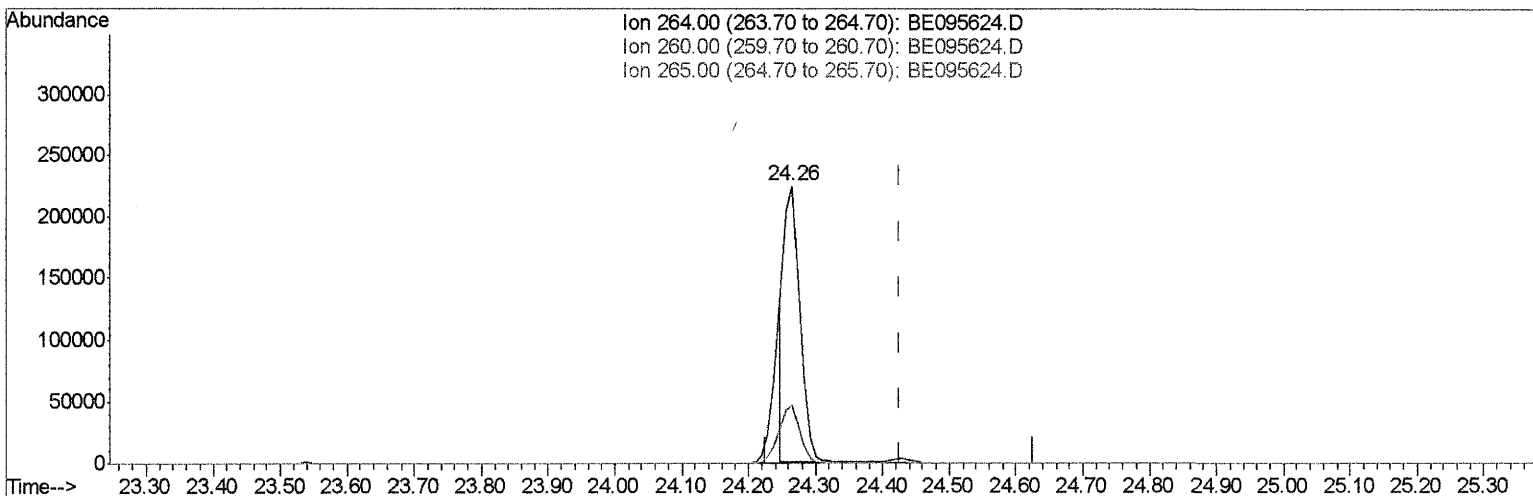

TIC: BE095624.D

(20) Perylene-d12 (I)

24.264min (-0.162) 0.40ng/ui

response 370669

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.09#
265.00	103.50	21.40#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
 Data File : BE095624.D
 Acq On : 10 Feb 2018 00:57
 Operator : SJ/JU
 Sample : J1339-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1




Instrument :
 BNA_E
 ClientSampleId :
 F6D22

Manual Integrations
 APPROVED

Sohil

2/12/2018 11:39:25 AM

Quant Time: Feb 10 02:01:12 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration

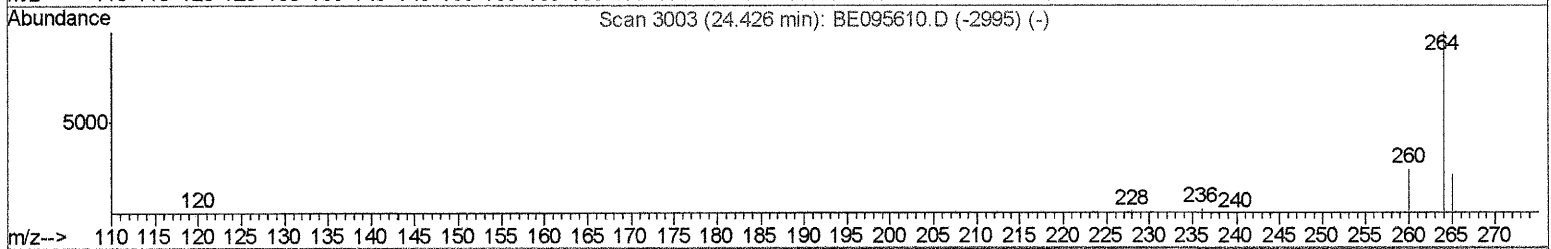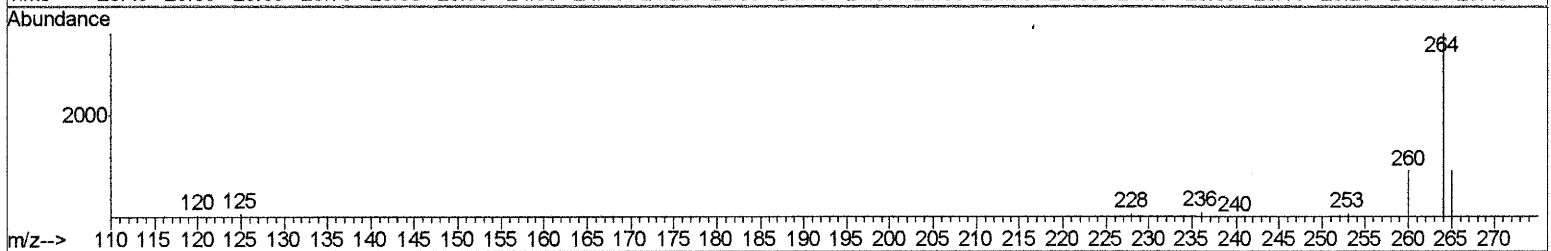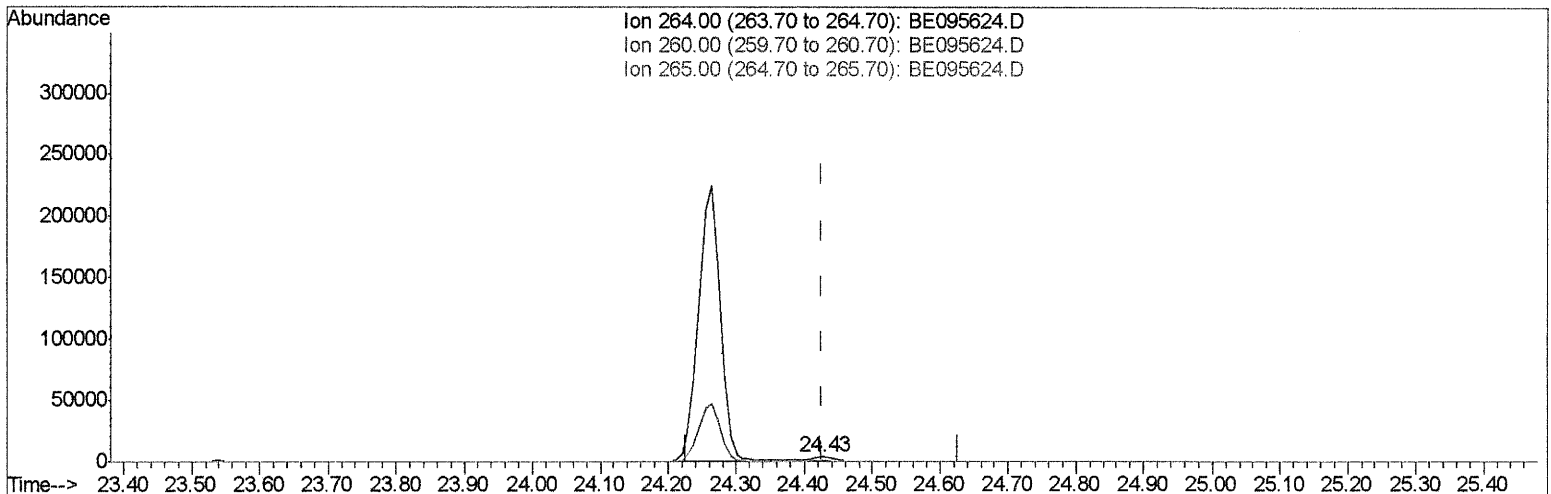

TIC: BE095624.D

(20) Perylene-d12 (I)

24.427min (+0.000) 0.40ng/ul m

SJ 2/13/18

response 6920

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.61
265.00	103.50	25.75#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095624.D
Acq On : 10 Feb 2018 00:57
Operator : SJ/JU
Sample : J1339-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D22

Manual Integrations
APPROVED

Sohil

2/12/2018 11:39:25 AM

Quant Time: Feb 10 02:49:50 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1878	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5510	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3558	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8492	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7648	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6920m	0.40	ng/ul	0.00

SJ 2/13/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2696	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7288	0.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
11) Pentachlorophenol	17.36	266	124003	75.391	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed