


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095632.D
Acq On : 10 Feb 2018 5:58
Operator : SJ/JU
Sample : J1339-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C94

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:50 AM

Quant Time: Feb 12 01:01:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

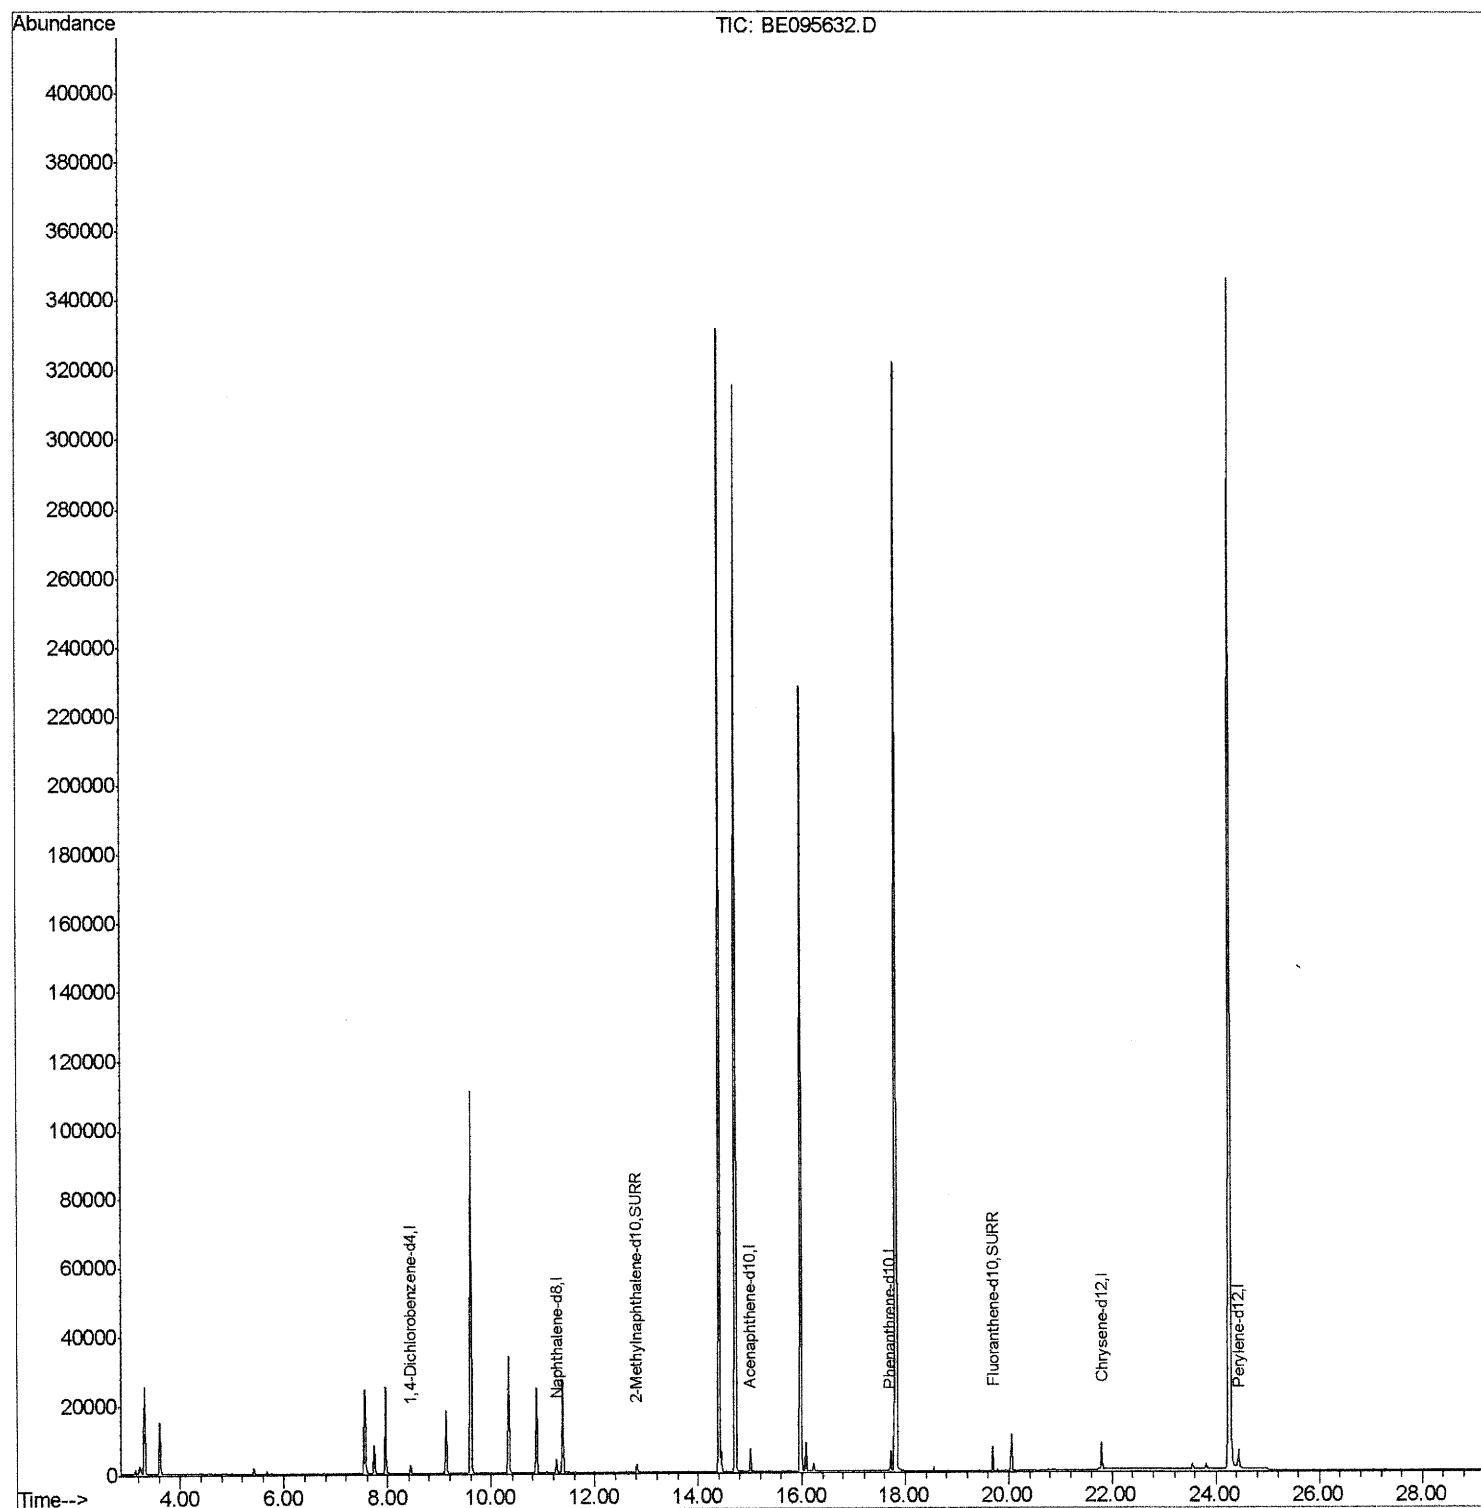




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095632.D
Acq On : 10 Feb 2018 5:58
Operator : SJ/JU
Sample : J1339-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C94

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:50 AM

Quant Time: Feb 12 00:20:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

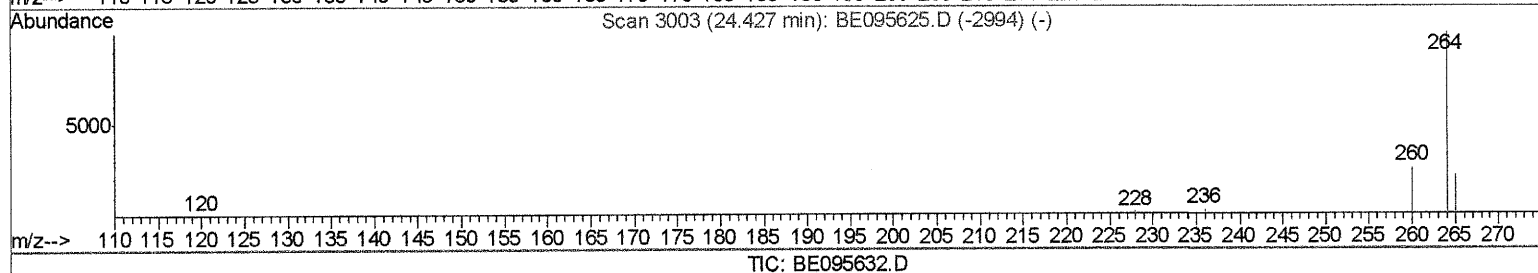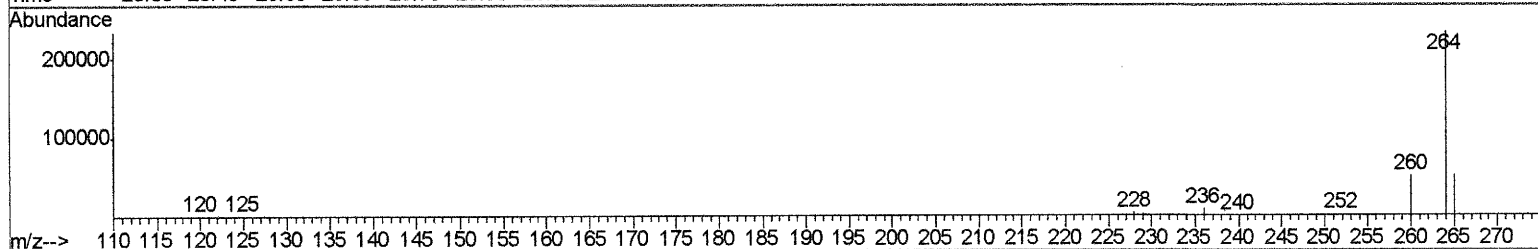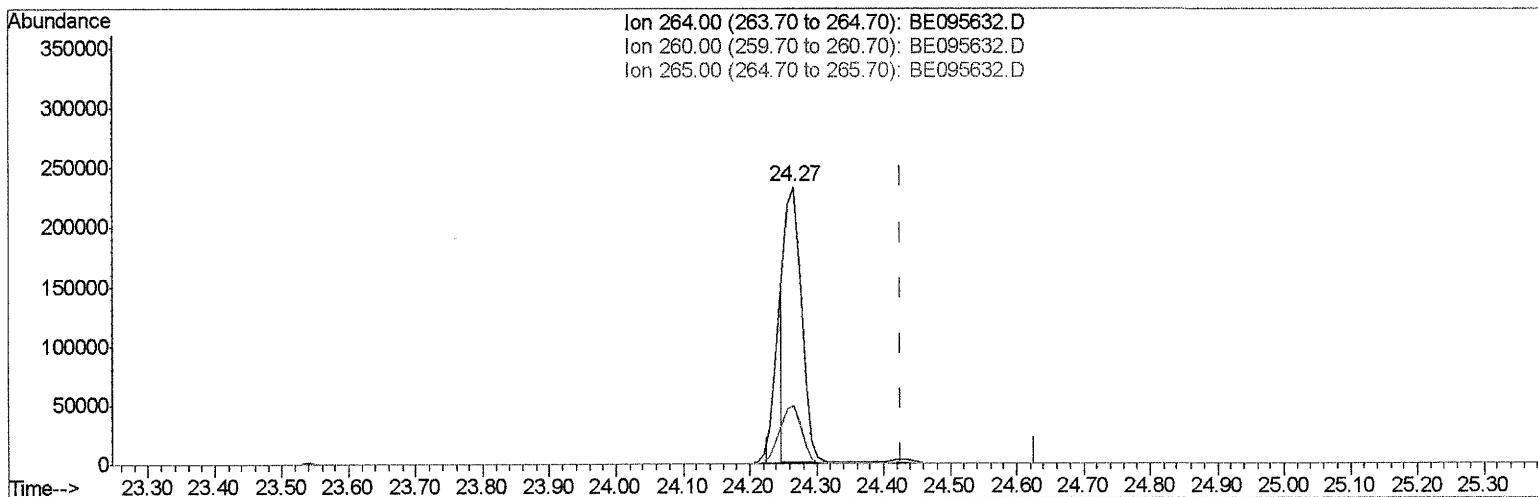

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 381917

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.99#
265.00	103.50	21.50#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095632.D
Acq On : 10 Feb 2018 5:58
Operator : SJ/JU
Sample : J1339-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C94

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:50 AM

Quant Time: Feb 12 00:20:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

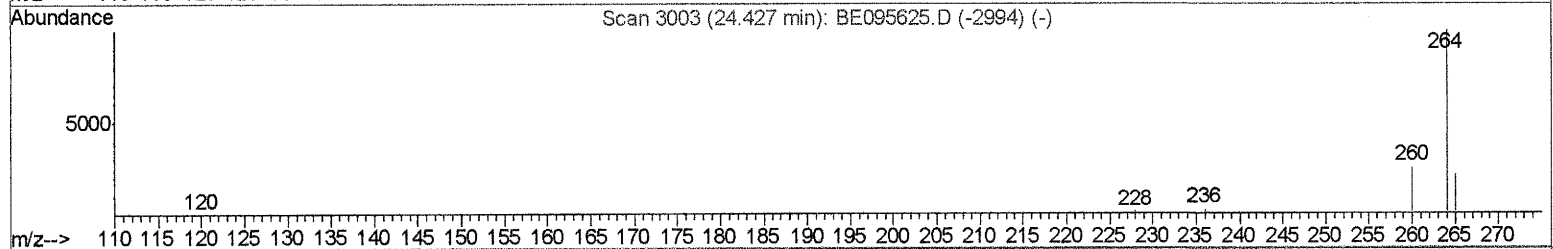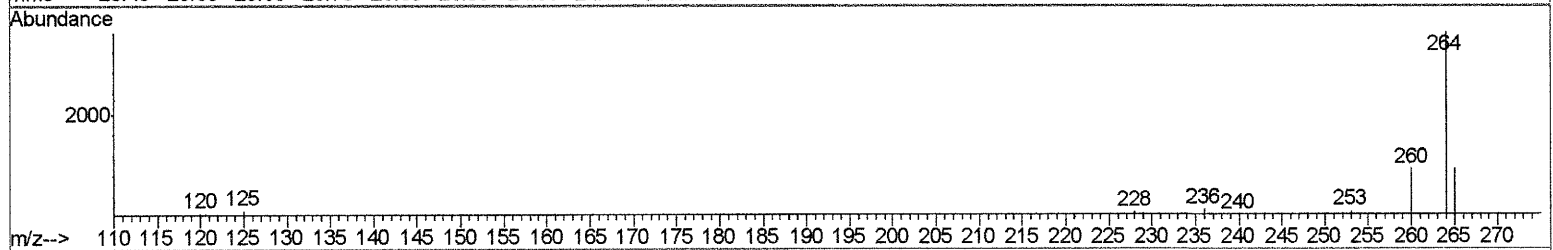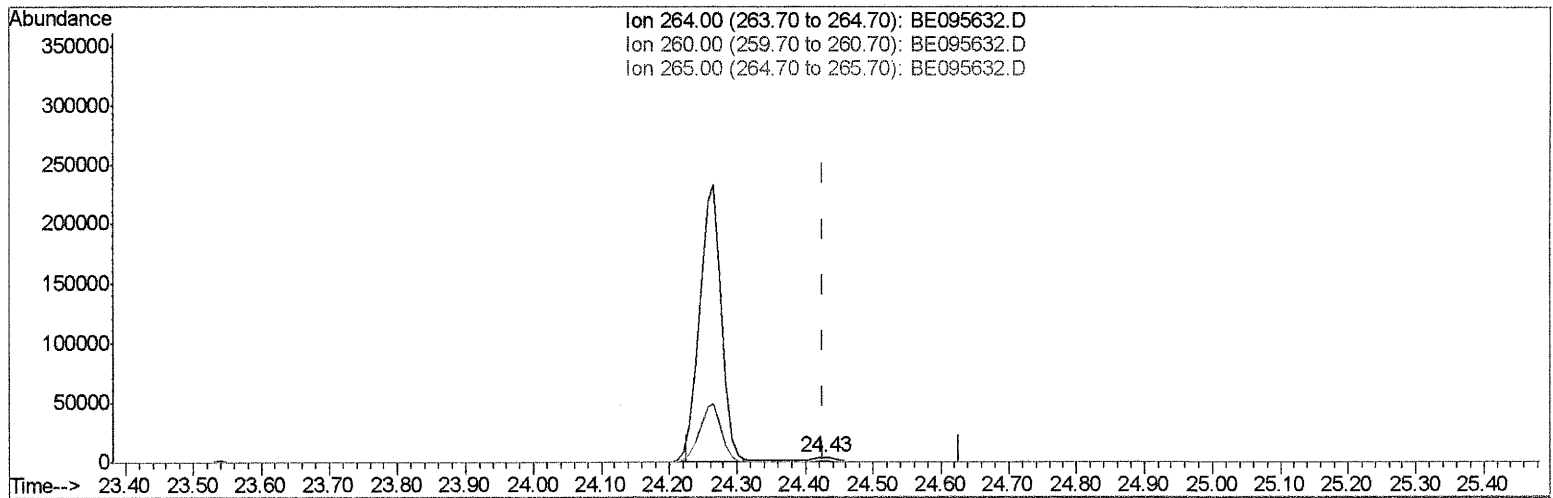

TIC: BE095632.D

(20) Perylene-d12 (I)

24.427min (+0.000) 0.40ng/ul m

SJ 2/13/18

response 6783

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.59
265.00	103.50	25.73#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095632.D
Acq On : 10 Feb 2018 5:58
Operator : SJ/JU
Sample : J1339-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C94

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:50 AM

Quant Time: Feb 12 01:01:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1742	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5143	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3328	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7824	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7263	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6783m	0.40	ng/ul	0.00

SJ 2/13/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2879	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7790	0.26	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed