


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095637.D
Acq On : 10 Feb 2018 8:54
Operator : SJ/JU
Sample : J1355-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D52

Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:24 AM

Quant Time: Feb 12 01:20:26 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

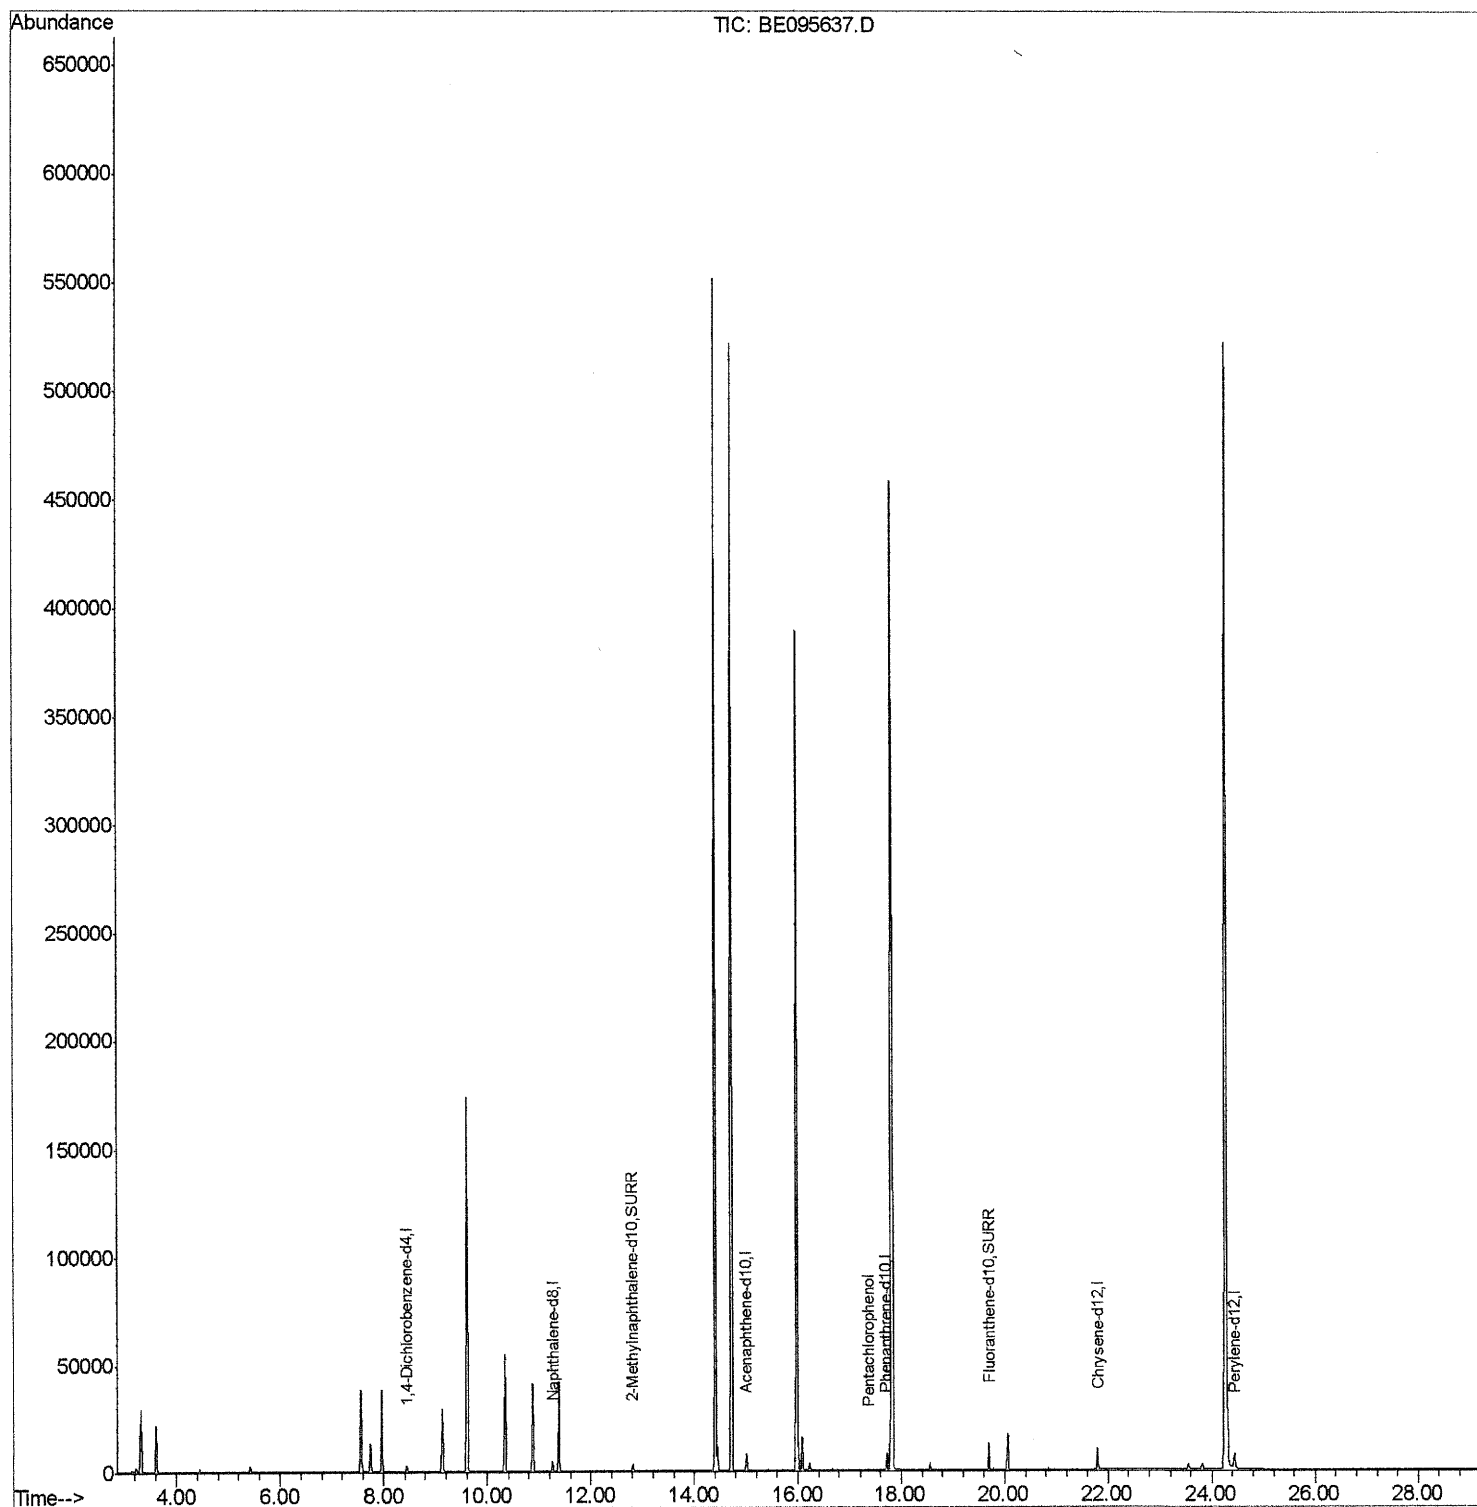




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095637.D
Acq On : 10 Feb 2018 8:54
Operator : SJ/JU
Sample : J1355-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D52

Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:24 AM

Quant Time: Feb 12 00:20:38 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

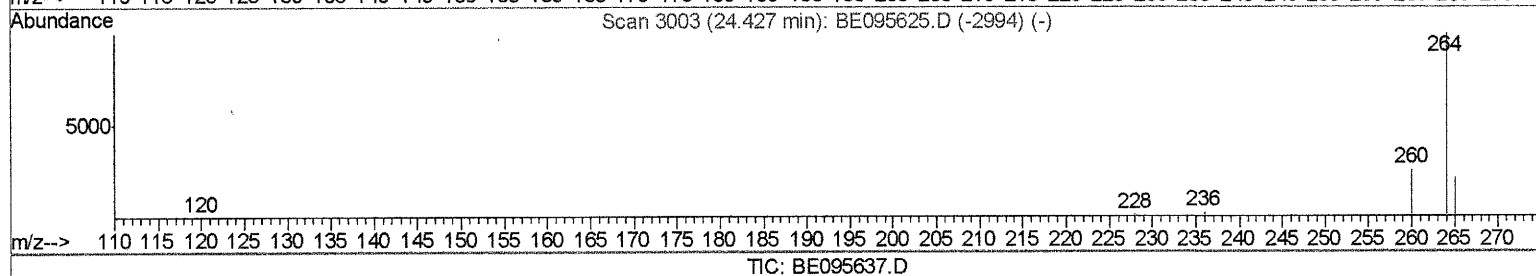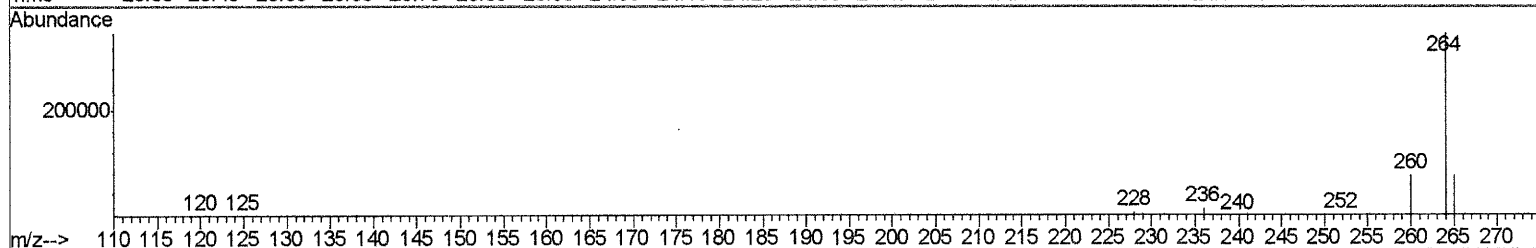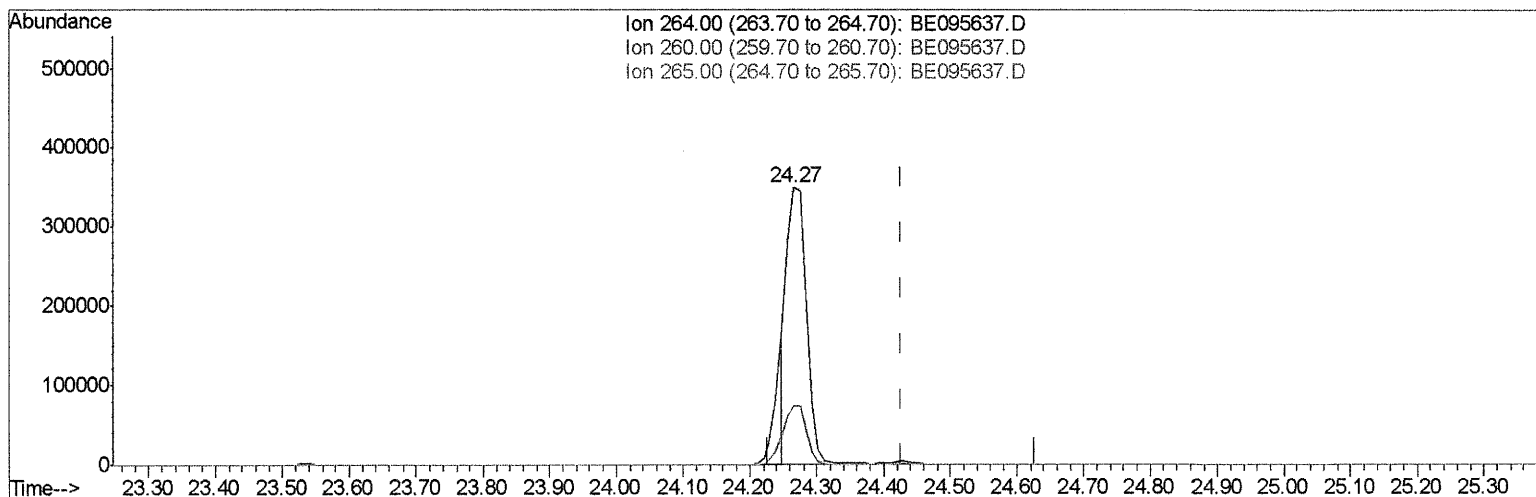

(20) Perylene-d12 (I)

24.265min (-0.162) 0.40ng/ul

response 702976

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.45#
265.00	103.50	21.41#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095637.D
Acq On : 10 Feb 2018 8:54
Operator : SJ/JU
Sample : J1355-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D52

Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:24 AM

Quant Time: Feb 12 01:19:36 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

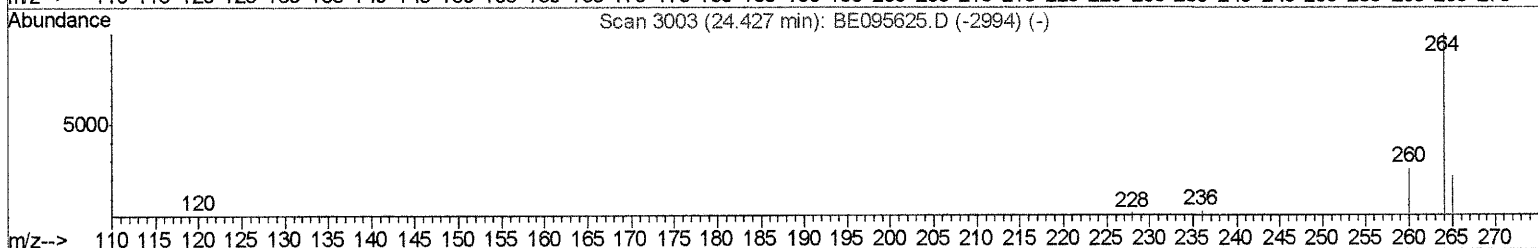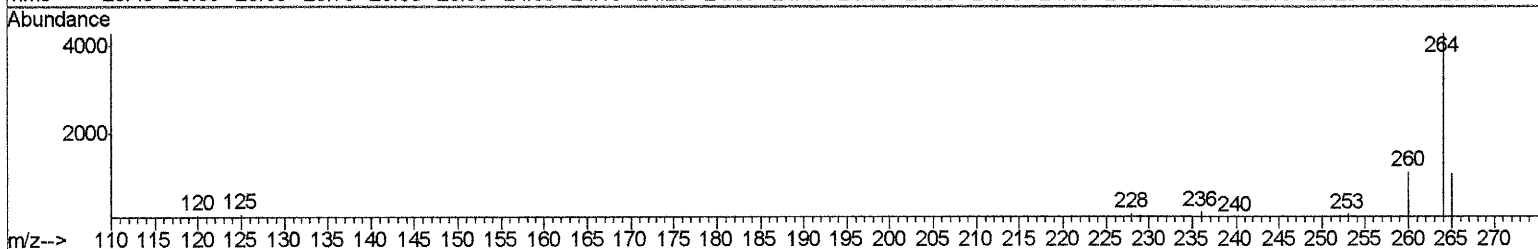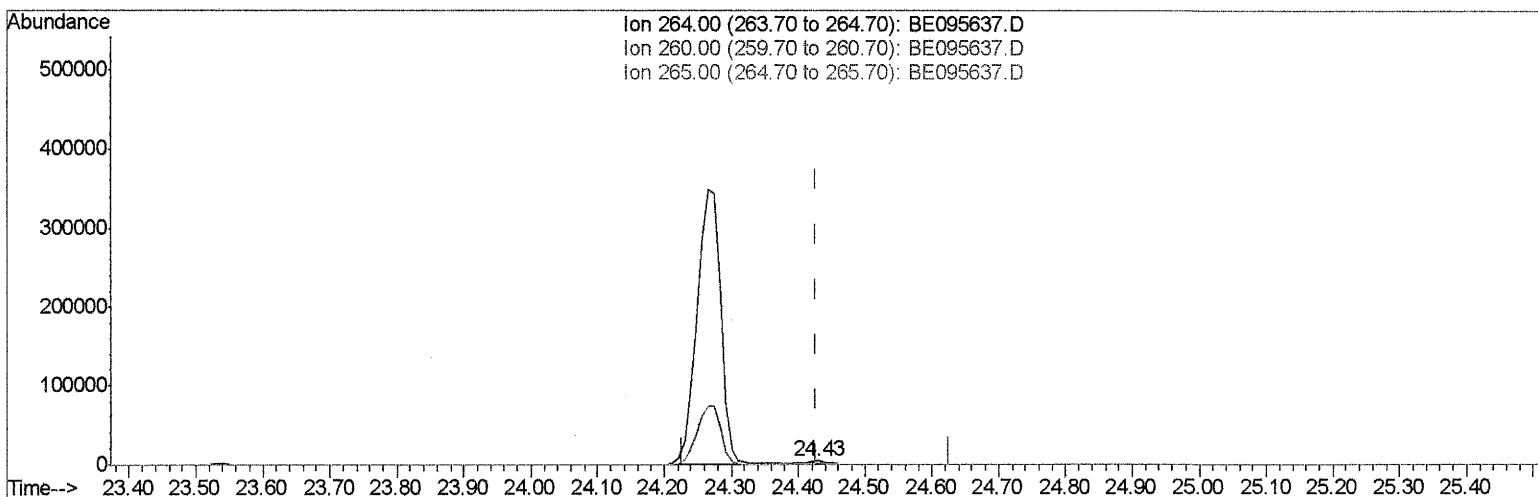

TIC: BE095637.D

(20) Perylene-d12 (I)

24.427min (+0.000) 0.40ng/ul m

SJ 2/13/18

response 8050

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.24
265.00	103.50	24.40#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020918\
Data File : BE095637.D
Acq On : 10 Feb 2018 8:54
Operator : SJ/JU
Sample : J1355-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D52

Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:24 AM

Quant Time: Feb 12 01:20:26 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2039	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	6299	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4300	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9879	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8719	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8050m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4559	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	12824	0.34	ng/ul	0.00
Target Compounds						Ovalue
11) Pentachlorophenol	17.36	266	322	0.168	ng/ul	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SI 2/13/18