

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095611.D
 Acq On : 9 Feb 2018 17:11
 Operator : SJ/JU
 Sample : J1339-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D49

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:50 AM

Quant Time: Feb 10 01:06:31 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1552	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4431	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3039	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7188m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6216	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	5549m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2918	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8122	0.30	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.30	128	338	0.027	ng/ul#	53
8) Acenaphthene	15.06	153	1321	0.116	ng/ul#	26

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095611.D
Acq On : 9 Feb 2018 17:11
Operator : SJ/JU
Sample : J1339-19
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D49

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:50 AM

Quant Time: Feb 10 01:06:31 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

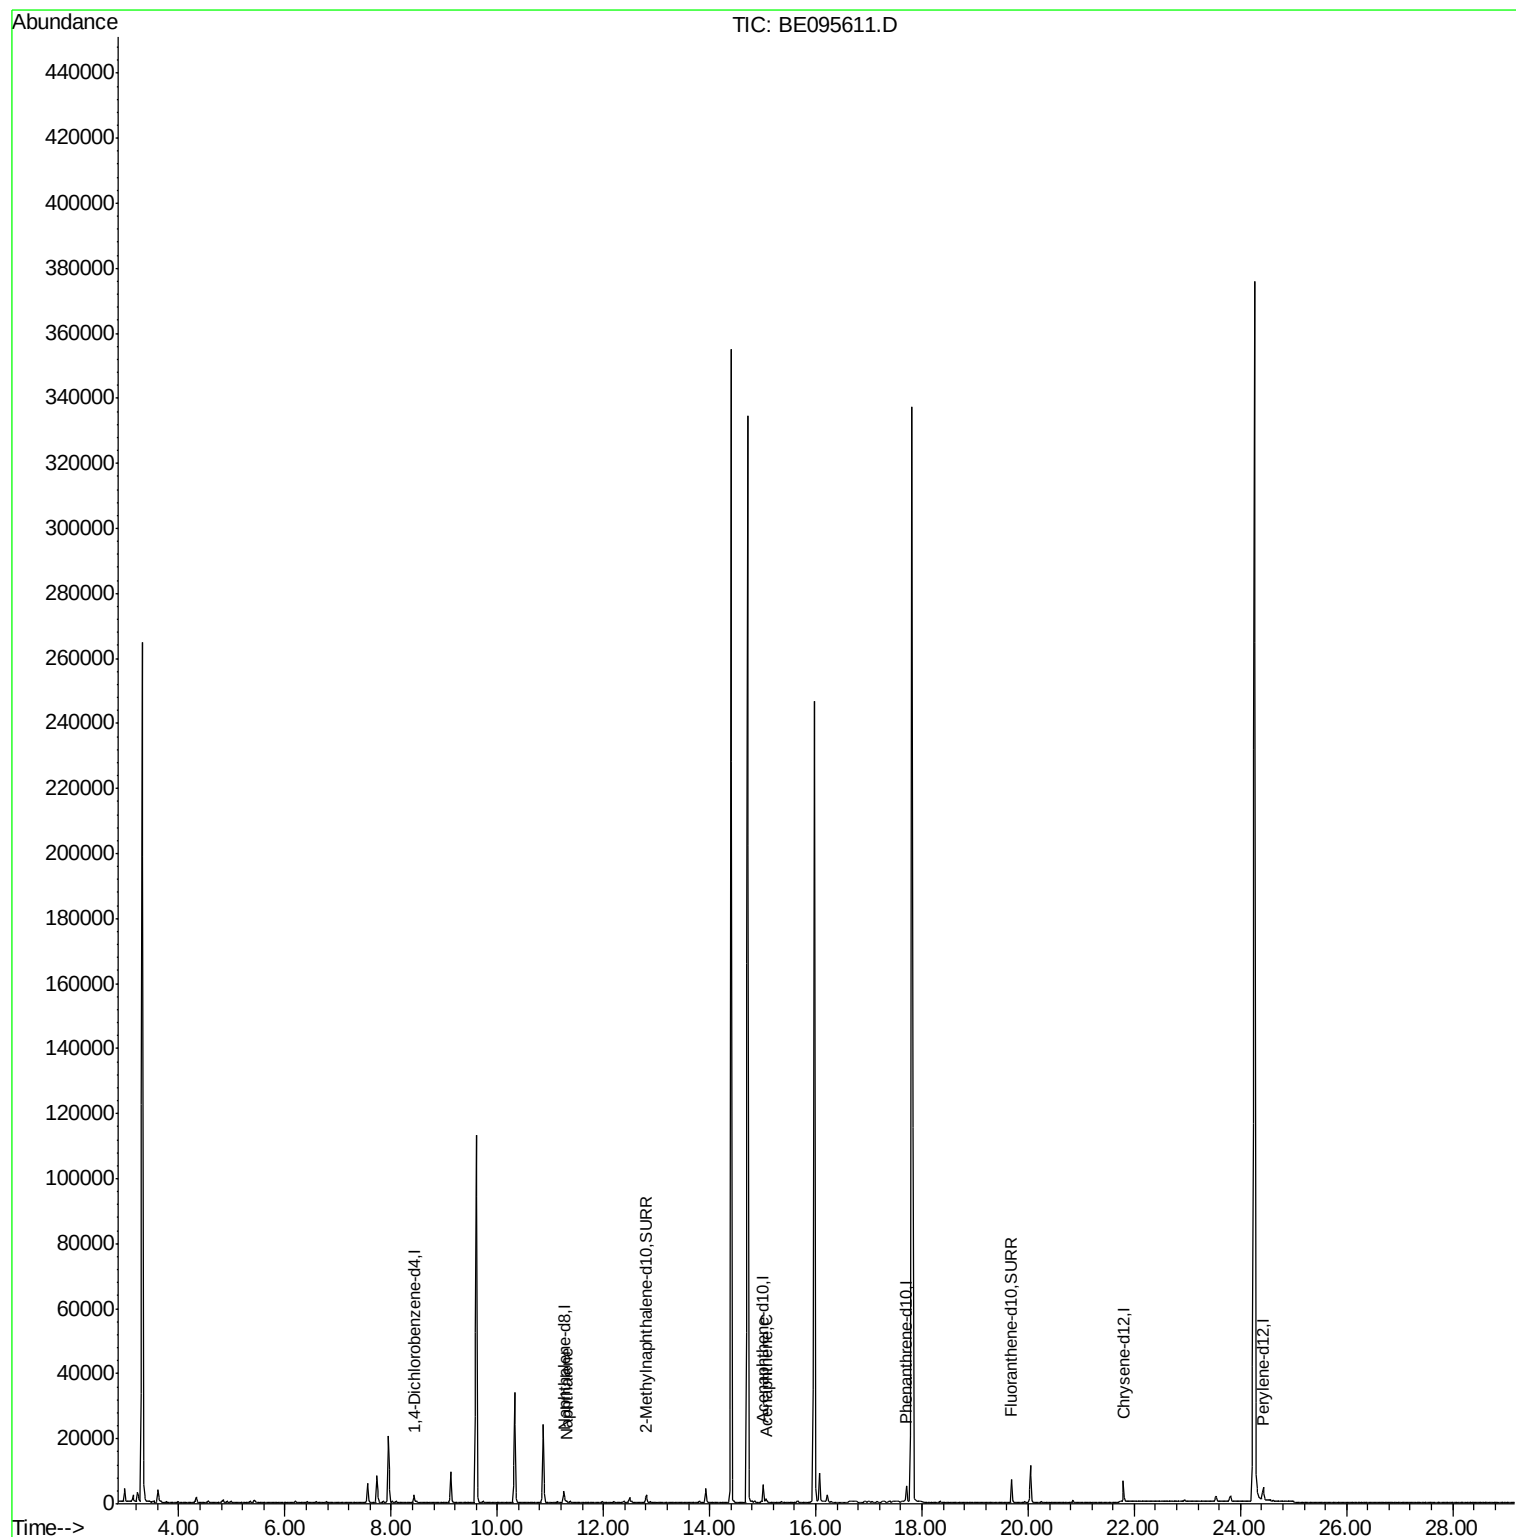

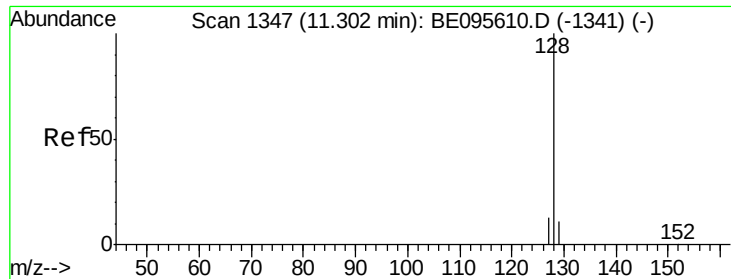

#3

Naphthalene

Concen: 0.027 ng/ul

RT: 11.30 min Scan# 1347

Delta R.T. -0.00 min

Lab File: BE095611.D

Acq: 9 Feb 2018 17:11

Instrument :

BNA_E





ClientSampled :

F6D49

Tgt Ion:	128	Resp:	338
Ion Ratio	Lower	Upper	
128	100		
129	29.3	11.3	16.9#
127	29.8	4.0	6.0#

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:50 AM

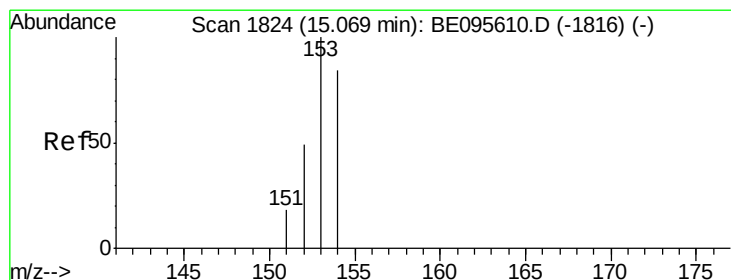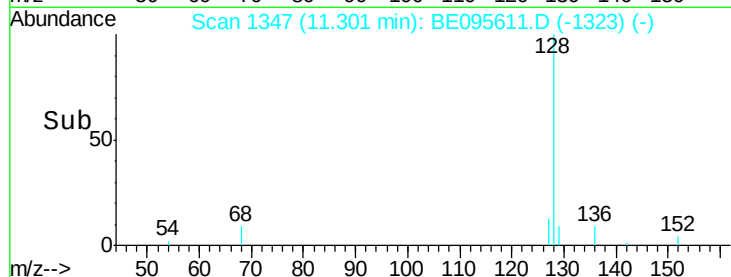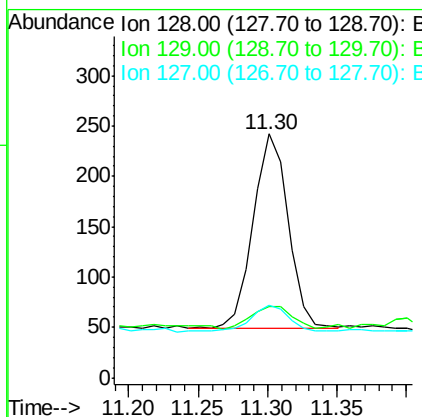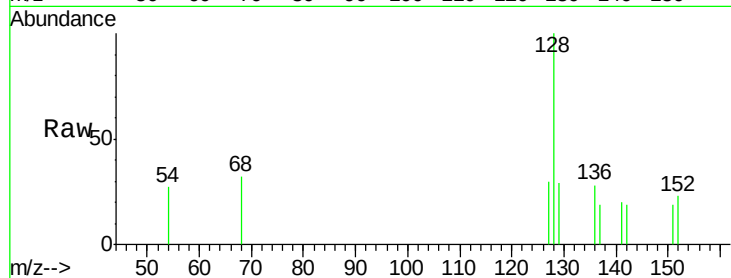

#8

Acenaphthene

Concen: 0.116 ng/ul

RT: 15.06 min Scan# 1823

Delta R.T. -0.01 min

Lab File: BE095611.D

Acq: 9 Feb 2018 17:11

Tgt Ion:	153	Resp:	1321
Ion Ratio	Lower	Upper	
153	100		
152	6.7	36.0	54.0#
154	13.6	72.0	108.0#

