

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095613.D
 Acq On : 9 Feb 2018 18:23
 Operator : SJ/JU
 Sample : J1355-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D28

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:56 AM

Quant Time: Feb 10 01:23:48 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1519	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4333	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	2869	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6662m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6034	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	5492m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3196	0.45	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8666	0.34	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	503	0.390	ng/ul	98
12) Phenanthrene	17.75	178	621m	0.028	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095613.D
Acq On : 9 Feb 2018 18:23
Operator : SJ/JU
Sample : J1355-03
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D28

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:56 AM

Quant Time: Feb 10 01:23:48 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

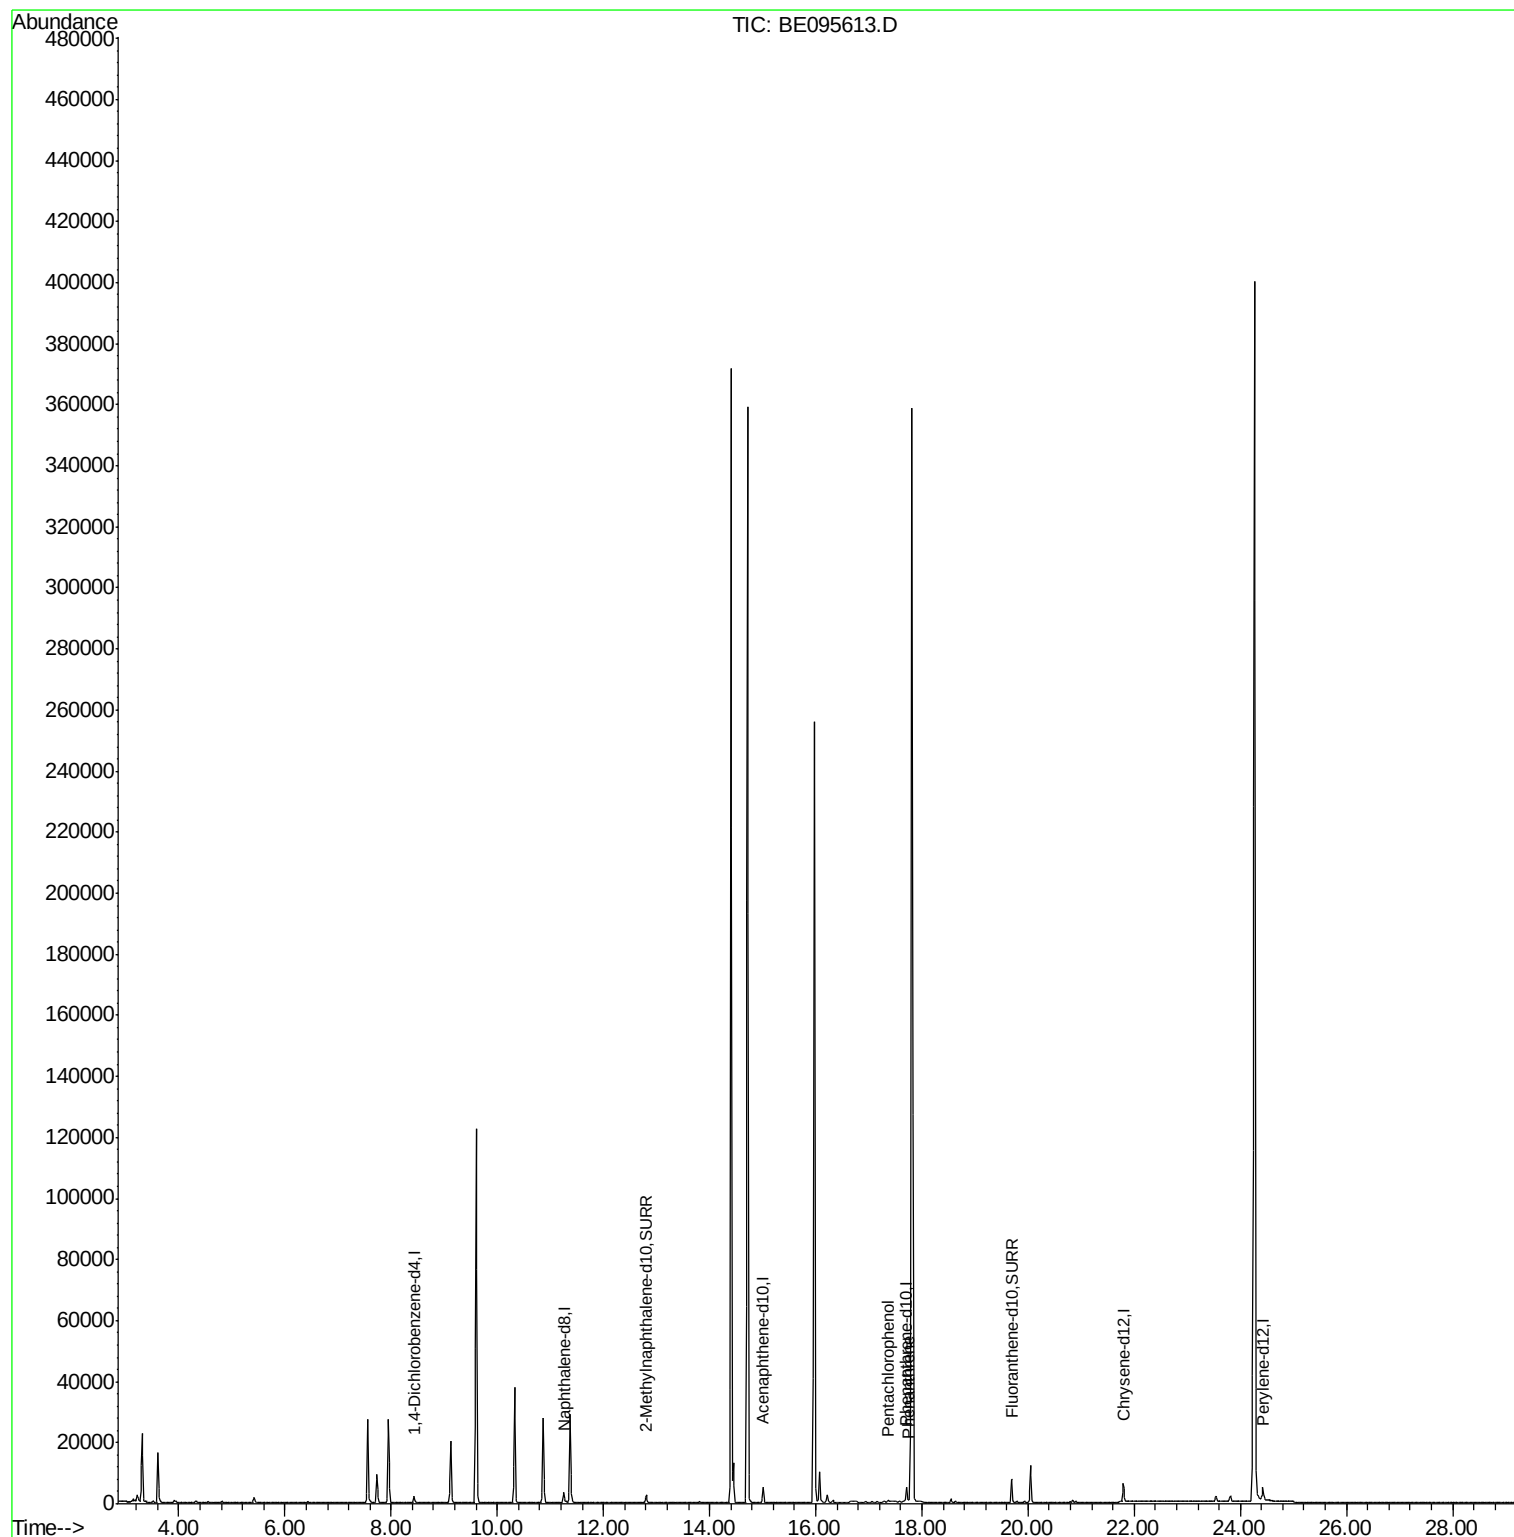

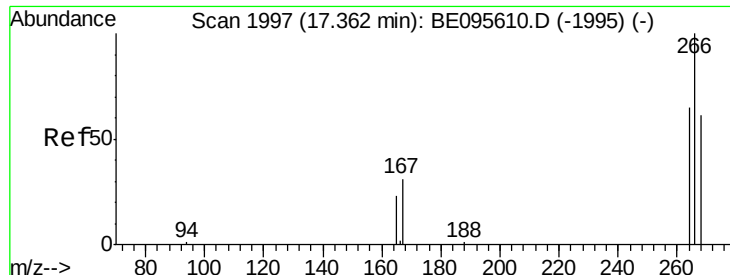





#11
 Pentachlorophenol
 Concen: 0.390 ng/ul
 RT: 17.36 min Scan# 1998
 Delta R.T. 0.00 min
 Lab File: BE095613.D
 Acq: 9 Feb 2018 18:23

Instrument :
 BNA_E
 ClientSampleId :
 F6D28

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.0	47.9	71.9
268	62.6	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:56 AM

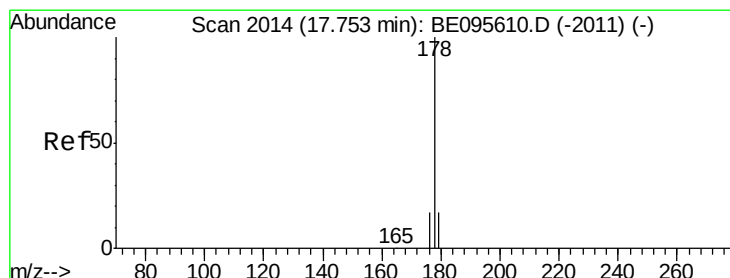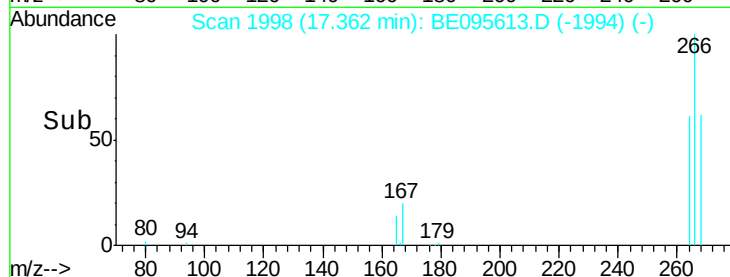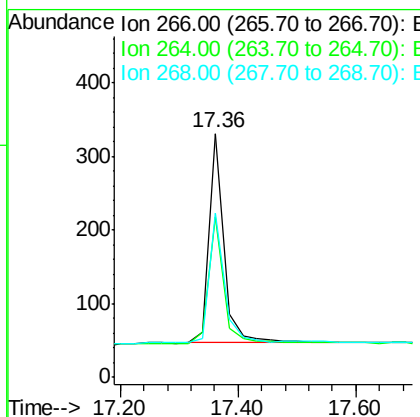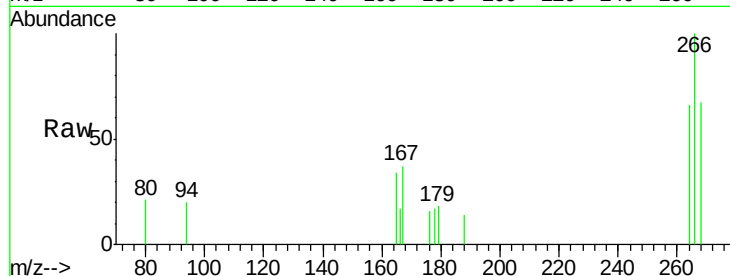

#12
 Phenanthrene
 Concen: 0.028 ng/ul m
 RT: 17.75 min Scan# 2015
 Delta R.T. 0.00 min
 Lab File: BE095613.D
 Acq: 9 Feb 2018 18:23

Tgt Ion	Ratio	Lower	Upper
178	100		
179	28.3	18.4	27.6#
176	27.1	13.6	20.4#

