

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095614.D
 Acq On : 9 Feb 2018 18:59
 Operator : SJ/JU
 Sample : J1339-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D56

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:59 AM

Quant Time: Feb 10 01:27:23 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 00:56:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1727	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	4983	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3295	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7433	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7005	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	6622m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2644	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7132	0.25	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	106	0.074	ng/ul	Qvalue 95
17) Pyrene	20.07	202	1034m	0.044	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095614.D
Acq On : 9 Feb 2018 18:59
Operator : SJ/JU
Sample : J1339-18
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D56

Manual Integrations
APPROVED

Sohil
2/12/2018 11:38:59 AM

Quant Time: Feb 10 01:27:23 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 00:56:50 2018
Response via : Initial Calibration

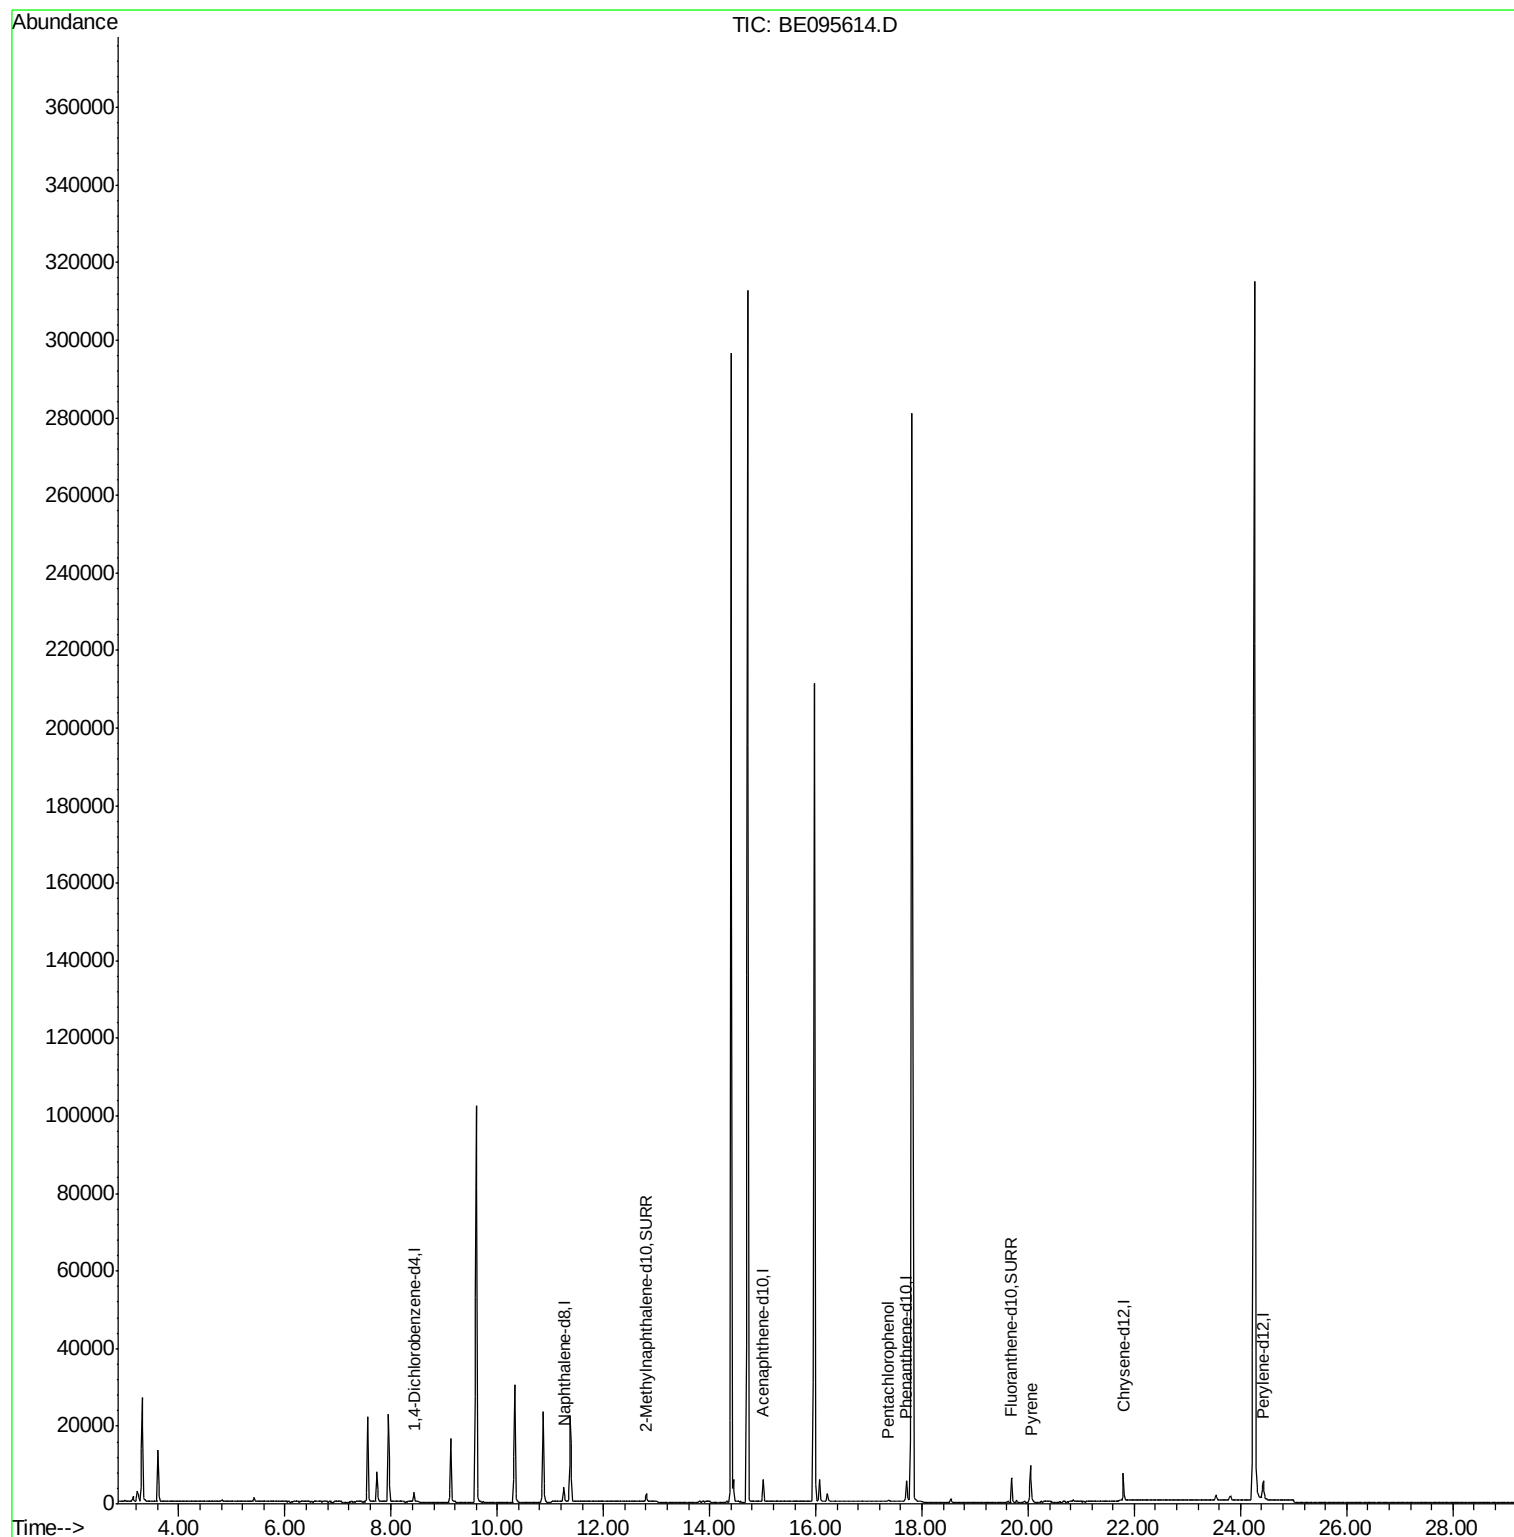

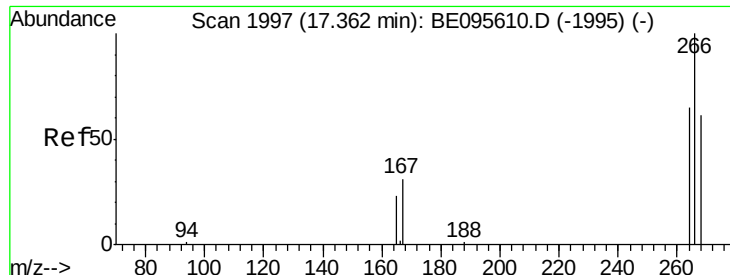





#11
 Pentachlorophenol
 Concen: 0.074 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095614.D
 Acq: 9 Feb 2018 18:59

Instrument :
 BNA_E
 ClientSampleId :
 F6D56

Tgt Ion	Ratio	Lower	Upper
266	100		
264	67.9	47.9	71.9
268	62.3	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:38:59 AM

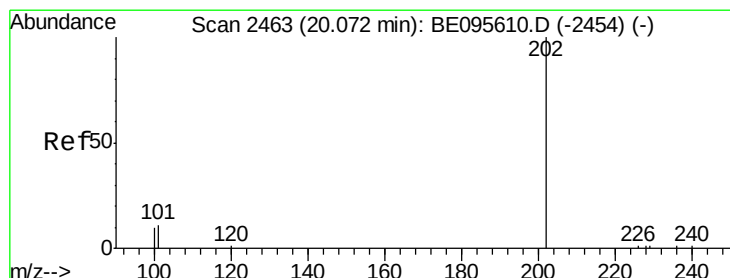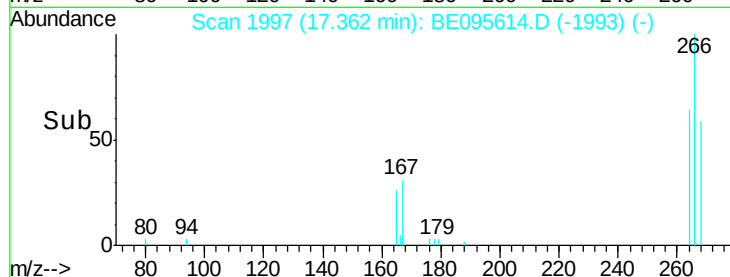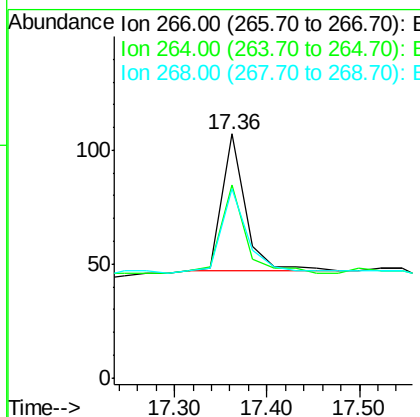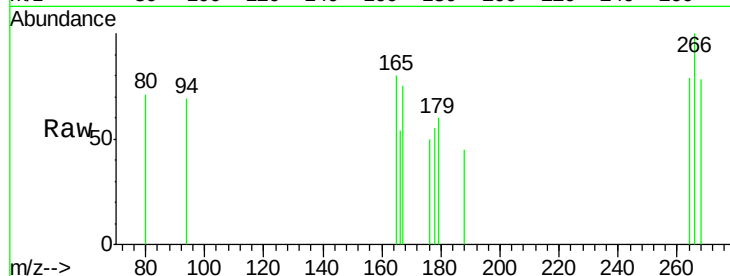

#17
 Pyrene
 Concen: 0.044 ng/ul m
 RT: 20.07 min Scan# 2464
 Delta R.T. 0.00 min
 Lab File: BE095614.D
 Acq: 9 Feb 2018 18:59

Tgt Ion	Ratio	Lower	Upper
202	100		
101	17.3	18.2	27.4#
100	18.4	15.6	23.4

