

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095630.D
 Acq On : 10 Feb 2018 4:47
 Operator : SJ/JU
 Sample : J1339-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D15

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:39:45 AM

Quant Time: Feb 12 00:51:49 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 02:59:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2160	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7789	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4390m	0.40	ng/ul	0.01
10) Phenanthrene-d10	17.71	188	8154m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7433	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7126m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3480m	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	10641	0.34	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	8563	5.422	ng/ul	98
17) Pyrene	20.08	202	2900	0.116	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095630.D
Acq On : 10 Feb 2018 4:47
Operator : SJ/JU
Sample : J1339-01
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D15

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:45 AM


Quant Time: Feb 12 00:51:49 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

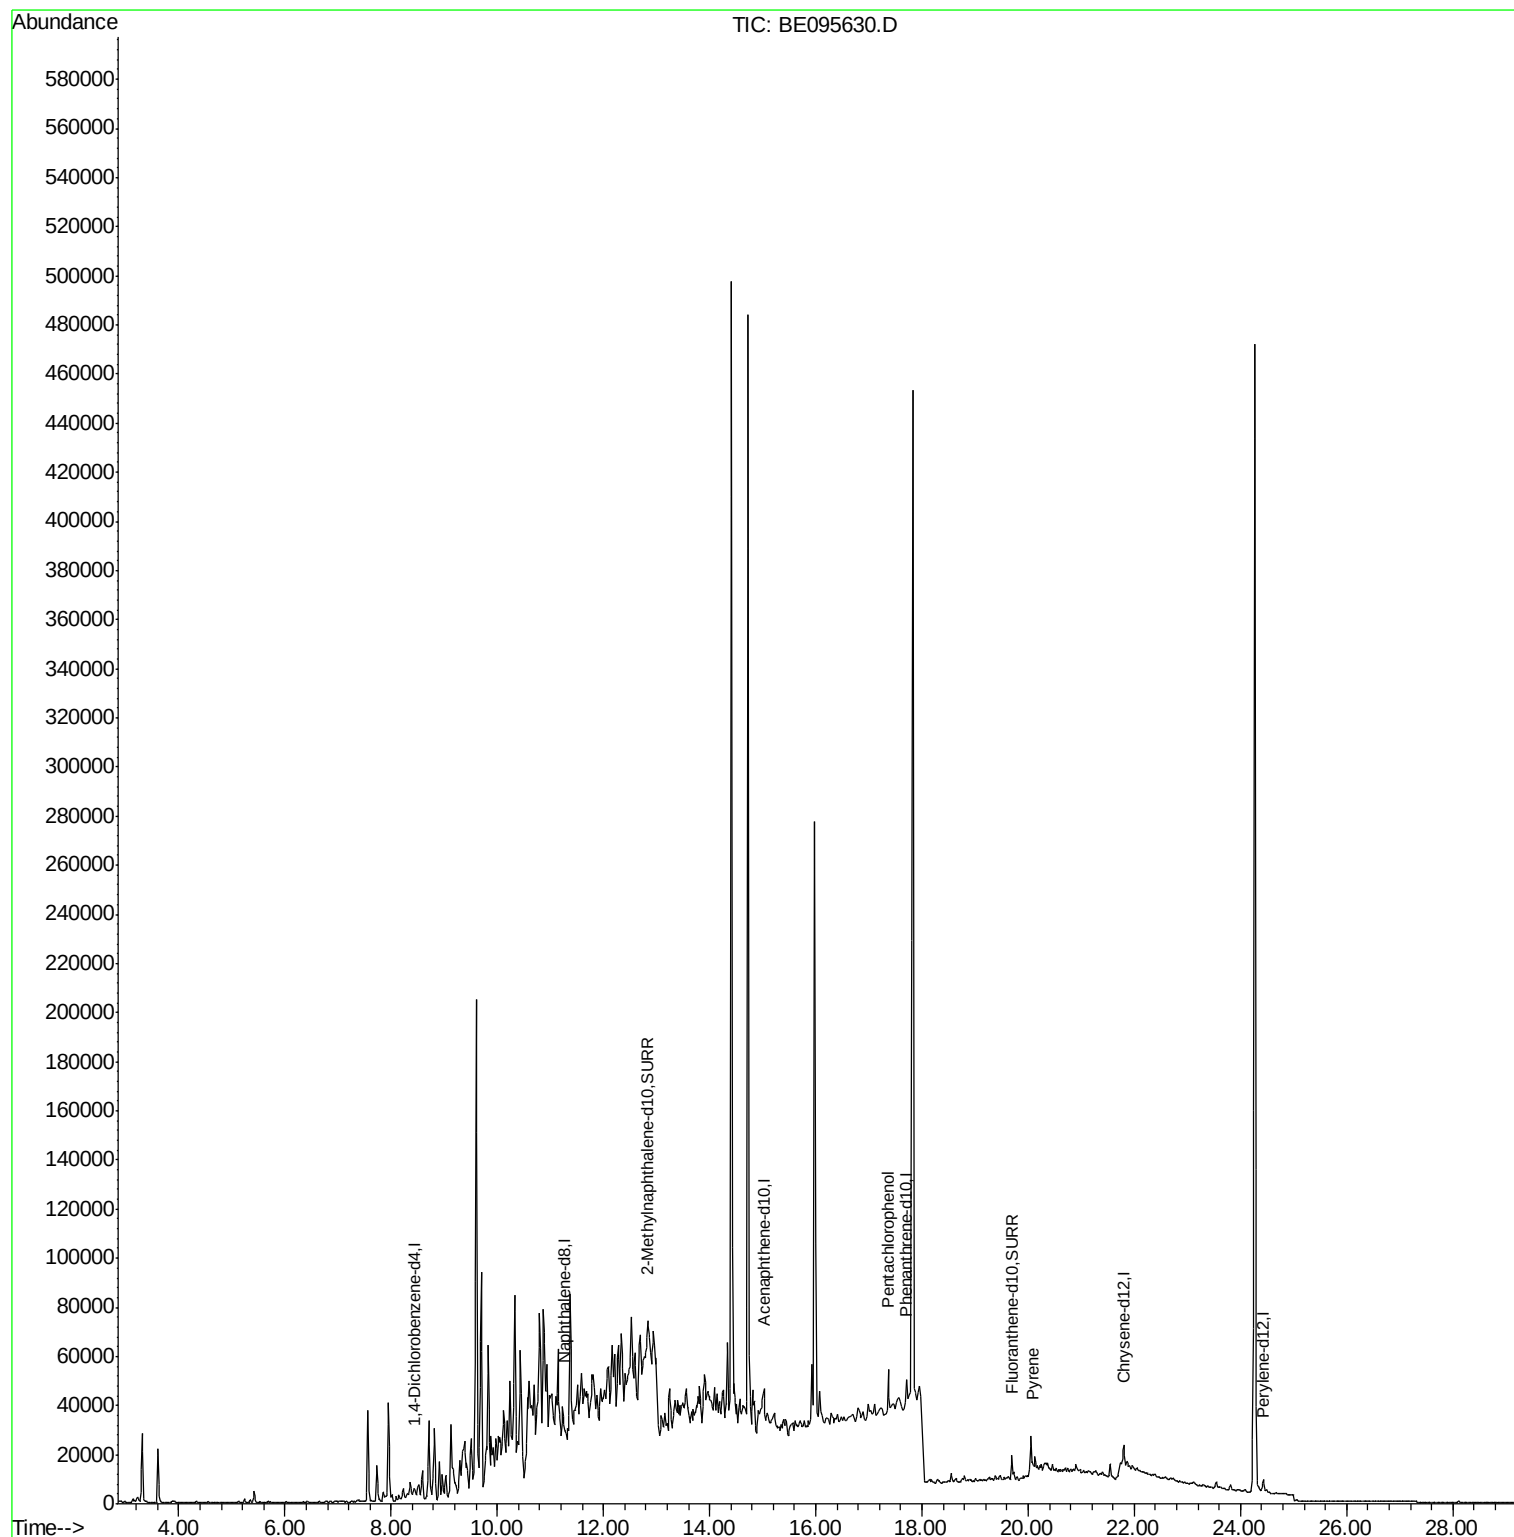

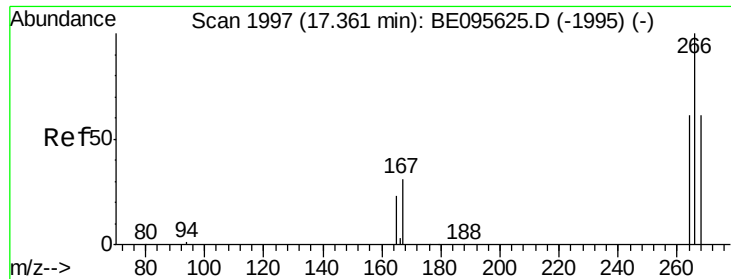

#11
 Pentachlorophenol
 Concen: 5.422 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095630.D
 Acq: 10 Feb 2018 4:47




Instrument :
 BNA_E
 ClientSampleId :
 F6D15

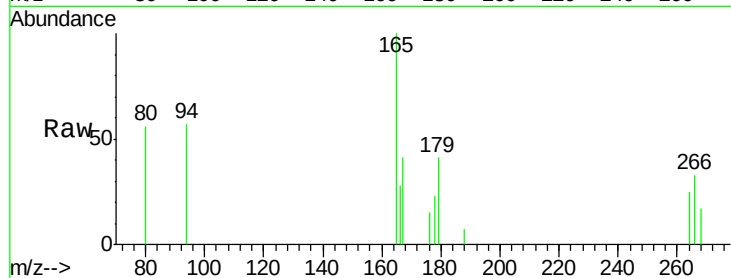


Tgt Ion	Ratio	Resp	Lower	Upper
266	100	8563		
264	59.4		47.9	71.9
268	60.1		49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:39:45 AM

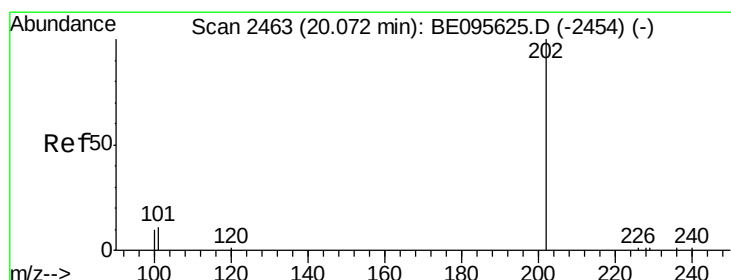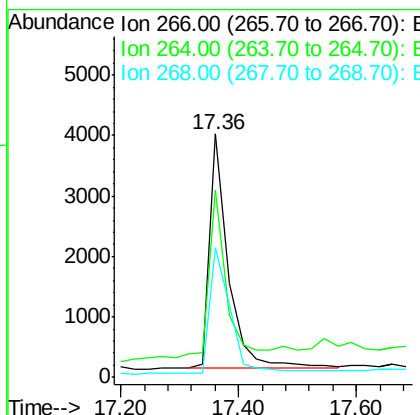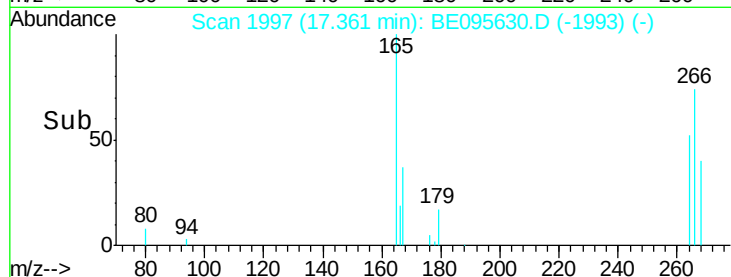

#17
 Pyrene
 Concen: 0.116 ng/ul
 RT: 20.08 min Scan# 2465
 Delta R.T. 0.01 min
 Lab File: BE095630.D
 Acq: 10 Feb 2018 4:47

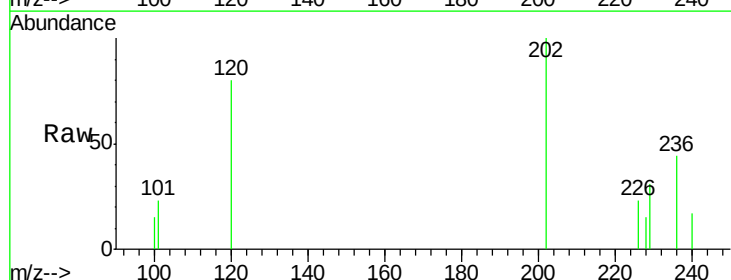

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	2900		
101	22.6		18.2	27.4
100	14.7		15.6	23.4#

