

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095634.D
 Acq On : 10 Feb 2018 7:07
 Operator : SJ/JU
 Sample : J1339-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D19

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:39:56 AM

Quant Time: Feb 12 01:13:22 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 02:59:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1973	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5834	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3902	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8900	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8152	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7479m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3465	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9418	0.28	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	88488	51.332	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095634.D
Acq On : 10 Feb 2018 7:07
Operator : SJ/JU
Sample : J1339-10
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D19

Manual Integrations
APPROVED

Sohil
2/12/2018 11:39:56 AM

Quant Time: Feb 12 01:13:22 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

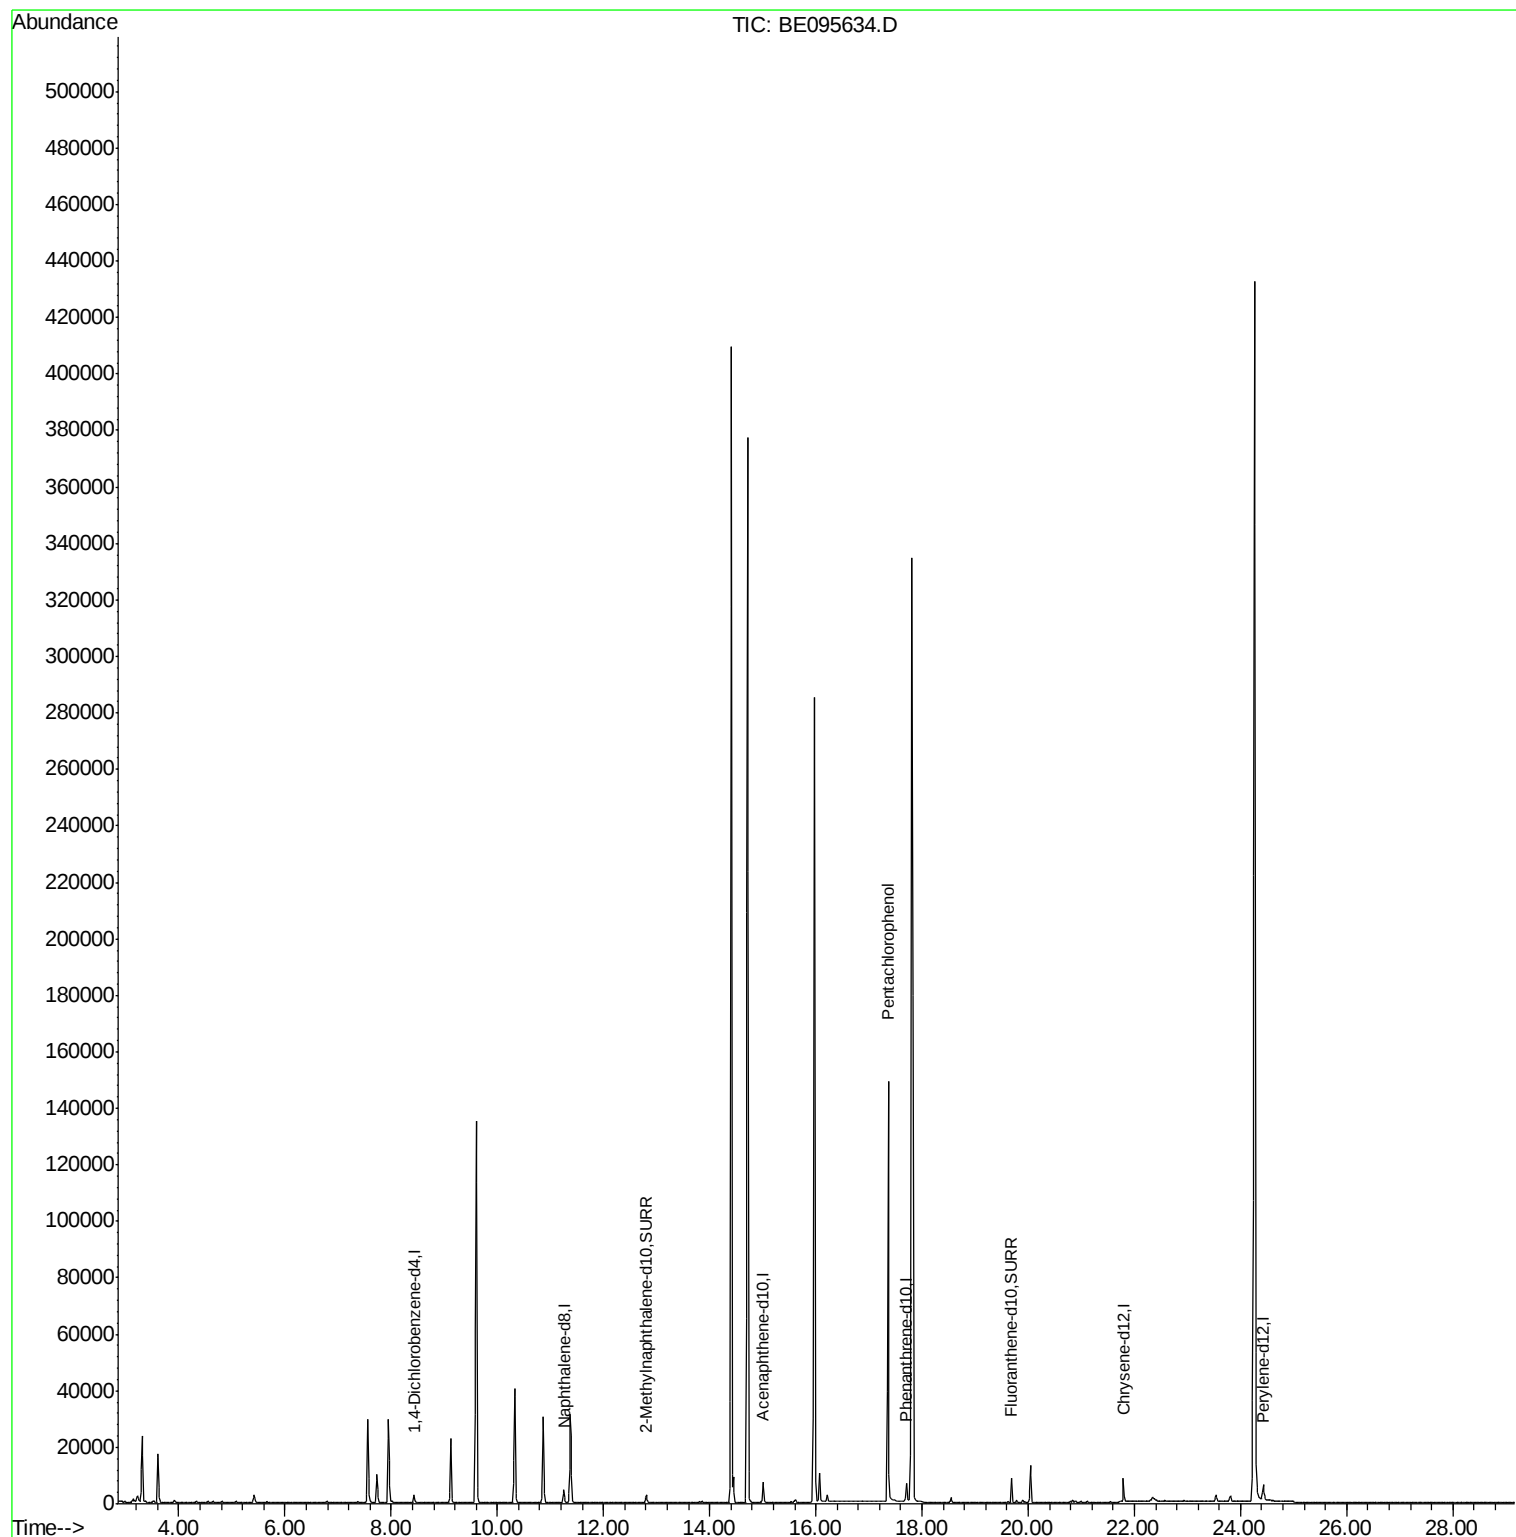

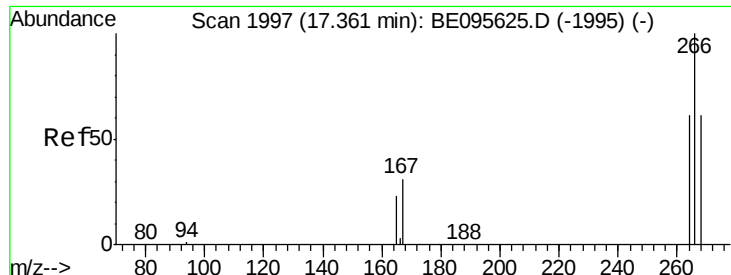


#11
 Pentachlorophenol
 Concen: 51.332 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095634.D
 Acq: 10 Feb 2018 7:07

Instrument :
 BNA_E
 ClientSampleId :
 F6D19

Tgt Ion:	266	Resp:	88488
Ion Ratio	Lower	Upper	
266	100		
264	62.6	47.9	71.9
268	62.8	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:39:56 AM

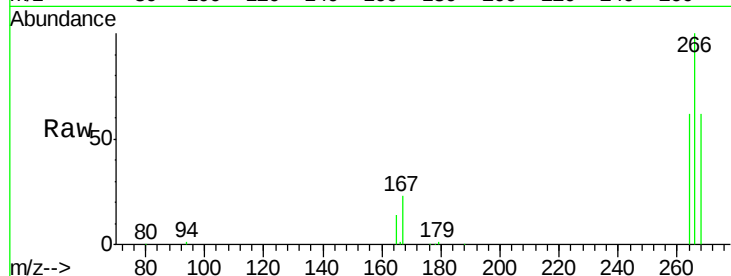

Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

