

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095640.D
 Acq On : 10 Feb 2018 10:42
 Operator : SJ/JU
 Sample : J1355-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D54

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:40:31 AM

2/12/2018 11:40:31 AM

Quant Time: Feb 12 01:39:35 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 10 02:59:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1978	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5987	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4049	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9032	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8220	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7423m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4266	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	11907	0.34	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.30	128	652	0.039	ng/ul#	71
5) 2-Methylnaphthalene	12.88	142	738	0.066	ng/ul	97
11) Pentachlorophenol	17.36	266	528	0.302	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095640.D
Acq On : 10 Feb 2018 10:42
Operator : SJ/JU
Sample : J1355-10
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D54


Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:31 AM

2/12/2018 11:40:31 AM

Quant Time: Feb 12 01:39:35 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 10 02:59:57 2018
Response via : Initial Calibration

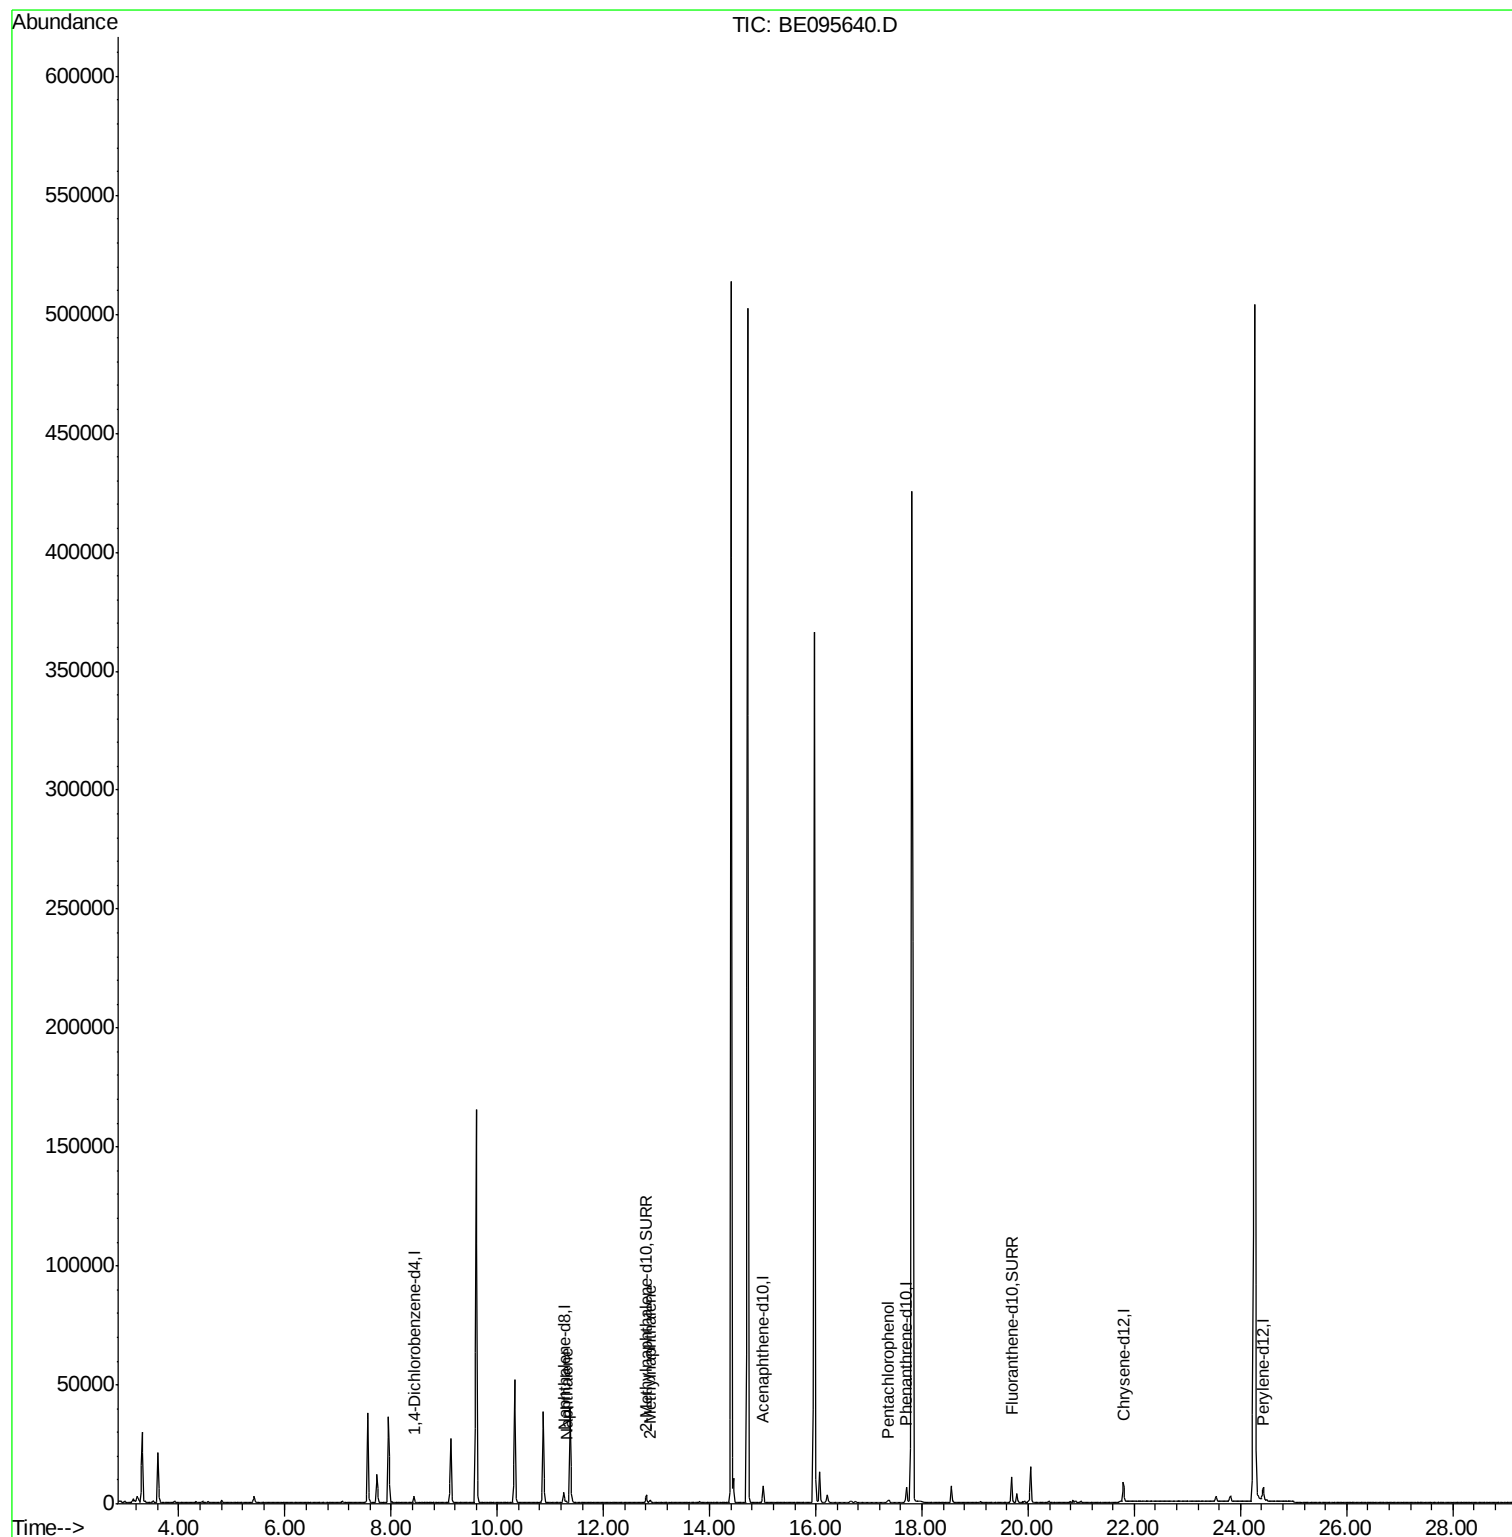

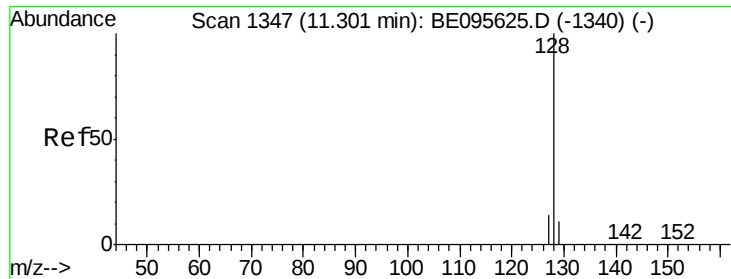

#3

Naphthalene

Concen: 0.039 ng/ul

RT: 11.30 min Scan# 1347

Delta R.T. 0.00 min

Lab File: BE095640.D

Acq: 10 Feb 2018 10:42

Instrument :

BNA_E

ClientSampleId :

F6D54


Tgt Ion:	128	Resp:	652
Ion Ratio	Lower	Upper	
128	100		
129	22.9	11.3	16.9#
127	21.5	4.0	6.0#

Manual Integrations
APPROVED




Sohil

2/12/2018 11:40:31 AM

2/12/2018 11:40:31 AM

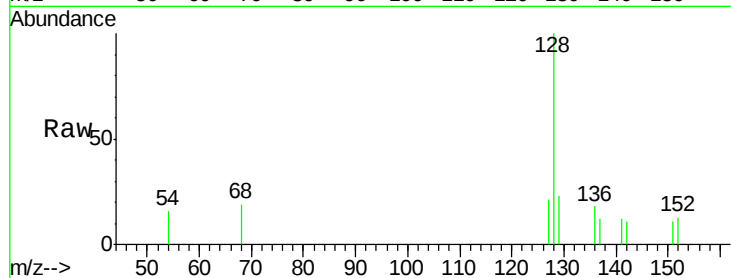

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

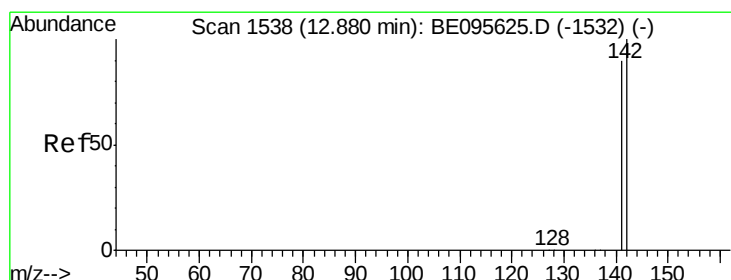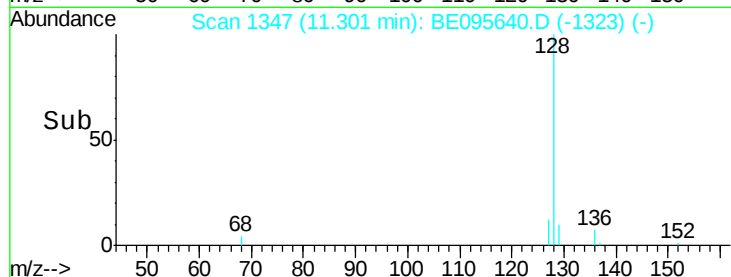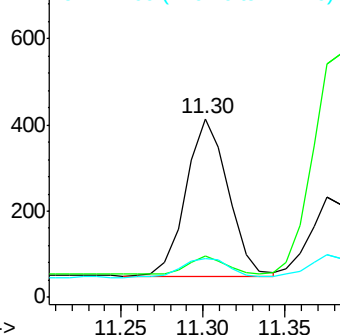

#5

2-Methylnaphthalene

Concen: 0.066 ng/ul


RT: 12.88 min Scan# 1538

Delta R.T. 0.00 min



Lab File: BE095640.D


Acq: 10 Feb 2018 10:42

Tgt Ion:	142	Resp:	738
Ion Ratio	Lower	Upper	
142	100		
141	88.2	72.6	108.8

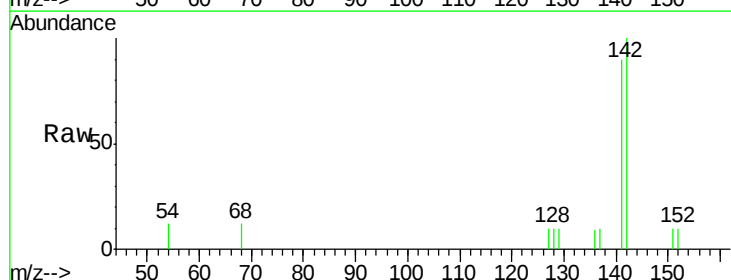

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E

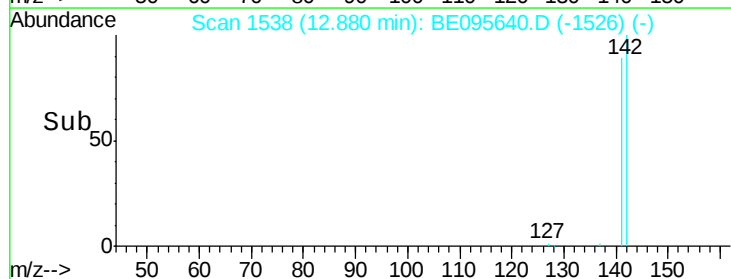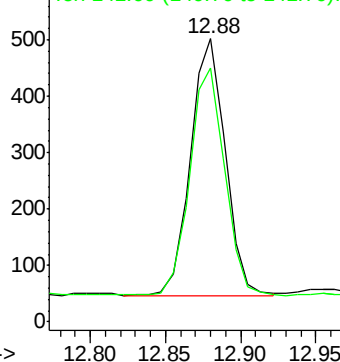

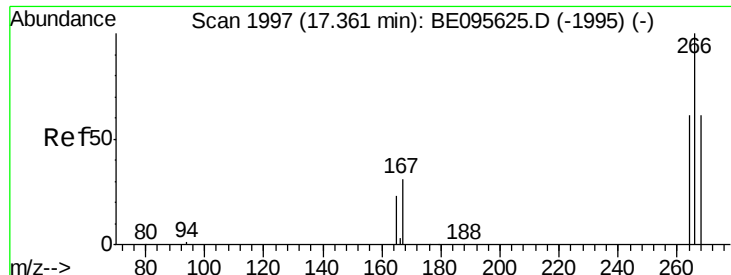

#11
 Pentachlorophenol
 Concen: 0.302 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095640.D
 Acq: 10 Feb 2018 10:42

Instrument :
 BNA_E
 ClientSampleId :
 F6D54

Tgt Ion:	266	Resp:	528
Ion Ratio	Lower	Upper	
266	100		
264	62.3	47.9	71.9
268	61.4	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:40:31 AM

2/12/2018 11:40:31 AM

