

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095643.D
 Acq On : 10 Feb 2018 13:05
 Operator : SJ/JU
 Sample : J1355-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D31

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:40:39 AM

Quant Time: Feb 12 02:03:05 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 12 01:48:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2129	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	6344	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4216	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9852	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8775	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	7883m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.80	152	4379	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	11733	0.31	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	278	0.146	ng/ul	91
12) Phenanthrene	17.75	178	810m	0.024	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095643.D
Acq On : 10 Feb 2018 13:05
Operator : SJ/JU
Sample : J1355-06
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D31

Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:39 AM

Quant Time: Feb 12 02:03:05 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 01:48:13 2018
Response via : Initial Calibration

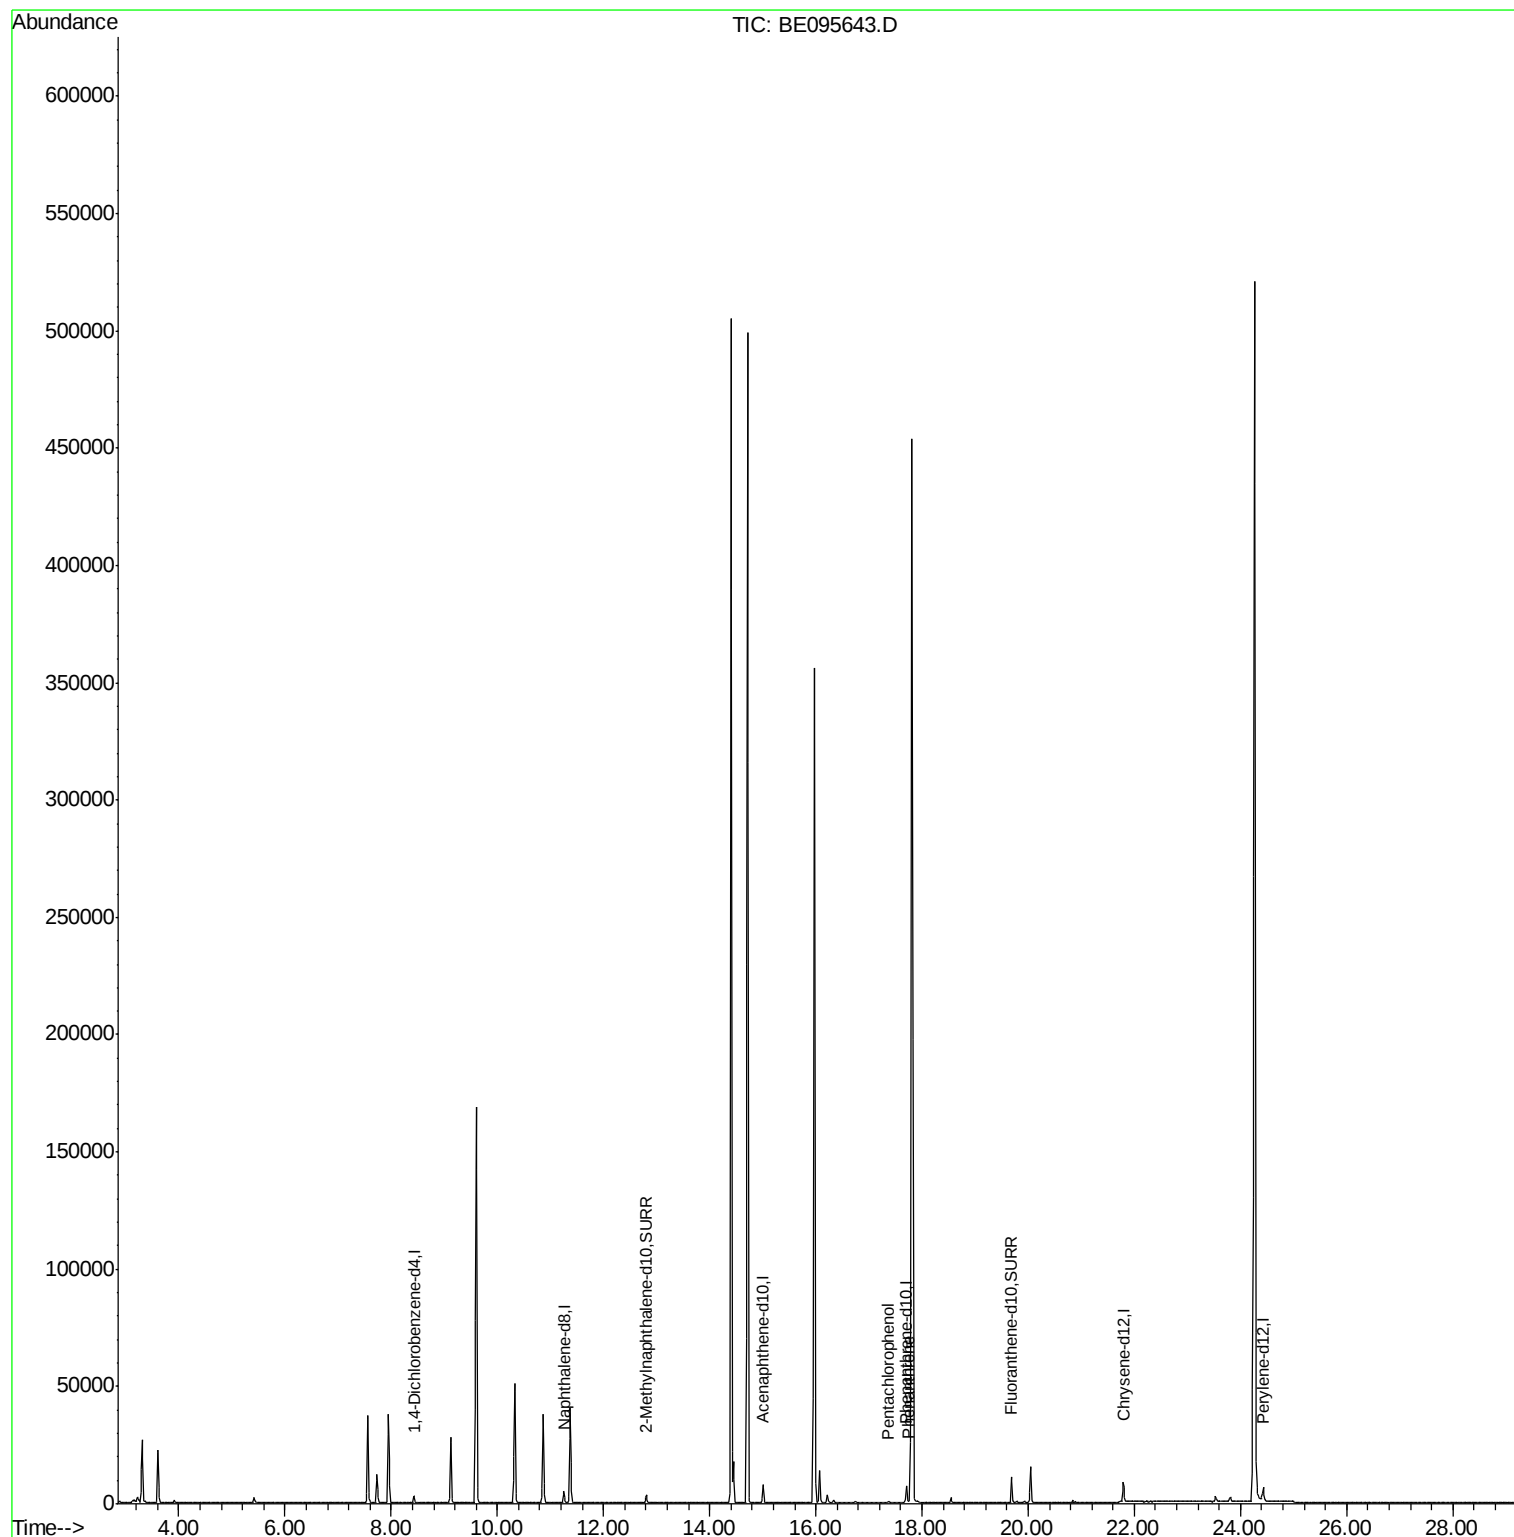

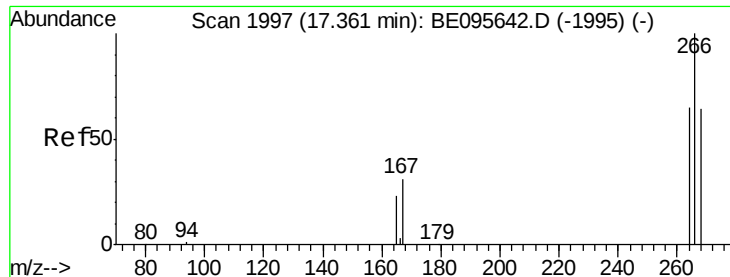





#11
 Pentachlorophenol
 Concen: 0.146 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095643.D
 Acq: 10 Feb 2018 13:05

Instrument :
 BNA_E
 ClientSampleId :
 F6D31

Tgt Ion	Ratio	Lower	Upper
266	100		
264	68.0	47.9	71.9
268	67.3	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:40:39 AM

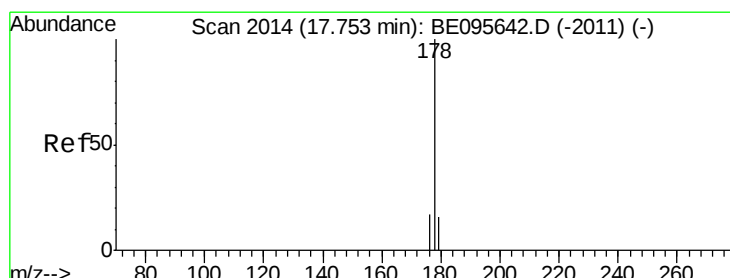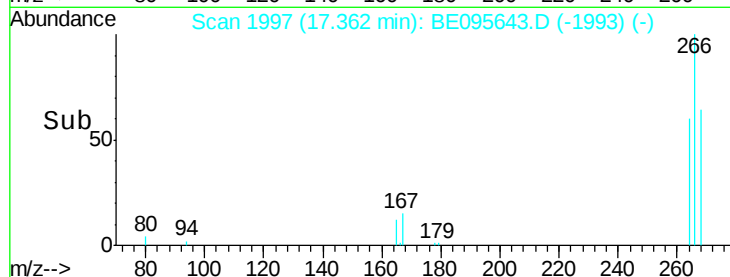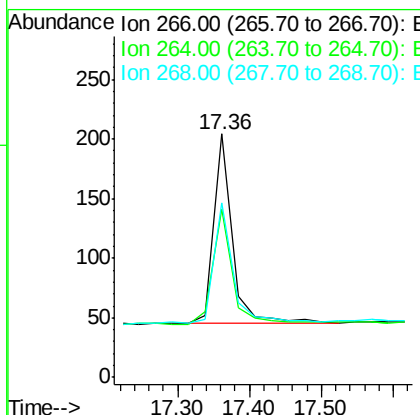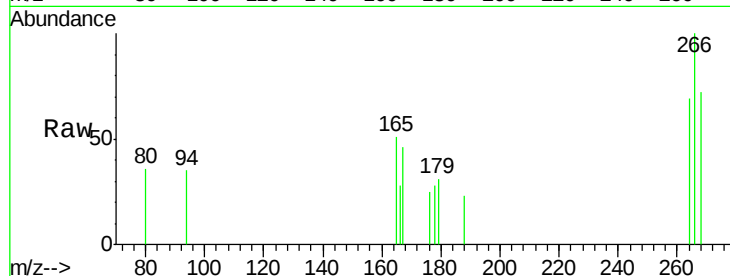

#12
 Phenanthrene
 Concen: 0.024 ng/ul m
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095643.D
 Acq: 10 Feb 2018 13:05

Tgt Ion	Ratio	Lower	Upper
178	100		
179	28.0	18.4	27.6#
176	25.1	13.6	20.4#

