

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
 Data File : BE095644.D
 Acq On : 10 Feb 2018 13:41
 Operator : SJ/JU
 Sample : J1355-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D30

Manual Integrations
 APPROVED

Sohil
 2/12/2018 11:40:41 AM

Quant Time: Feb 12 02:05:25 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 12 01:48:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2153	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	6560	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4385	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	10121	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	9146	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8244m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4533	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	12461	0.32	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.75	178	756m	0.022	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020918\
Data File : BE095644.D
Acq On : 10 Feb 2018 13:41
Operator : SJ/JU
Sample : J1355-05
Misc :
ALS Vial : 44 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
F6D30

Manual Integrations
APPROVED

Sohil
2/12/2018 11:40:41 AM

Quant Time: Feb 12 02:05:25 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 12 01:48:13 2018
Response via : Initial Calibration

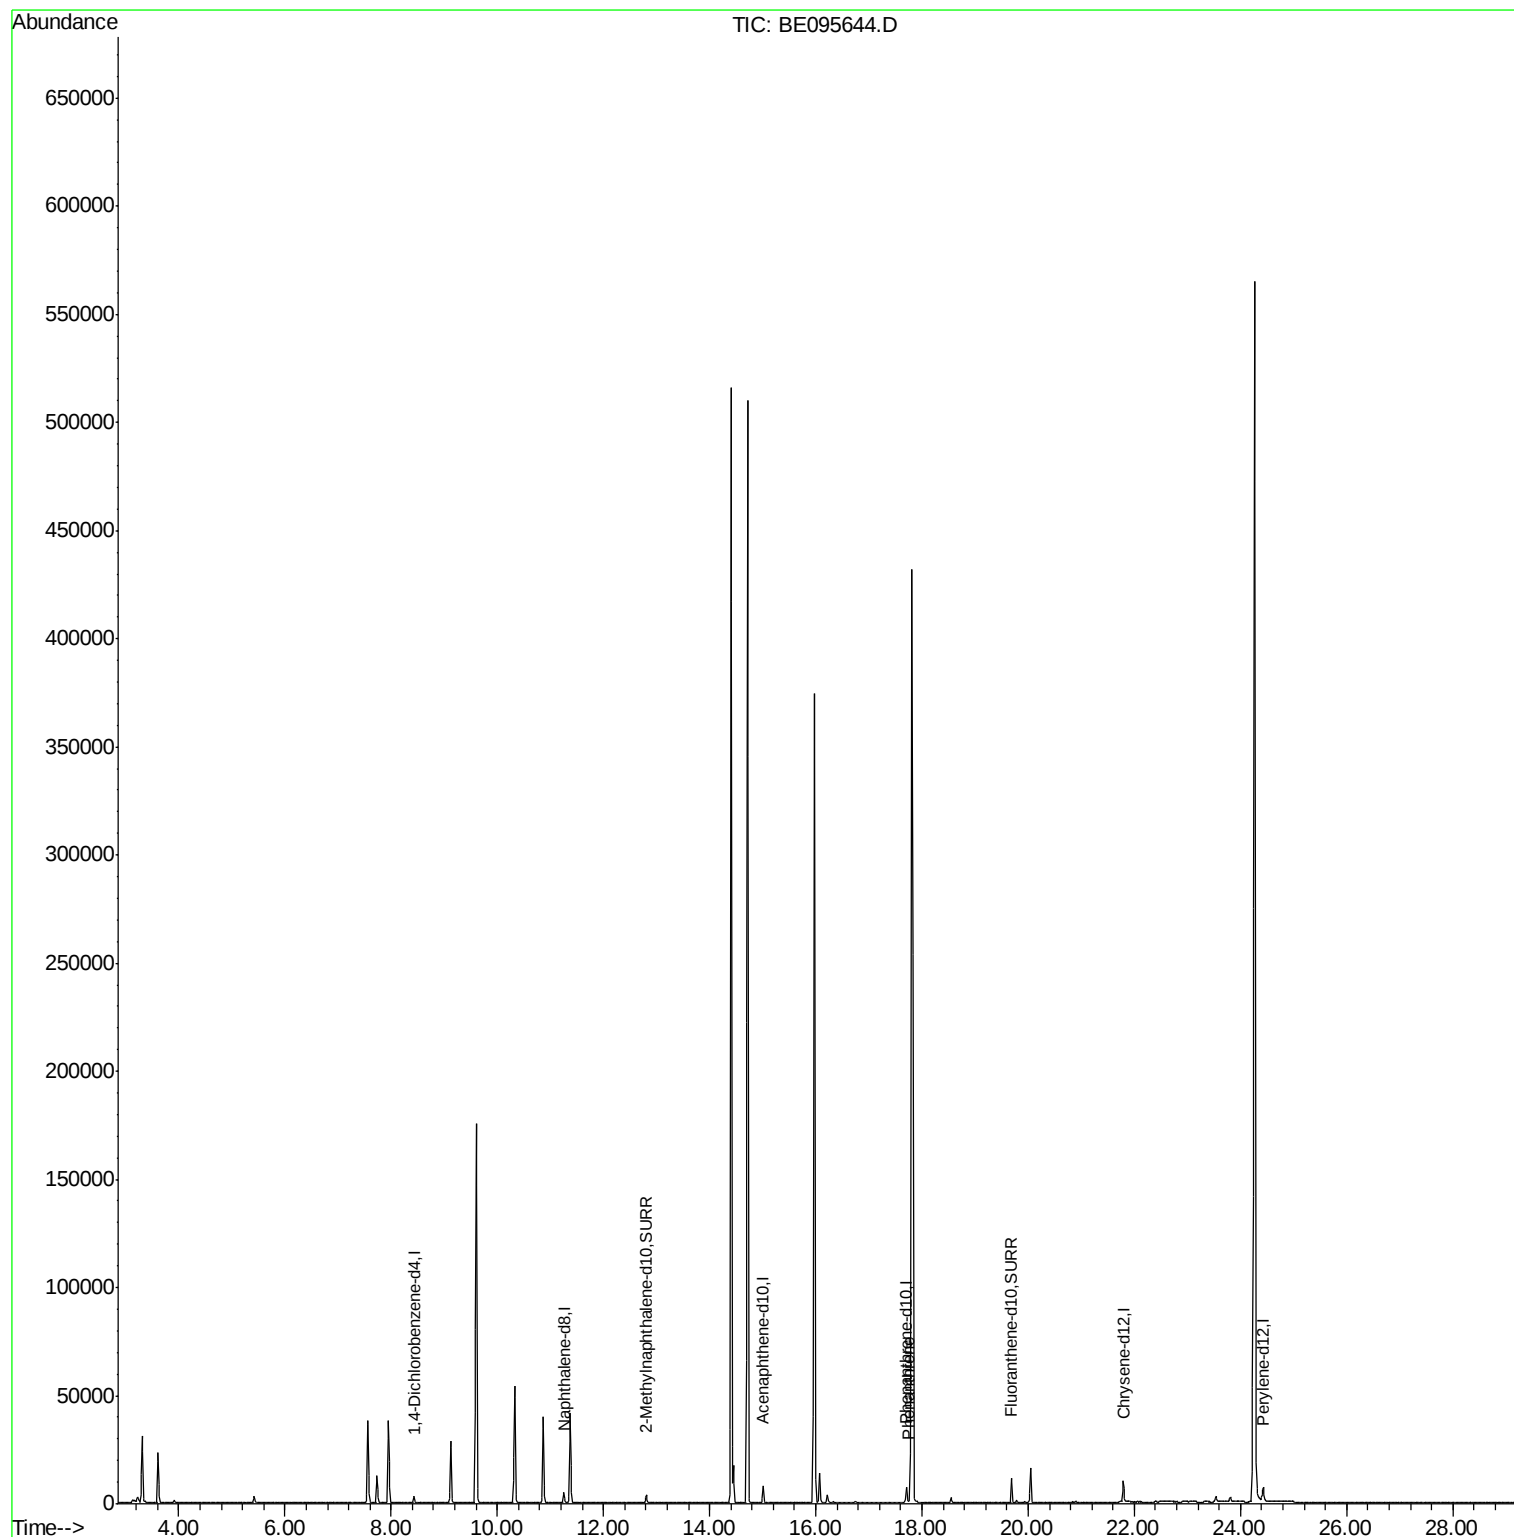

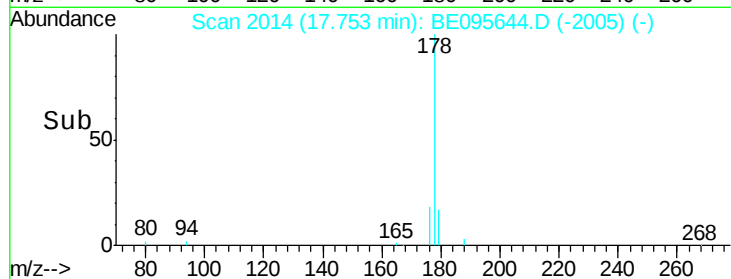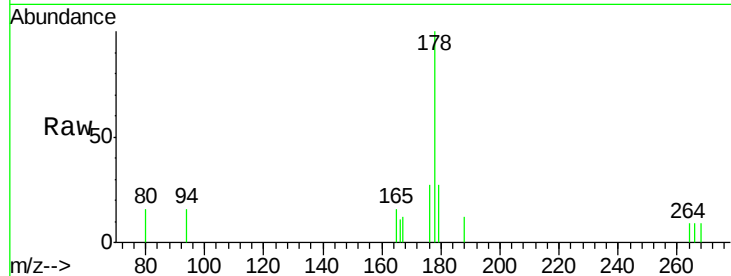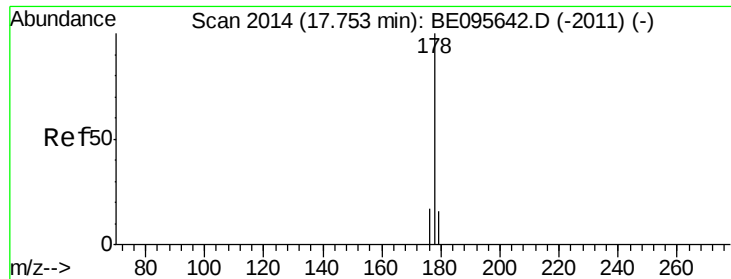

#12

Phenanthrene

Concen: 0.022 ng/ul m

RT: 17.75 min Scan# 2014

Delta R.T. 0.00 min

Lab File: BE095644.D

Acq: 10 Feb 2018 13:41

Instrument :

BNA_E

ClientSampleId :

F6D30

Tgt Ion:178 Resp: 756

Ion Ratio Lower Upper

178 100

179 27.5 18.4 27.6

176 26.7 13.6 20.4#

Manual Integrations

APPROVED

Sohil

2/12/2018 11:40:41 AM

