


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021015\
 Data File : BE089551.D
 Acq On : 10 Feb 2015 15:39
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE021015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 11 11:21:59 2015

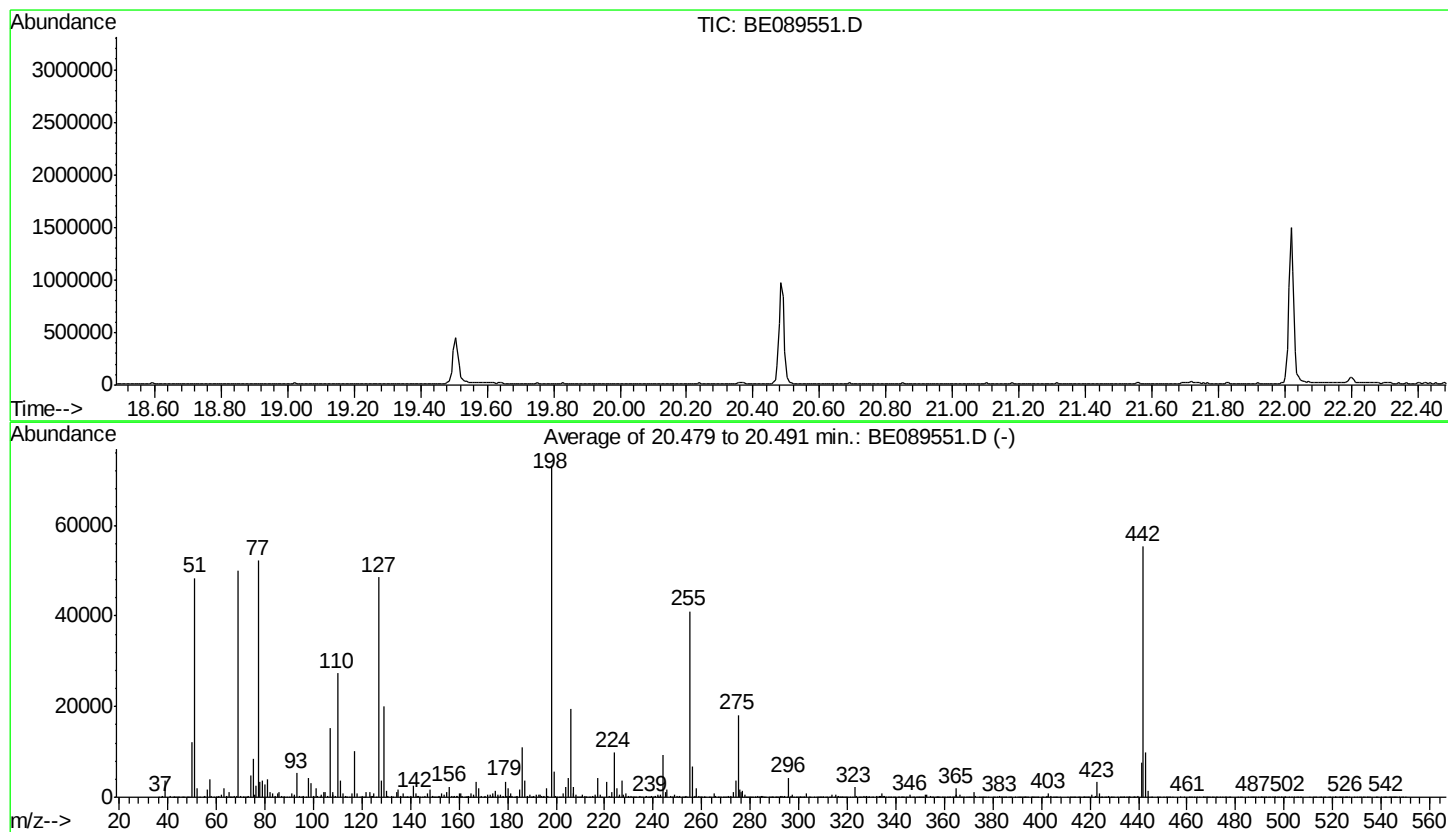

AutoFind: Scans 3249, 3250, 3251; Background Corrected with Scan 3239

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.1	48377	PASS
68	69	0.00	2	0.4	177	PASS
69	198	0.00	100	68.2	49919	PASS
70	69	0.00	2	0.4	198	PASS
127	198	10	80	66.3	48554	PASS
197	198	0.00	2	0.3	240	PASS
198	198	100	100	100.0	73187	PASS
199	198	5	9	7.7	5632	PASS
275	198	10	60	24.8	18170	PASS
365	198	1	100	2.6	1916	PASS
441	442	0.01	24	13.6	7523	PASS
442	198	50	100	75.6	55343	PASS
443	442	15	24	18.0	9980	PASS