

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021017\
 Data File : BE092720.D
 Acq On : 10 Feb 2017 14:15
 Operator : SJ/MA
 Sample : PB96821BSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB96821BSD


Manual Integrations
 APPROVED

mohammad
 2/13/2017 12:51:01 PM

Quant Time: Feb 10 16:02:38 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 17 10:14:01 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	10338	5.00	ng	-0.02
7) Naphthalene-d8	10.89	136	42237	5.00	ng	-0.02
12) Acenaphthene-d10	14.76	164	23782	5.00	ng	-0.02
18) Phenanthrene-d10	17.53	188	41348	5.00	ng	0.00
24) Chrysene-d12	21.70	240	54388	5.00	ng	-0.02
31) Perylene-d12	24.04	264	46372	5.00	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.62	112	21939	9.51	ng	-0.03
5) Phenol-d6	7.29	99	28266	9.99	ng	-0.04
8) Nitrobenzene-d5	9.29	82	12965	4.73	ng	-0.04
13) 2,4,6-Tribromophenol	16.26	330	5875	8.36	ng	-0.03
14) 2-Fluorobiphenyl	13.39	172	27133	4.64	ng	-0.03
26) Terphenyl-d14	20.14	244	29688	3.86	ng	-0.02
Target Compounds						
2) 1,4-Dioxane	3.36	88	5158	3.70	ng	# 73
3) n-Nitrosodimethylamine	3.71	42	8007	4.29	ng	# 100
6) bis(2-Chloroethyl)ether	7.54	93	12754	4.25	ng	# 28
9) Naphthalene	10.95	128	39905	4.52	ng	94
10) Hexachlorobutadiene	11.24	225	6115	4.69	ng	99
11) 2-Methylnaphthalene	12.58	142	25501	4.66	ng	# 86
15) Acenaphthylene	14.48	152	161960	4.94	ng	100
16) Acenaphthene	14.83	154	23687	4.51	ng	93
17) Fluorene	15.81	166	30096	4.56	ng	99
19) Hexachlorobenzene	16.84	284	8827	6.57	ng	# 66
20) Pentachlorophenol	17.21	266	5595	13.16	ng	89
21) Phenanthrene	17.56	178	48592	5.32	ng	# 94
22) Anthracene	17.65	178	48377	5.74	ng	98
23) Fluoranthene	19.56	202	214098	5.29	ng	100
25) Pyrene	19.92	202	216065	4.03	ng	99
27) Benzo(a)anthracene	21.68	228	243133m	4.54	ng	
28) Chrysene	21.72	228	213948m	3.55	ng	
29) Bis(2-ethylhexyl)phthalate	21.59	149	23145	2.31	ng	# 56
30) Indeno(1,2,3-cd)pyrene	26.50	276	259475	3.98	ng	98
32) Benzo(b)fluoranthene	23.31	252	53975	4.81	ng	95
33) Benzo(k)fluoranthene	23.36	252	57137	5.07	ng	92
34) Benzo(a)pyrene	23.93	252	54460	5.17	ng	95
35) Dibenzo(a,h)anthracene	26.51	278	53837	5.22	ng	95
36) Benzo(g,h,i)perylene	27.26	276	224883	5.16	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

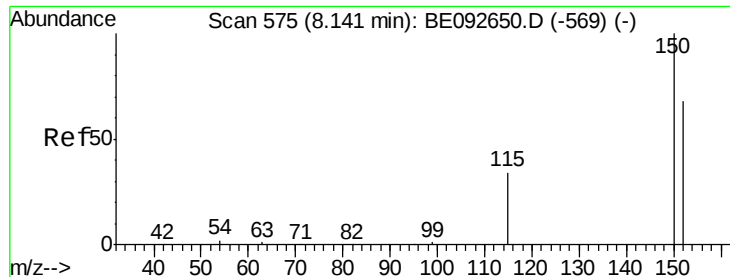

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.12 min Scan# 574

Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E





ClientSampleId :

PB96821BSD

Tgt Ion	Ratio	Lower	Upper
152	100		
150	153.3	106.0	159.0
115	55.1	31.2	46.8

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#2

1,4-Dioxane

Concen: 3.70 ng




RT: 3.36 min Scan# 67


Delta R.T. -0.01 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
88	100		
58	95.5	63.6	95.4
43	62.5	28.0	42.0





#3

n-Nitrosodimethylamine

Concen: 4.29 ng

RT: 3.71 min Scan# 97

Delta R.T. -0.03 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E





ClientSampleId :

PB96821BSD

Tgt Ion:	42	Resp:	8007
Ion Ratio	Lower	Upper	
42	100		
74	107.5	86.0	129.0
44	8.4	5.1	7.7#

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#4

2-Fluorophenol

Concen: 9.51 ng




RT: 5.62 min Scan# 355


Delta R.T. -0.03 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion:	112	Resp:	21939
Ion Ratio	Lower	Upper	
112	100		
64	67.9	53.5	80.3
63	36.2	27.9	41.9





#5

Phenol-d6

Concen: 9.99 ng

RT: 7.29 min Scan# 538

Delta R.T. -0.04 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E





ClientSampleId :

PB96821BSD

Tgt Ion:	99	Resp:	28266
Ion Ratio	Lower	Upper	
99	100		
42	0.0	16.0	24.0#
71	33.3	30.6	45.8

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#6

bis(2-Chloroethyl)ether

Concen: 4.25 ng




RT: 7.54 min Scan# 549


Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion:	93	Resp:	12754
Ion Ratio	Lower	Upper	
93	100		
63	0.0	71.6	107.4#
95	32.1	24.0	36.0





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.89 min Scan# 705

Delta R.T. -0.02 min

Lab File: BE092720.D


Acq: 10 Feb 2017 14:15

Instrument :

BNA_E

ClientSampleId :




PB96821BSD



Tgt Ion	Ratio	Resp	Lower	Upper
136	100	42237		
137	10.5	8.2	12.4	
54	9.7	9.6	14.4	
68	7.0	6.7	10.1	

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#8

Nitrobenzene-d5

Concen: 4.73 ng




RT: 9.29 min Scan# 625


Delta R.T. -0.04 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	12965		
128	56.4	39.0	58.4	
54	37.9	44.8	67.2	





#9

Naphthalene

Concen: 4.52 ng

RT: 10.95 min Scan# 708

Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E





ClientSampleId :

PB96821BSD

Tgt Ion:	128	Resp:	39905
Ion Ratio	Lower	Upper	
128	100		
129	12.0	11.2	16.8
127	11.9	11.6	17.4

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#10

Hexachlorobutadiene

Concen: 4.69 ng




RT: 11.24 min Scan# 723


Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion:	225	Resp:	6115
Ion Ratio	Lower	Upper	
225	100		
223	62.5	50.6	76.0
227	64.1	51.4	77.0









#11
2-Methylnaphthalene
Concen: 4.66 ng
RT: 12.58 min Scan# 810
Delta R.T. -0.03 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion	Ratio	Lower	Upper
142	100		
141	81.5	73.7	110.5
115	30.6	34.0	51.0#




Manual Integrations
APPROVED


mohammad
2/13/2017 12:51:01 PM



#12
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.76 min Scan# 977
Delta R.T. -0.02 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
164	100		
162	114.2	71.4	107.0#
160	56.1	27.4	41.2#









#13
 2,4,6-Tribromophenol
 Concen: 8.36 ng
 RT: 16.26 min Scan# 1084
 Delta R.T. -0.03 min
 Lab File: BE092720.D
 Acq: 10 Feb 2017 14:15

Instrument :
 BNA_E
 ClientSampleId :
 PB96821BSD

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	5875		
332	96.9	75.4	113.0	
141	43.2	31.0	46.6	




Manual Integrations
 APPROVED


mohammad
 2/13/2017 12:51:01 PM



#14
 2-Fluorobiphenyl
 Concen: 4.64 ng
 RT: 13.39 min Scan# 880
 Delta R.T. -0.03 min
 Lab File: BE092720.D
 Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	27133		
171	34.0	30.1	45.1	
170	22.5	21.8	32.6	









#15
Acenaphthylene
Concen: 4.94 ng
RT: 14.48 min Scan# 960
Delta R.T. -0.03 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion	Ratio	Lower	Upper
152	100		
151	4.9	3.9	5.9
153	13.0	10.4	15.6




Manual Integrations
APPROVED


mohammad
2/13/2017 12:51:01 PM



#16
Acenaphthene
Concen: 4.51 ng
RT: 14.83 min Scan# 981
Delta R.T. -0.02 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
154	100		
153	456.2	350.8	526.2
152	227.3	171.1	256.7









#17
Fluorene
Concen: 4.56 ng
RT: 15.81 min Scan# 1045
Delta R.T. -0.03 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion	Ratio	Lower	Upper
166	100		
165	99.2	78.2	117.4
167	13.3	11.0	16.4




Manual Integrations
APPROVED


mohammad
2/13/2017 12:51:01 PM



#18
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.53 min Scan# 1152
Delta R.T. -0.00 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
188	100		
94	3.0	3.2	4.8#
80	2.4	2.6	3.8#






#19
Hexachlorobenzene
Concen: 6.57 ng
RT: 16.84 min Scan# 1122
Delta R.T. -0.02 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD




Tgt Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	31.4	27.9	41.9

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM






Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E




#20
Pentachlorophenol
Concen: 13.16 ng
RT: 17.21 min Scan# 1138
Delta R.T. -0.02 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
266	100		
268	68.0	62.5	93.7
264	62.8	57.2	85.8

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E





#21

Phenanthrene

Concen: 5.32 ng

RT: 17.56 min Scan# 1153

Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E





ClientSampleId :

PB96821BSD

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.9	15.8	23.8
179	14.9	16.0	24.0

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#22

Anthracene

Concen: 5.74 ng




RT: 17.65 min Scan# 1157


Delta R.T. -0.05 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.6	15.0	22.4
179	14.7	12.2	18.2





#23

Fluoranthene

Concen: 5.29 ng

RT: 19.56 min Scan# 1263

Delta R.T. -0.03 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E


ClientSampleId :

PB96821BSD




Tgt Ion:	202	Resp:	214098
Ion Ratio	Lower	Upper	
202	100		
101	2.7	2.2	3.4
203	17.2	13.7	20.5

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E



#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.70 min Scan# 1373




Delta R.T. -0.02 min


Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion:	240	Resp:	54388
Ion Ratio	Lower	Upper	
240	100		
120	2.4	2.6	4.0#
236	28.1	24.6	37.0

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E









#25
 Pyrene
 Concen: 4.03 ng
 RT: 19.92 min Scan# 1284
 Delta R.T. -0.03 min
 Lab File: BE092720.D
 Acq: 10 Feb 2017 14:15

Instrument :
 BNA_E
 ClientSampleId :
 PB96821BSD

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
200	5.4	4.2	6.4
203	18.0	13.9	20.9




Manual Integrations
 APPROVED


mohammad
 2/13/2017 12:51:01 PM



#26
 Terphenyl-d14
 Concen: 3.86 ng
 RT: 20.14 min Scan# 1297
 Delta R.T. -0.02 min
 Lab File: BE092720.D
 Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Resp Lower	Resp Upper
244	100		
212	7.4	6.7	10.1
122	2.5	3.6	5.4#





#27

Benzo(a)anthracene

Concen: 4.54 ng m

RT: 21.68 min Scan# 1372

Delta R.T. -0.02 min

Lab File: BE092720.D





Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.9	23.6	35.4
229	17.0	13.3	19.9

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#28

Chrysene

Concen: 3.55 ng m




RT: 21.72 min Scan# 1374


Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
228	100		
226	40.7	36.3	54.5
229	12.1	10.6	16.0





#29

Bis(2-ethylhexyl)phthalate

Concen: 2.31 ng

RT: 21.59 min Scan# 1368

Delta R.T. -0.02 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Instrument :

BNA_E





ClientSampleId :

PB96821BSD

Tgt Ion:	149	Resp:	23145
Ion Ratio	Lower	Upper	
149	100		
167	0.0	16.0	24.0#
279	0.0	16.0	24.0#

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#30

Indeno(1,2,3-cd)pyrene

Concen: 3.98 ng




RT: 26.50 min Scan# 1710


Delta R.T. -0.05 min

Lab File: BE092720.D

Acq: 10 Feb 2017 14:15

Tgt Ion:	276	Resp:	259475
Ion Ratio	Lower	Upper	
276	100		
138	27.4	20.3	30.5
277	24.8	19.7	29.5









#31
Perylene-d12
Concen: 5.00 ng
RT: 24.04 min Scan# 1540
Delta R.T. -0.02 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.7	20.1	30.1
265	21.6	17.9	26.9




Manual Integrations
APPROVED


mohammad
2/13/2017 12:51:01 PM



#32
Benzo(b)fluoranthene
Concen: 4.81 ng
RT: 23.31 min Scan# 1477
Delta R.T. -0.03 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.1	18.7	28.1
125	10.8	10.5	15.7









#33
Benzo(k)fluoranthene
Concen: 5.07 ng
RT: 23.36 min Scan# 1481
Delta R.T. -0.03 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion: 252 Resp: 57137
Ion Ratio Lower Upper
252 100
253 20.5 20.3 30.5
125 10.8 9.6 14.4




Manual Integrations
APPROVED


mohammad
2/13/2017 12:51:01 PM



#34
Benzo(a)pyrene
Concen: 5.17 ng
RT: 23.93 min Scan# 1530
Delta R.T. -0.03 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion: 252 Resp: 54460
Ion Ratio Lower Upper
252 100
253 21.5 19.0 28.6
125 12.0 11.8 17.8









#35
Dibenzo(a,h)anthracene
Concen: 5.22 ng
RT: 26.51 min Scan# 1711
Delta R.T. -0.07 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Instrument :
BNA_E
ClientSampleId :
PB96821BSD

Tgt Ion	Ratio	Lower	Upper
278	100		
139	18.5	13.8	20.8
279	23.3	21.4	32.2

Manual Integrations
APPROVED

mohammad
2/13/2017 12:51:01 PM



#36
Benzo(g,h,i)perylene
Concen: 5.16 ng
RT: 27.26 min Scan# 1755
Delta R.T. -0.05 min
Lab File: BE092720.D
Acq: 10 Feb 2017 14:15

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.8	19.8	29.8
138	21.3	19.8	29.6

