


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE021017\  
 Data File : BE092717.D  
 Acq On : 10 Feb 2017 11:46  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE011617.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jan 17 10:14:01 2017

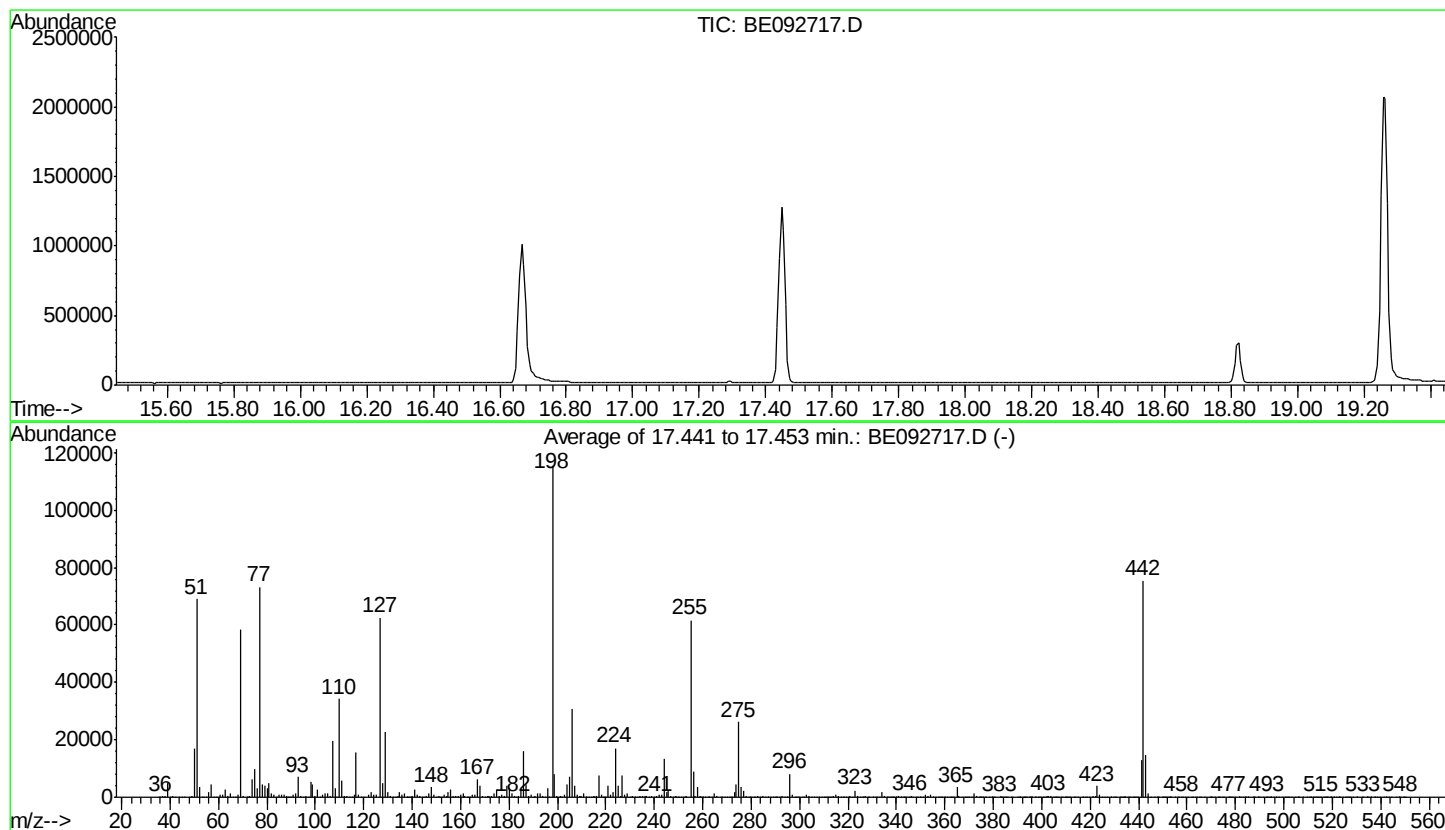

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2520

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 59.7      | 68920   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 954     | PASS             |
| 69          | 198          | 0.00         | 100          | 50.5      | 58298   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 282     | PASS             |
| 127         | 198          | 10           | 80           | 54.1      | 62441   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 115477  | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 7919    | PASS             |
| 275         | 198          | 10           | 60           | 22.6      | 26114   | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 3385    | PASS             |
| 441         | 442          | 0.01         | 24           | 17.0      | 12870   | PASS             |
| 442         | 198          | 50           | 100          | 65.4      | 75512   | PASS             |
| 443         | 442          | 15           | 24           | 19.7      | 14854   | PASS             |