

Data Path : Z:\HPCHEM1\BNA E\DATA\BE021318\
 Data File : BE095668.D
 Acq On : 12 Feb 2018 19:08
 Operator : SJ/JU
 Sample : PB106445BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 13 03:27:41 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE020618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 20:27:34 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	1042	0.40	ng	0.00
7) Naphthalene-d8	11.26	136	3901	0.40	ng	-0.02
13) Acenaphthene-d10	15.00	164	2158	0.40	ng	0.00
19) Phenanthrene-d10	17.71	188	5037	0.40	ng	0.00
27) Chrysene-d12	21.79	240	5187	0.40	ng	0.00
34) Perylene-d12	24.43	264	5030	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.92	112	1171	0.37	ng	0.00
5) Phenol-d6	7.56	99	1508	0.35	ng	0.00
8) Nitrobenzene-d5	9.62	82	1413	0.34	ng	0.00
11) 2-Methylnaphthalene-d10	12.80	152	2411	0.37	ng	0.00
14) 2,4,6-Tribromophenol	16.47	330	233	0.24	ng	0.00
15) 2-Fluorobiphenyl	13.64	172	3394	0.36	ng	-0.02
25) Fluoranthene-d10	19.69	212	24055	0.36	ng	0.00
29) Terphenyl-d14	20.25	244	3825	0.35	ng	0.00
Target Compounds						
22) Pentachlorophenol	17.37	266	4	0.17	ng	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE021318\
Data File : BE095668.D
Acq On : 12 Feb 2018 19:08
Operator : SJ/JU
Sample : PB106445BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 13 03:27:41 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE020618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 20:27:34 2018
Response via : Initial Calibration

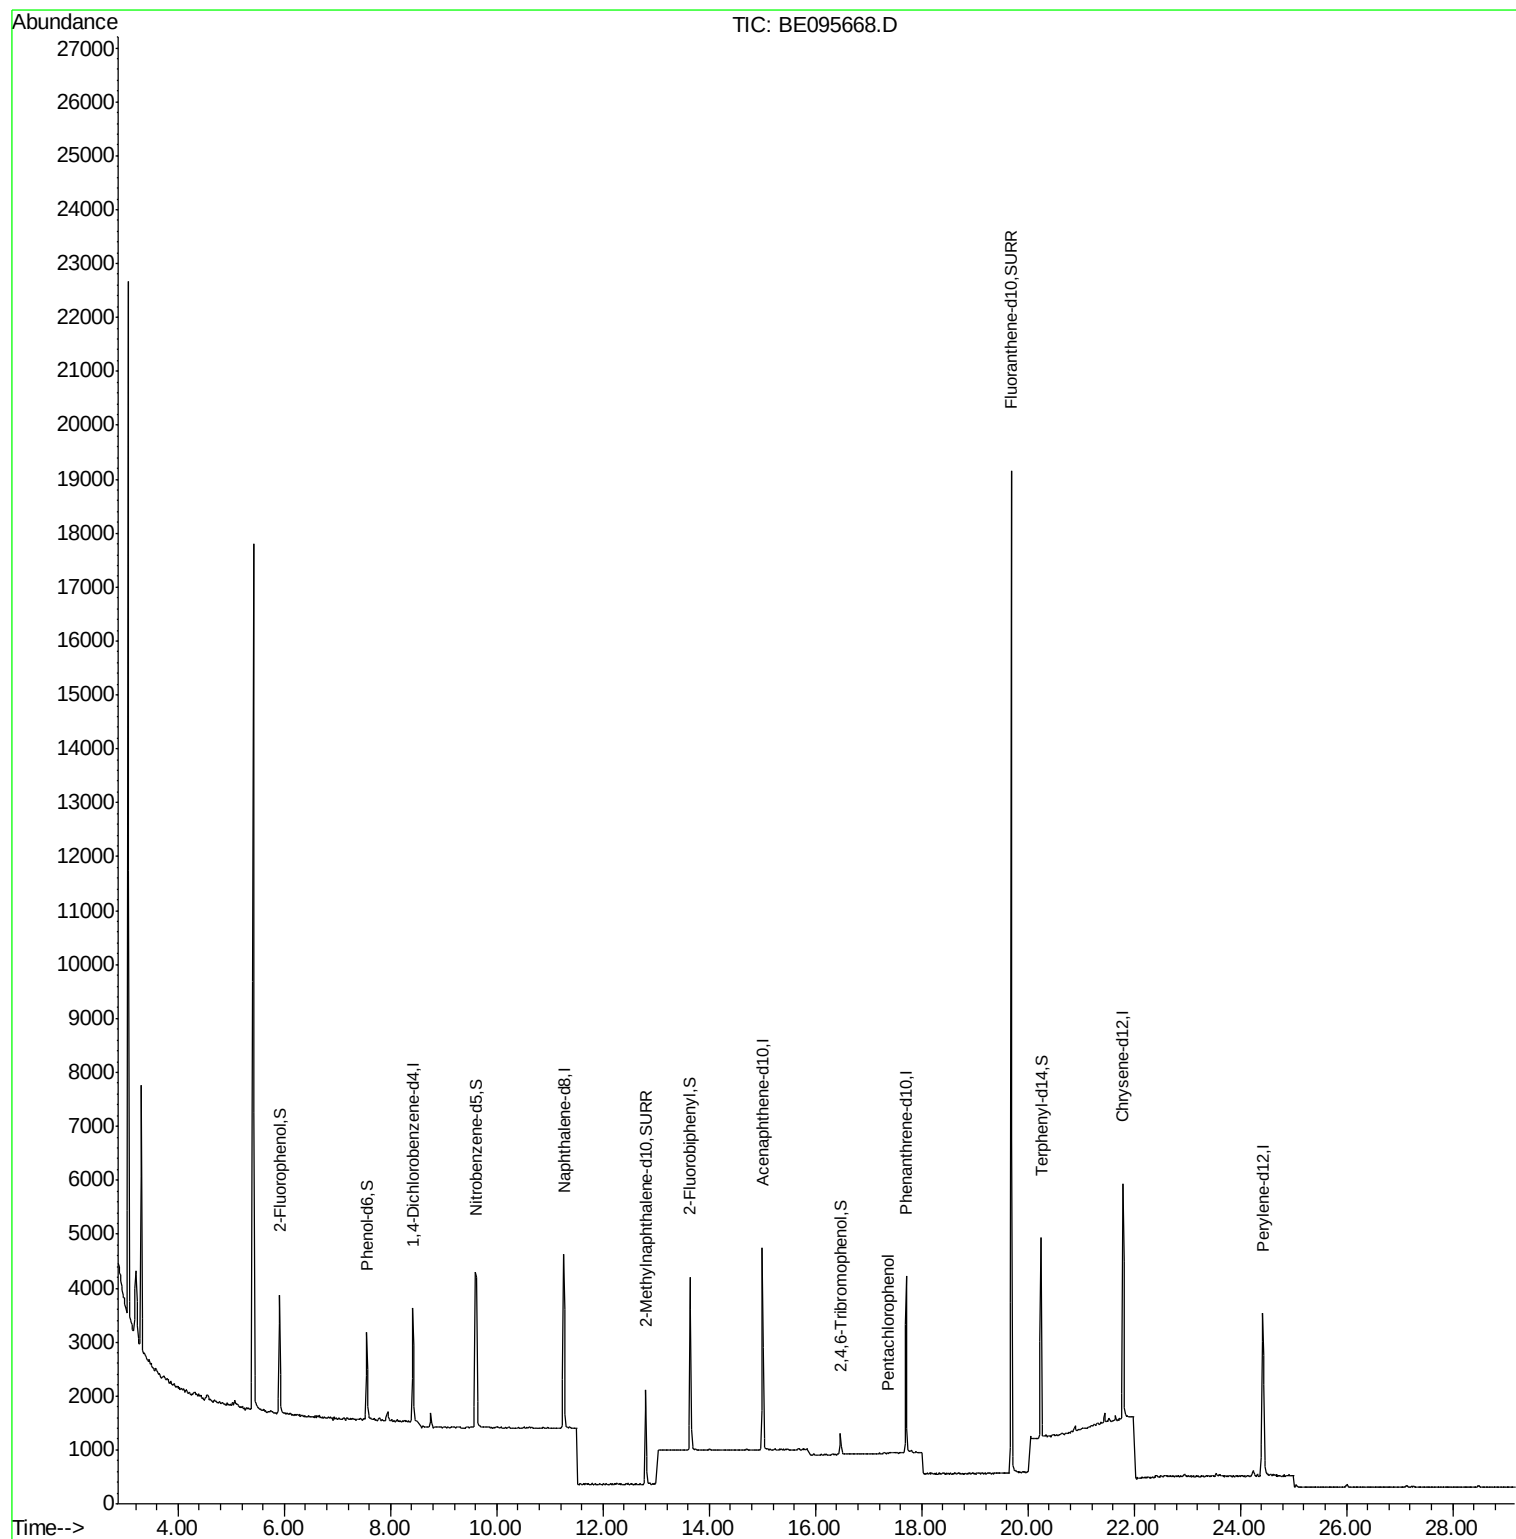

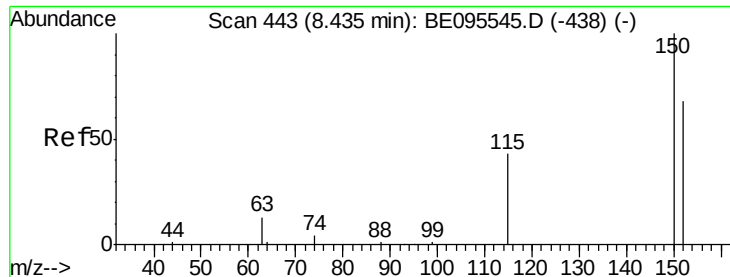

#1

1,4-Dichlorobenzene-d4

Concen: 0.40 ng

RT: 8.42 min Scan# 442

Delta R.T. -0.01 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 1042

Ion Ratio Lower Upper

152 100

150 145.2 117.2 175.8




115 68.6 57.0 85.6

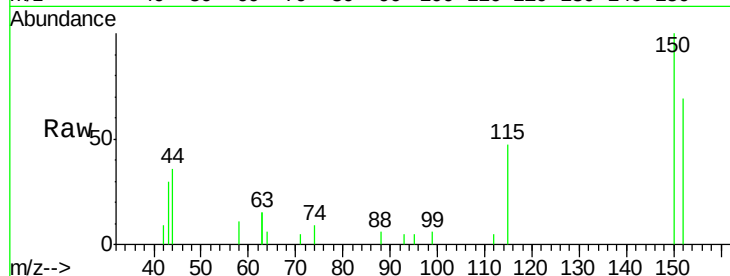

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

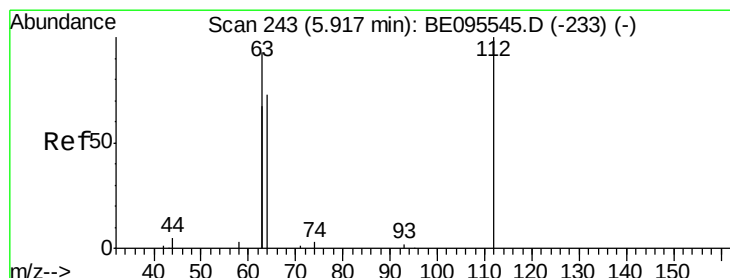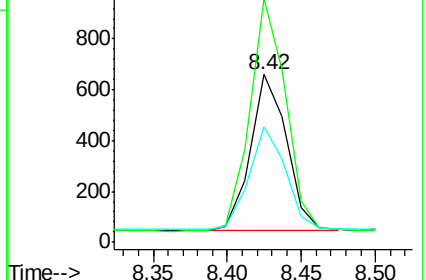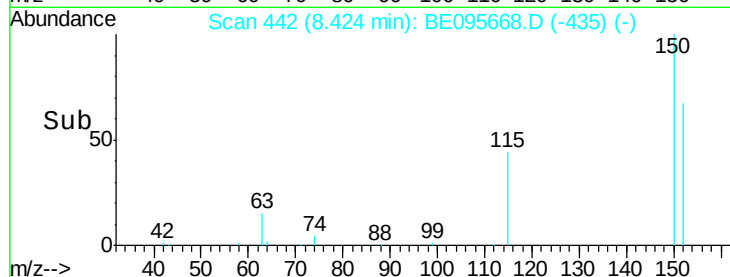

#4

2-Fluorophenol

Concen: 0.37 ng

RT: 5.92 min Scan# 243

Delta R.T. 0.00 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08


Tgt Ion:112 Resp: 1171

Ion Ratio Lower Upper

112 100

64 72.2 60.1 90.1



63 155.3 116.8 175.2

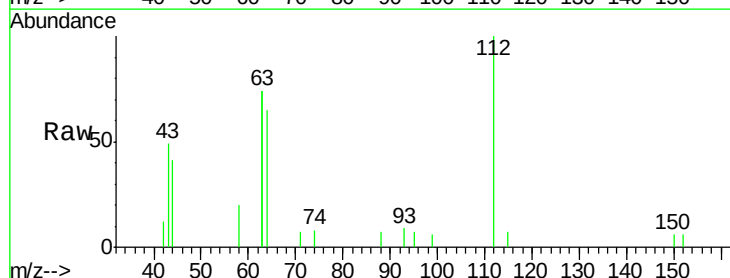


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

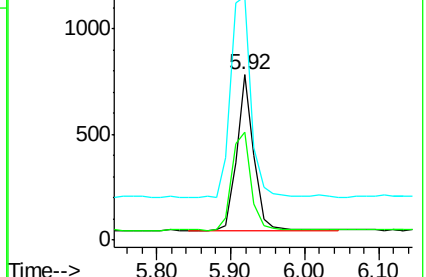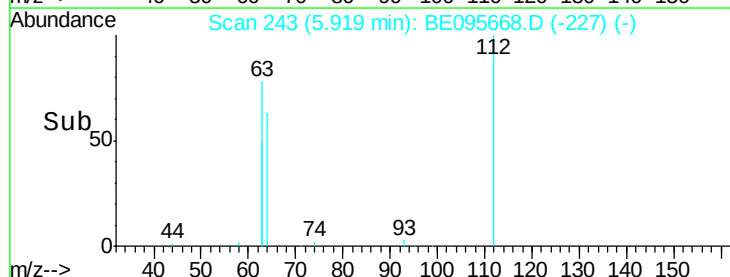



#5

Phenol-d6

Concen: 0.35 ng

RT: 7.56 min Scan# 373

Delta R.T. -0.01 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 99 Resp: 1508

Ion Ratio Lower Upper

99 100

42 25.3 20.2 30.2




71 39.7 28.4 42.6

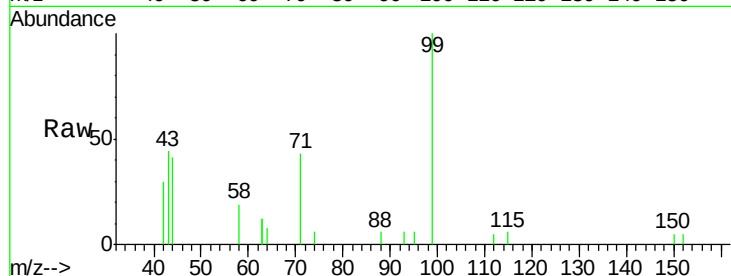

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

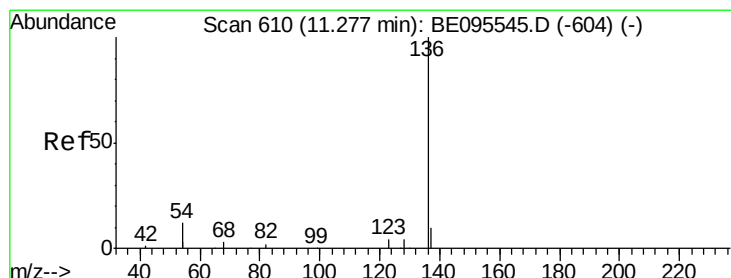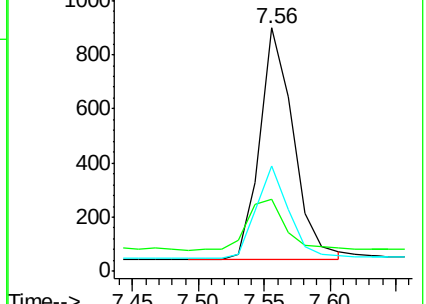

#7

Naphthalene-d8

Concen: 0.40 ng

RT: 11.26 min Scan# 609

Delta R.T. -0.02 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08

Tgt Ion: 136 Resp: 3901


Ion Ratio Lower Upper

136 100

137 12.6 9.5 14.3

54 65.2 29.1 43.7#

68 12.2 6.2 9.2#


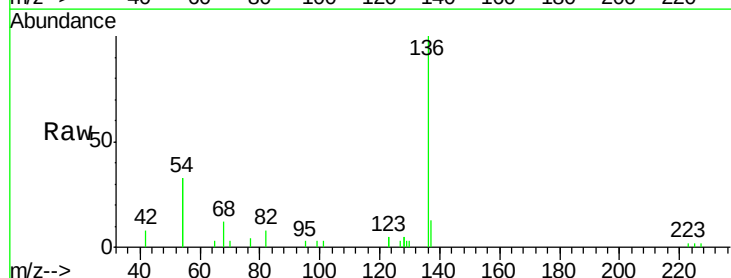



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



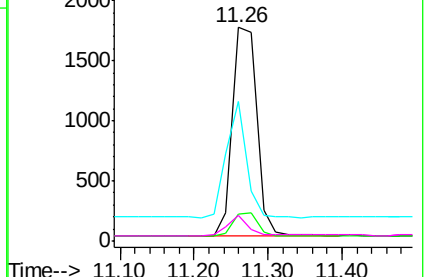





#8
 Nitrobenzene-d5
 Concen: 0.34 ng
 RT: 9.62 min Scan# 511
 Delta R.T. 0.00 min
 Lab File: BE095668.D
 Acq: 12 Feb 2018 19:08




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion	82	Resp	1413
Ion Ratio	Lower	Upper	
82	100		
128	177.2	150.0	225.0
54	191.5	154.2	231.4

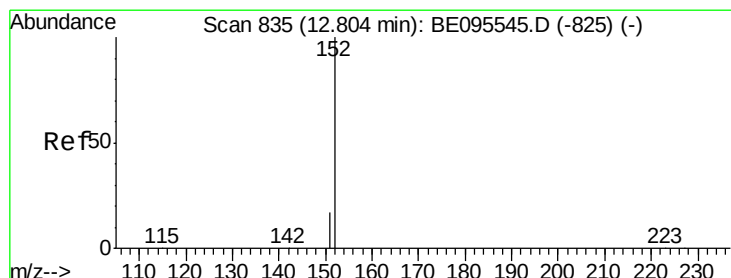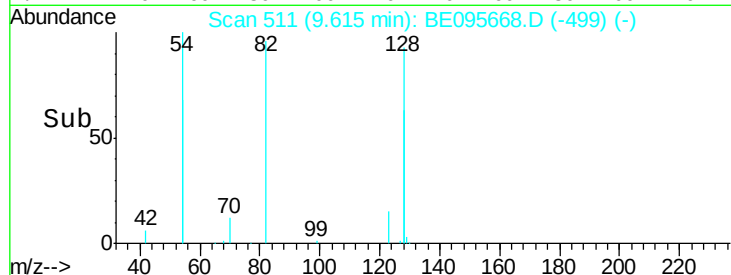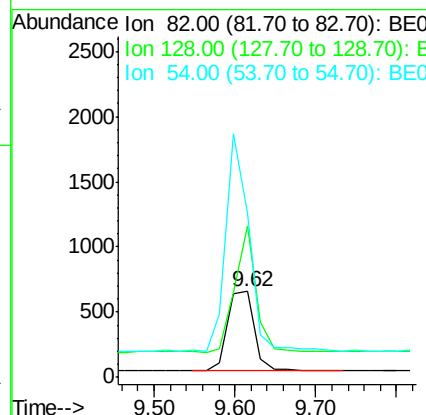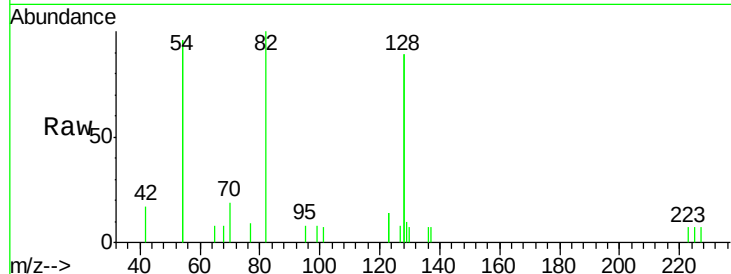

#11
 2-Methylnaphthalene-d10
 Concen: 0.37 ng
 RT: 12.80 min Scan# 835
 Delta R.T. -0.00 min
 Lab File: BE095668.D
 Acq: 12 Feb 2018 19:08

Tgt Ion	152	Resp	2411
Ion Ratio	Lower	Upper	
152	100		
151	19.6	15.4	23.0

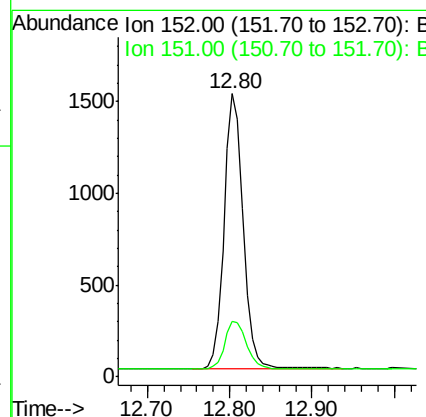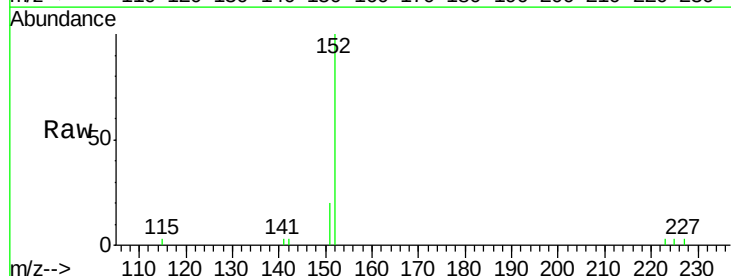

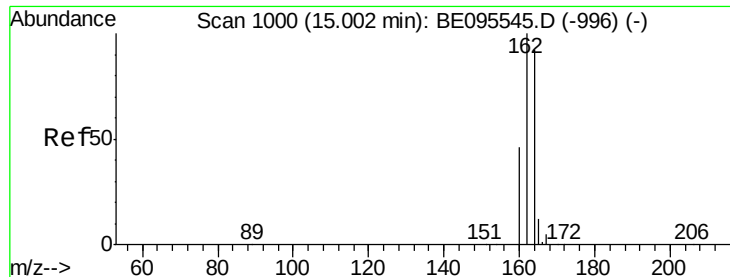

#13

Acenaphthene-d10

Concen: 0.40 ng

RT: 15.00 min Scan# 1000

Delta R.T. -0.00 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08

Instrument :

BNA_E

ClientSampleId :


Tot Ion:164 Resp: 2158

Ion Ratio Lower Upper

164 100

162 110.0 83.1 124.7




160 51.5 37.1 55.7

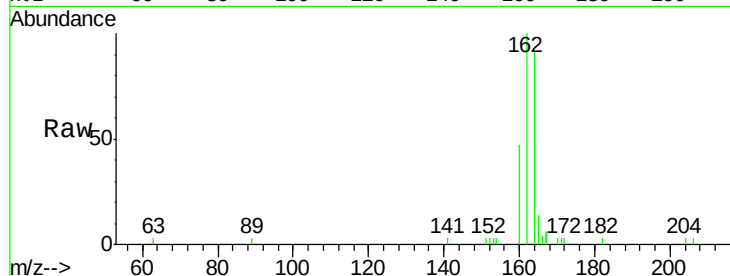

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

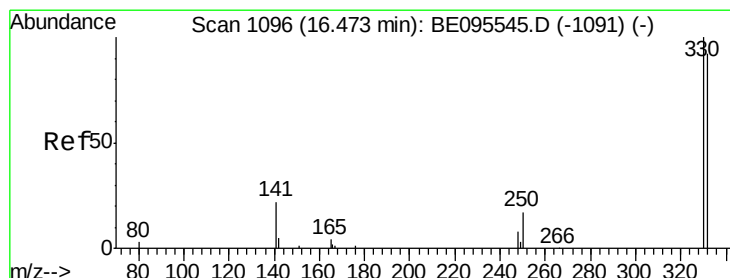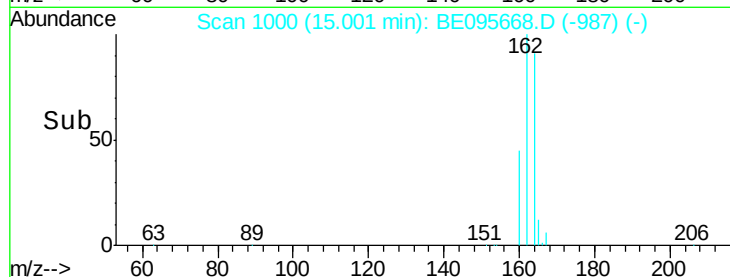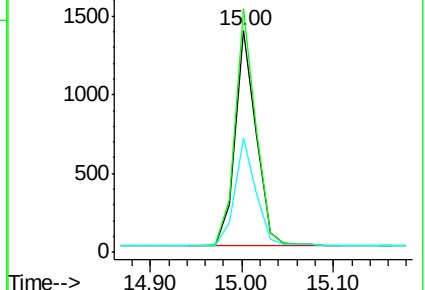

#14

2,4,6-Tribromophenol

Concen: 0.24 ng

RT: 16.47 min Scan# 1096

Delta R.T. 0.00 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08


Tgt Ion:330 Resp: 233

Ion Ratio Lower Upper

330 100

332 106.4 152.7 229.1#



141 48.9 33.7 50.5

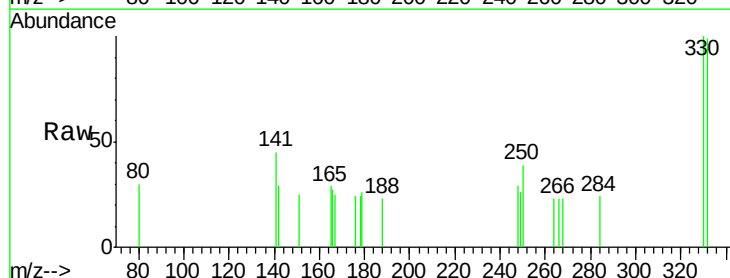


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

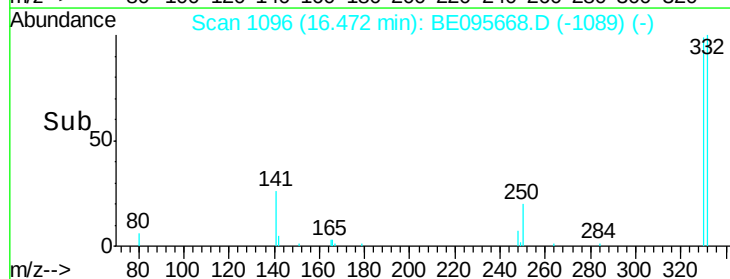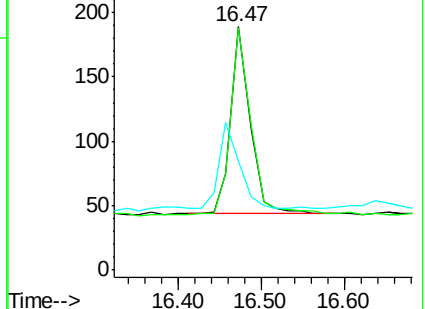


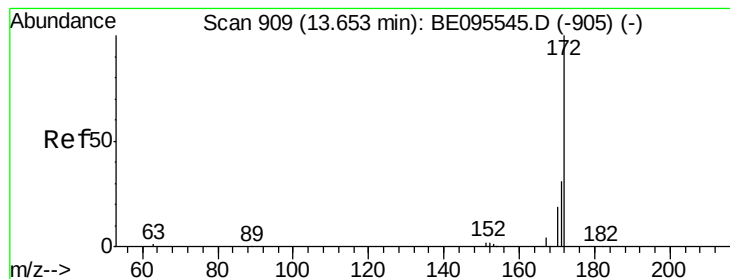




#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 13.64 min Scan# 908
Delta R.T. -0.02 min
Lab File: BE095668.D
Acq: 12 Feb 2018 19:08

Instrument :
BNA_E
ClientSampleId :

Tot Ion:172 Resp: 3394
Ion Ratio Lower Upper
172 100
171 38.9 29.9 44.9
170 27.3 21.8 32.8

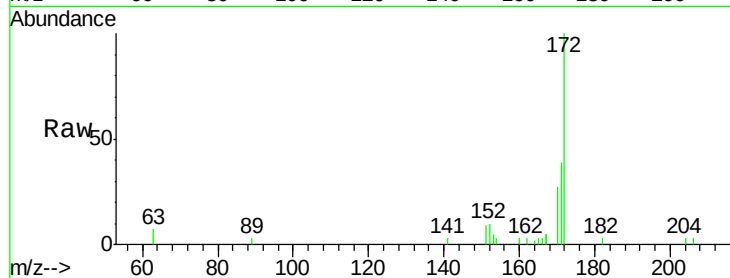


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

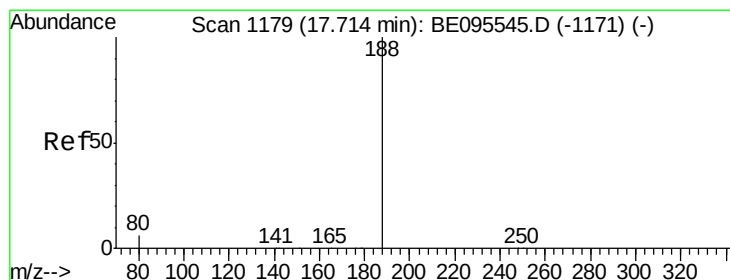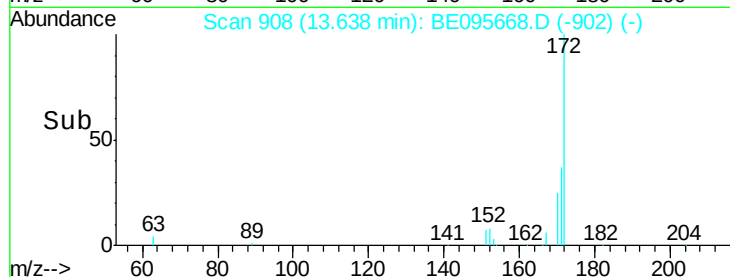
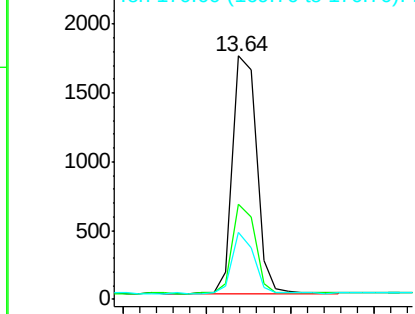



#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.71 min Scan# 1179
Delta R.T. 0.00 min
Lab File: BE095668.D
Acq: 12 Feb 2018 19:08

Tgt Ion:188 Resp: 5037
Ion Ratio Lower Upper
188 100
94 0.0 3.9 5.9#
80 7.5 3.6 5.4#

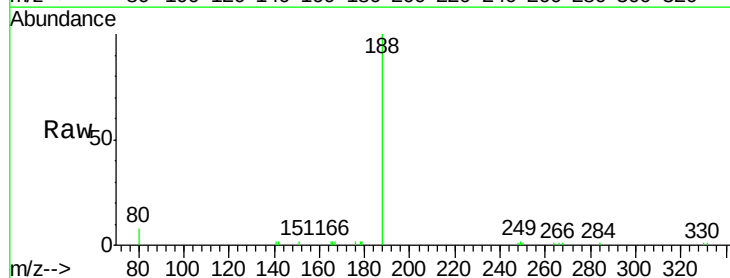

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0



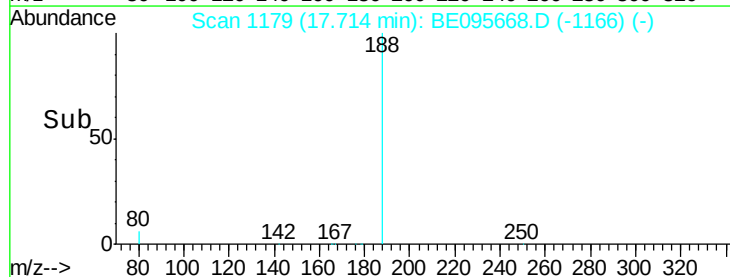
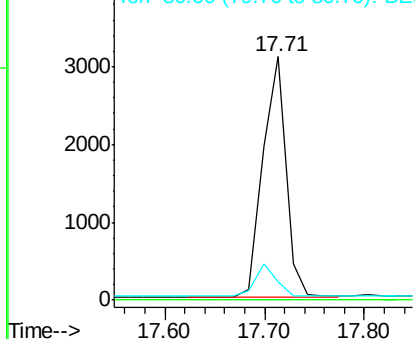




#22
 Pentachlorophenol
 Concen: 0.17 ng
 RT: 17.37 min Scan# 1156
 Delta R.T. 0.00 min
 Lab File: BE095668.D
 Acq: 12 Feb 2018 19:08




Instrument :
 BNA_E
 ClientSampled :


Tot Ion:266 Resp: 4
 Ion Ratio Lower Upper
 266 100
 264 97.8 72.5 108.7
 268 102.2 73.8 110.6

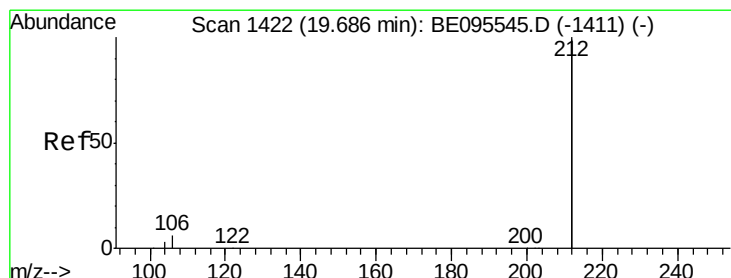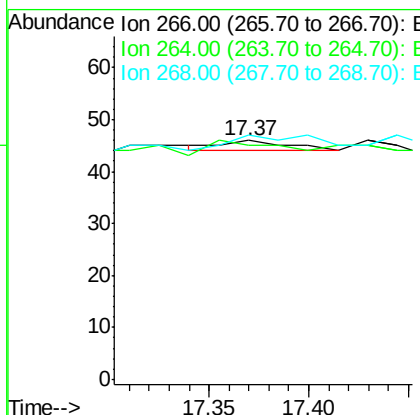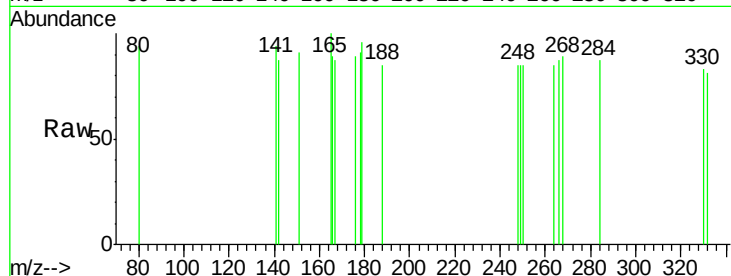

#25
 Fluoranthene-d10
 Concen: 0.36 ng
 RT: 19.69 min Scan# 1422
 Delta R.T. 0.00 min
 Lab File: BE095668.D
 Acq: 12 Feb 2018 19:08

Tgt Ion:212 Resp: 24055
 Ion Ratio Lower Upper
 212 100
 106 2.9 2.8 4.2
 104 1.7 1.6 2.4

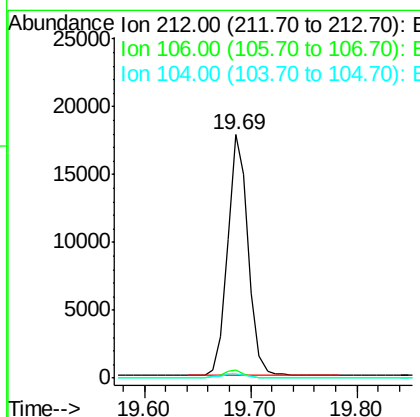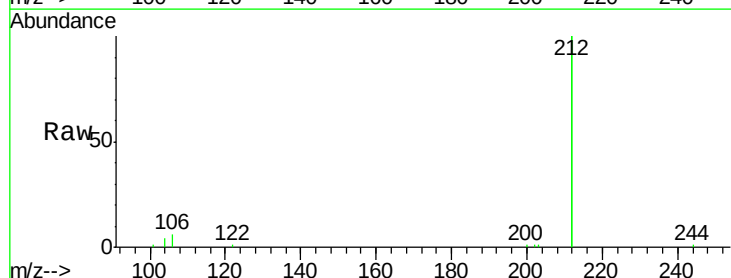

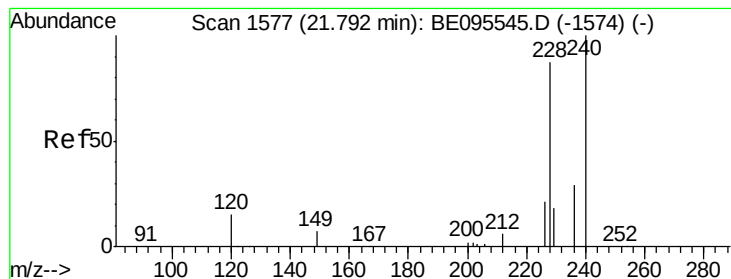

#27

Chrysene-d12

Concen: 0.40 ng

RT: 21.79 min Scan# 1577

Delta R.T. -0.00 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08

Instrument :

BNA_E

ClientSampleId :


Tot Ion:240 Resp: 5187

Ion Ratio Lower Upper

240 100

120 14.8 5.5 8.3#




236 29.4 20.7 31.1

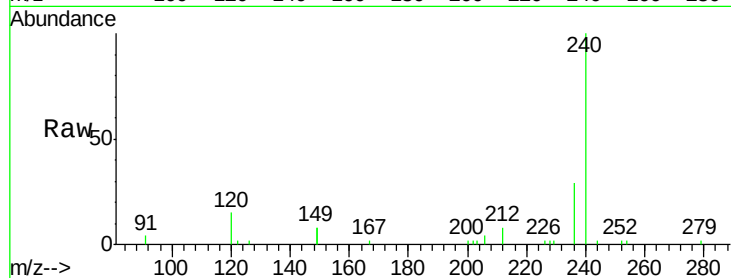

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

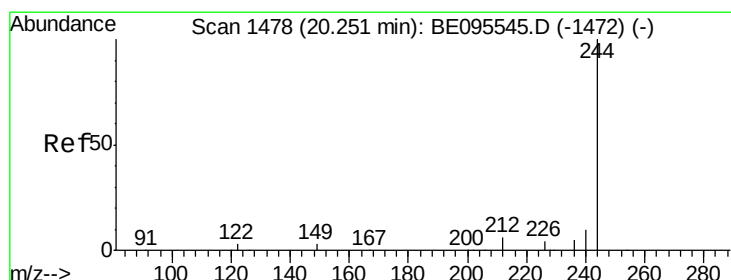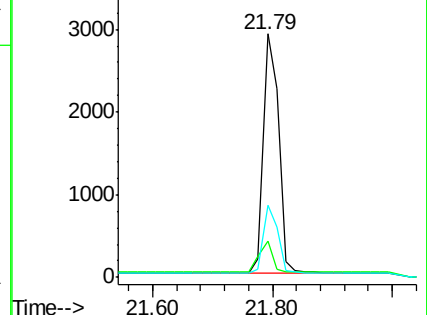

#29

Terphenyl-d14

Concen: 0.35 ng

RT: 20.25 min Scan# 1478

Delta R.T. -0.00 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08


Tgt Ion:244 Resp: 3825

Ion Ratio Lower Upper

244 100

212 8.0 25.4 38.0#



122 4.4 8.1 12.1#



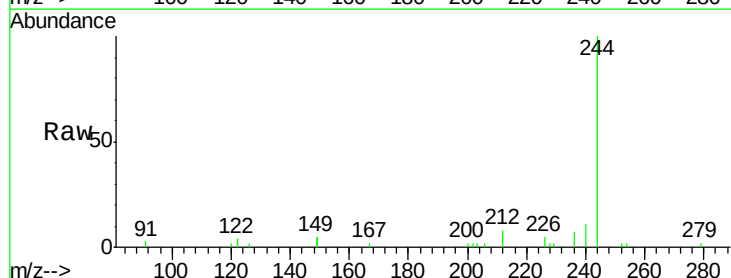


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

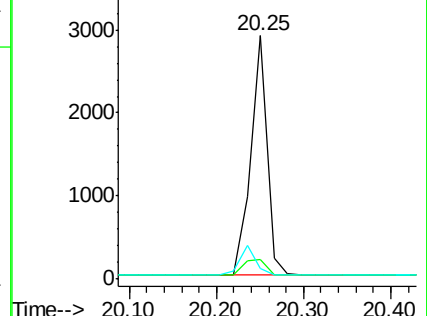

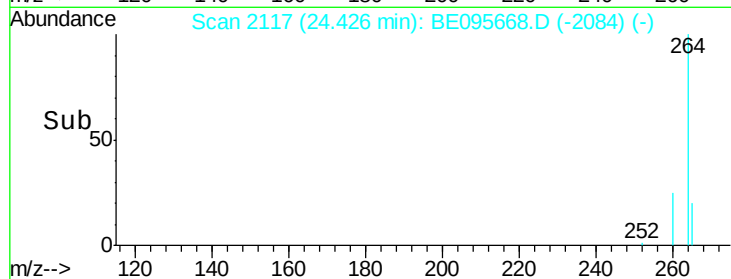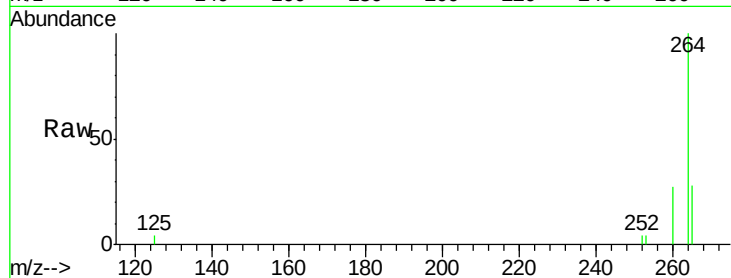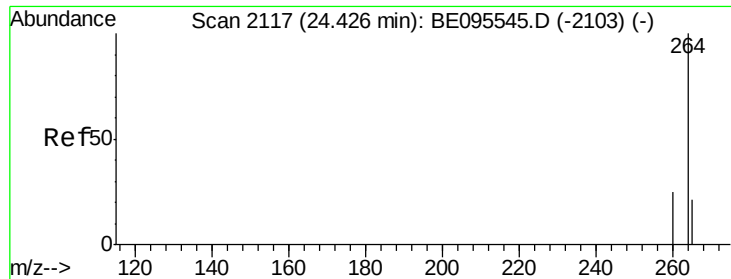

#34

Pervlene-d12

Concen: 0.40 ng

RT: 24.43 min Scan# 2117

Delta R.T. -0.00 min

Lab File: BE095668.D

Acq: 12 Feb 2018 19:08

Instrument :

BNA_E

ClientSampleId :

Tot Ion:264 Resp: 5030

Ion Ratio Lower Upper

264 100

260 26.9 20.5 30.7

265 28.3 22.8 34.2

