
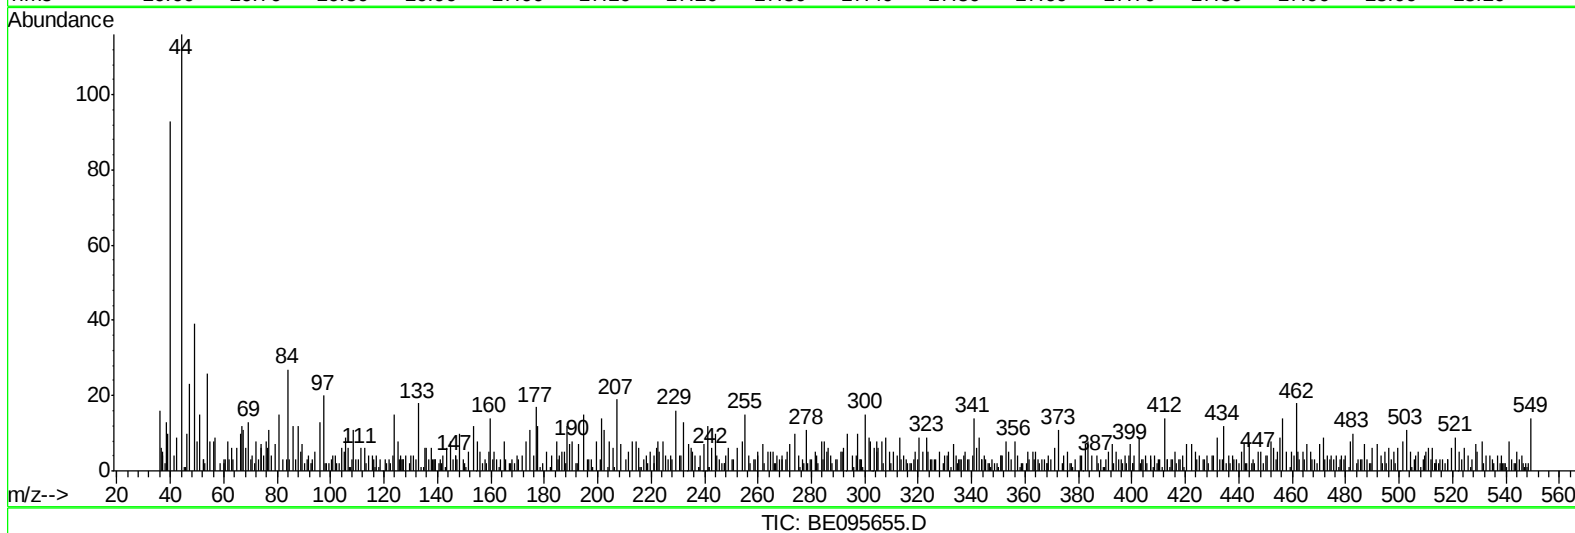


Data Path : Z:\HPCHEM1\BNA E\DATA\BE021318\
 Data File : BE095655.D
 Acq On : 12 Feb 2018 11:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 04:34:10 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 12:44:16 2018
 Response via : Initial Calibration

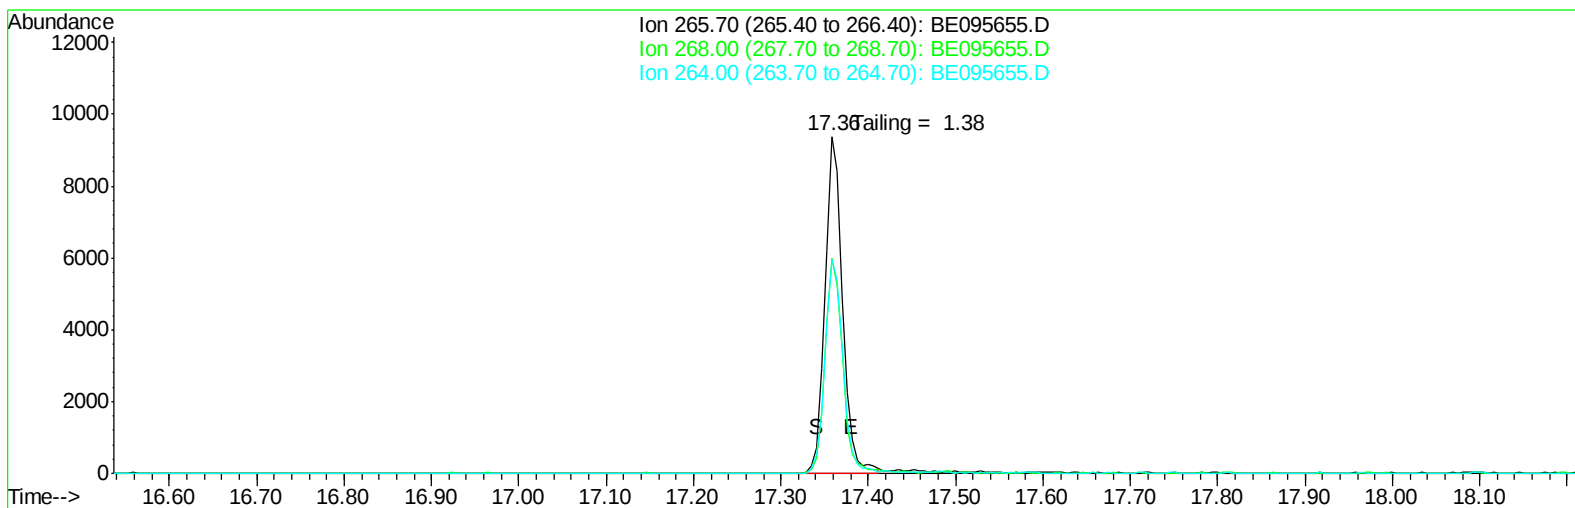

TIC: BE095655.D

(69) Pentachlorophenol (C)



10.907min (-0.303) 104.27ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	42.86#
264.00	61.90	142.86#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE021318\
Data File : BE095655.D
Acq On : 12 Feb 2018 11:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 04:34:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

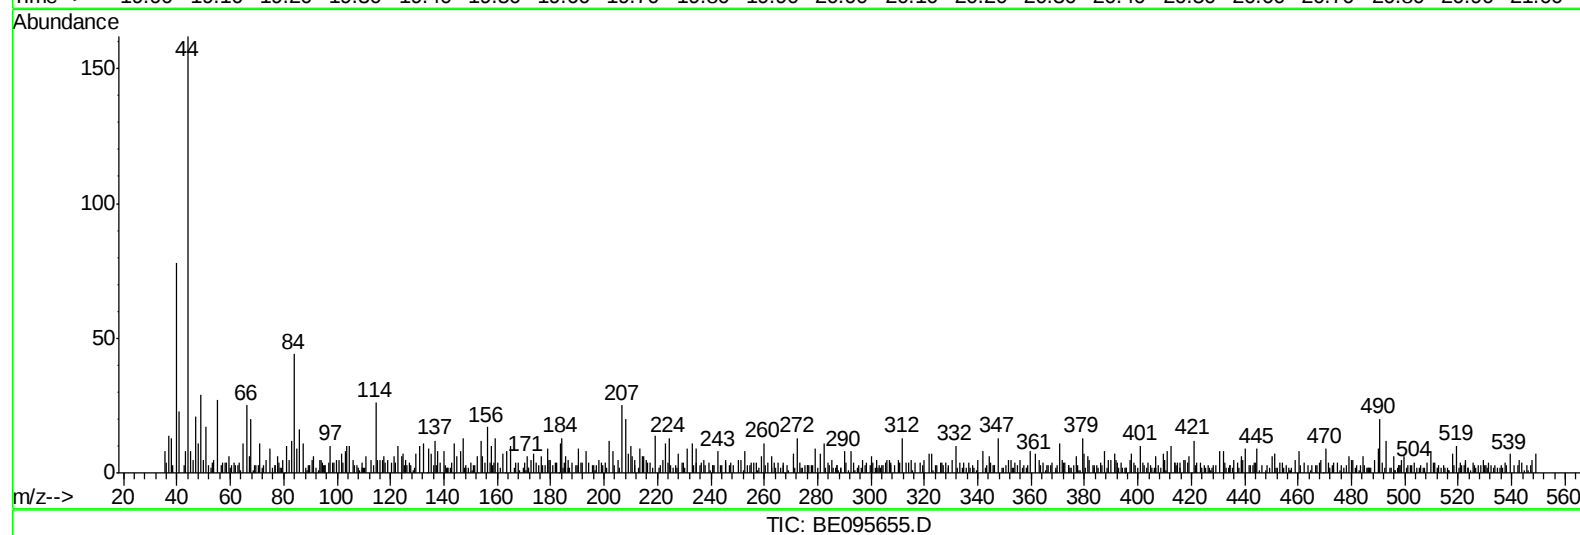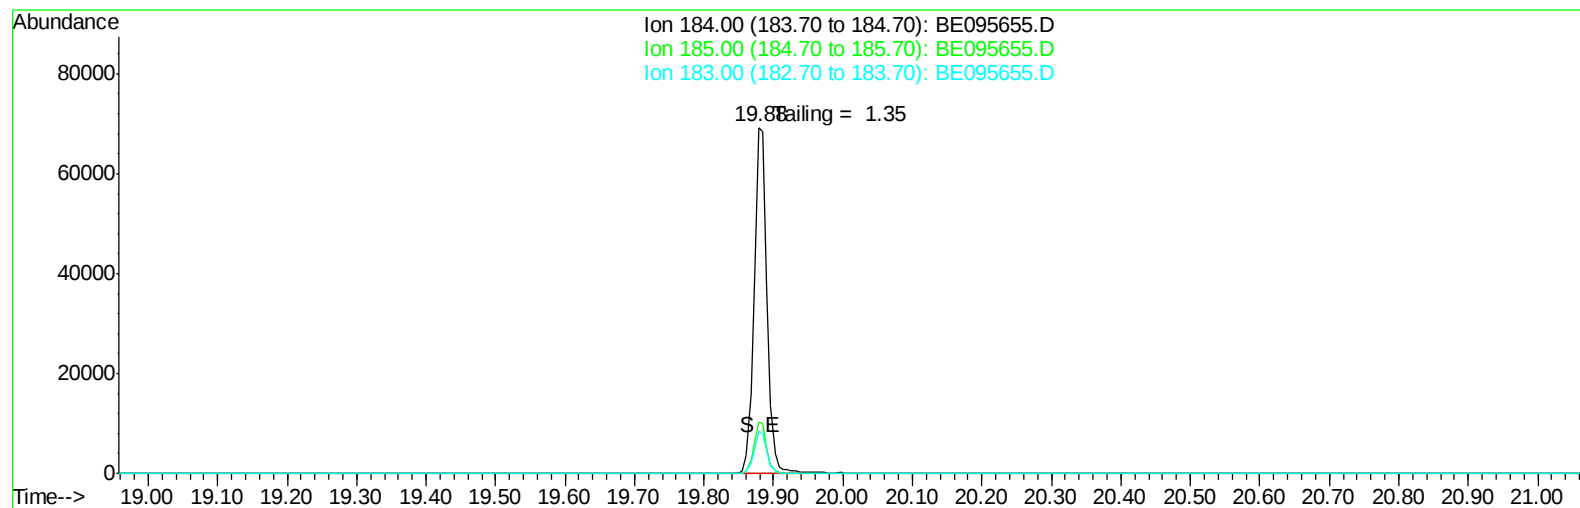

(76) Benzidine

12.405min (-0.334) 65.27ng

response 6

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	66.67#
183.00	11.60	73.33#
0.00	0.00	0.00