


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE021318\
Data File : BE095655.D
Acq On : 12 Feb 2018 11:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020618.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 06 20:27:34 2018

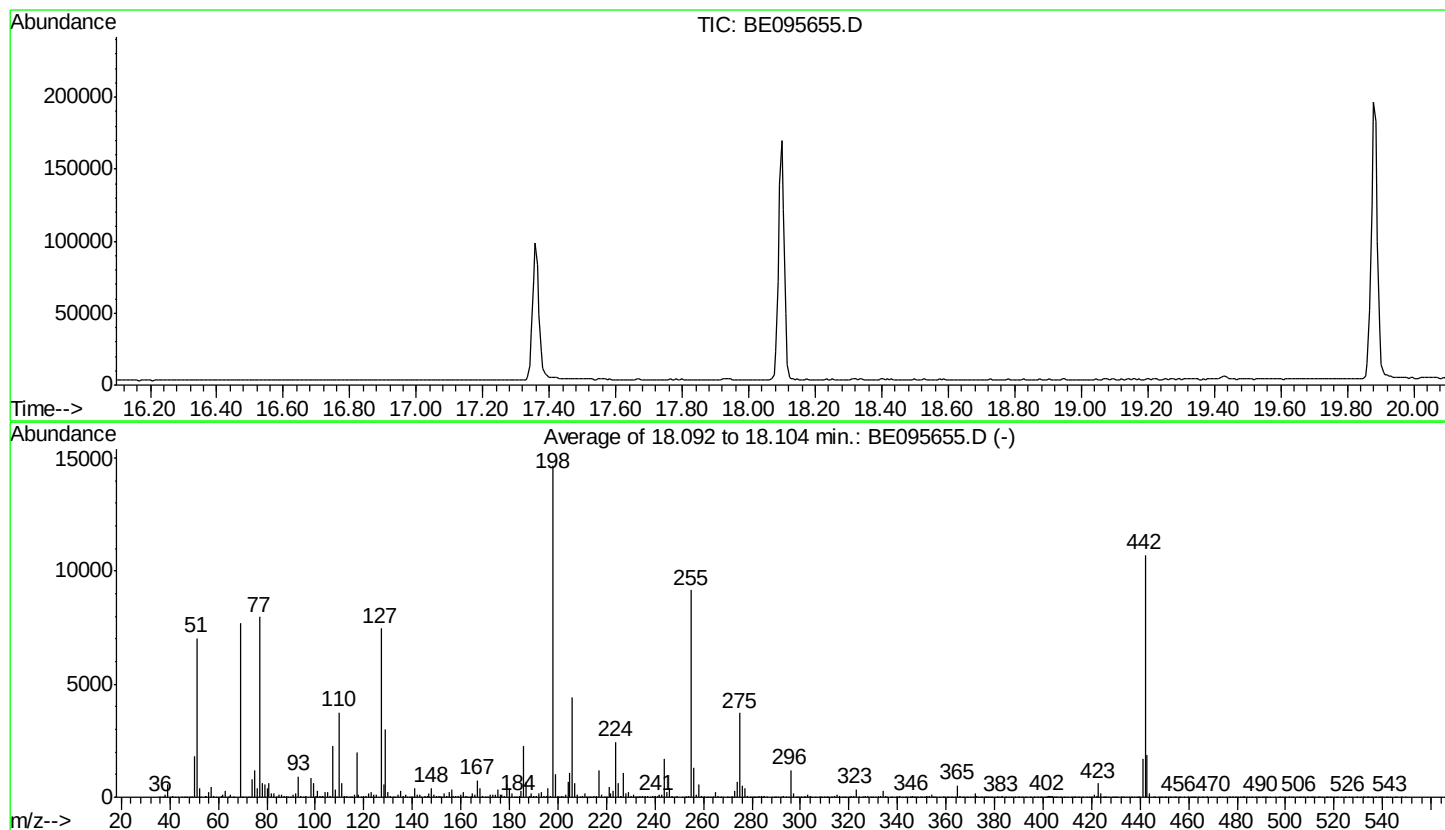

AutoFind: Scans 2639, 2640, 2641; Background Corrected with Scan 2631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	7028	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.4	7688	PASS
70	69	0.00	2	0.4	30	PASS
127	198	10	80	50.9	7461	PASS
197	198	0.00	2	0.3	38	PASS
198	198	100	100	100.0	14670	PASS
199	198	5	9	6.8	997	PASS
275	198	10	60	25.4	3727	PASS
365	198	1	100	3.6	524	PASS
441	442	0.01	24	15.8	1691	PASS
442	198	50	100	73.0	10712	PASS
443	442	15	24	17.7	1891	PASS