


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021517\
 Data File : BE092727.D
 Acq On : 15 Feb 2017 11:09
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE021517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 15 17:05:20 2017

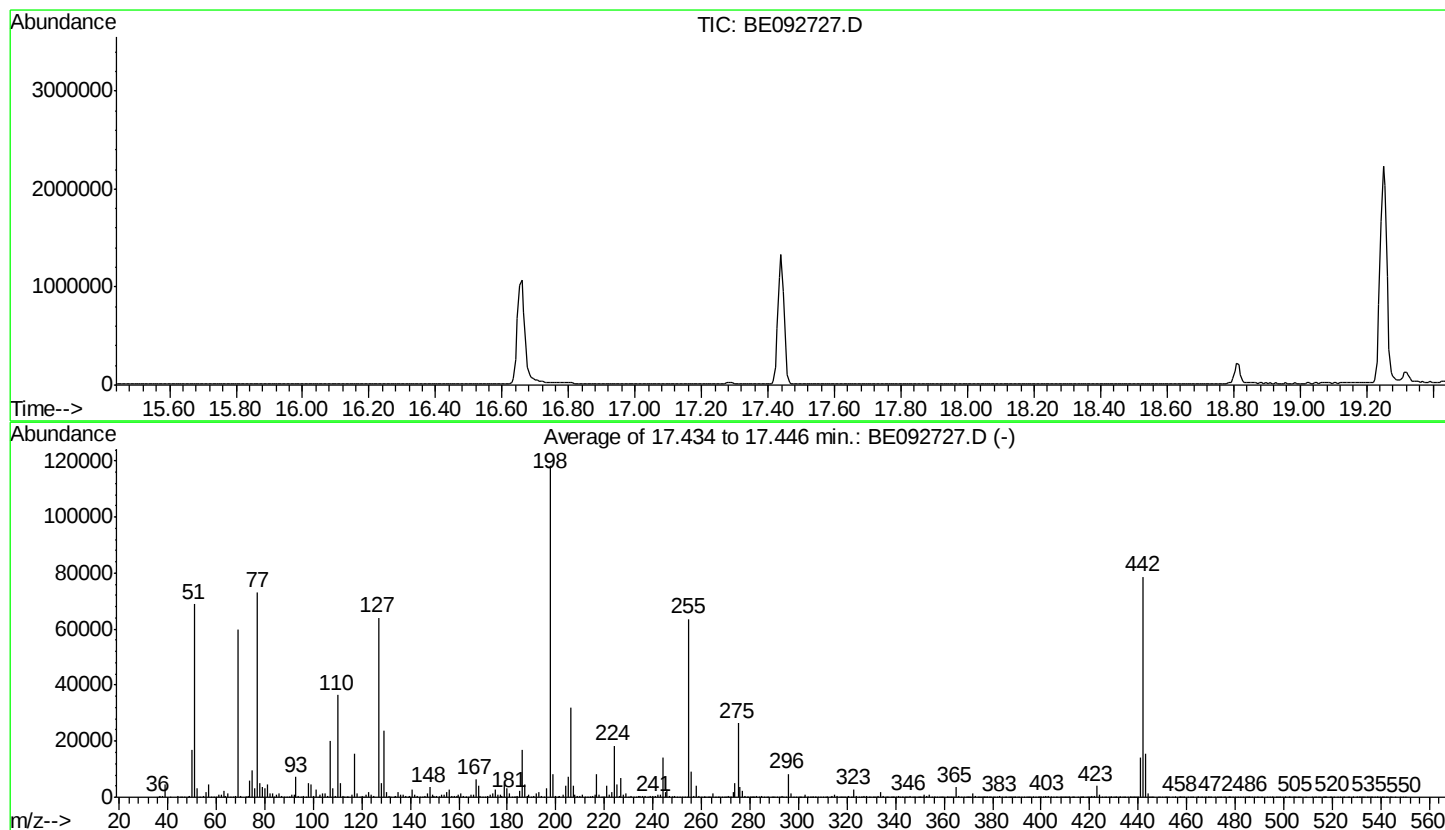

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	68766	PASS
68	69	0.00	2	0.8	509	PASS
69	198	0.00	100	50.7	59985	PASS
70	69	0.00	2	0.4	259	PASS
127	198	10	80	54.1	64066	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118323	PASS
199	198	5	9	7.1	8358	PASS
275	198	10	60	22.2	26288	PASS
365	198	1	100	3.0	3522	PASS
441	442	0.01	24	18.1	14286	PASS
442	198	50	100	66.5	78722	PASS
443	442	15	24	19.8	15603	PASS