


Data Path : Z:\HPCHEM1\BNA E\Data\BE021615\
 Data File : BE089568.D
 Acq On : 16 Feb 2015 11:48
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE021615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 17 03:31:44 2015

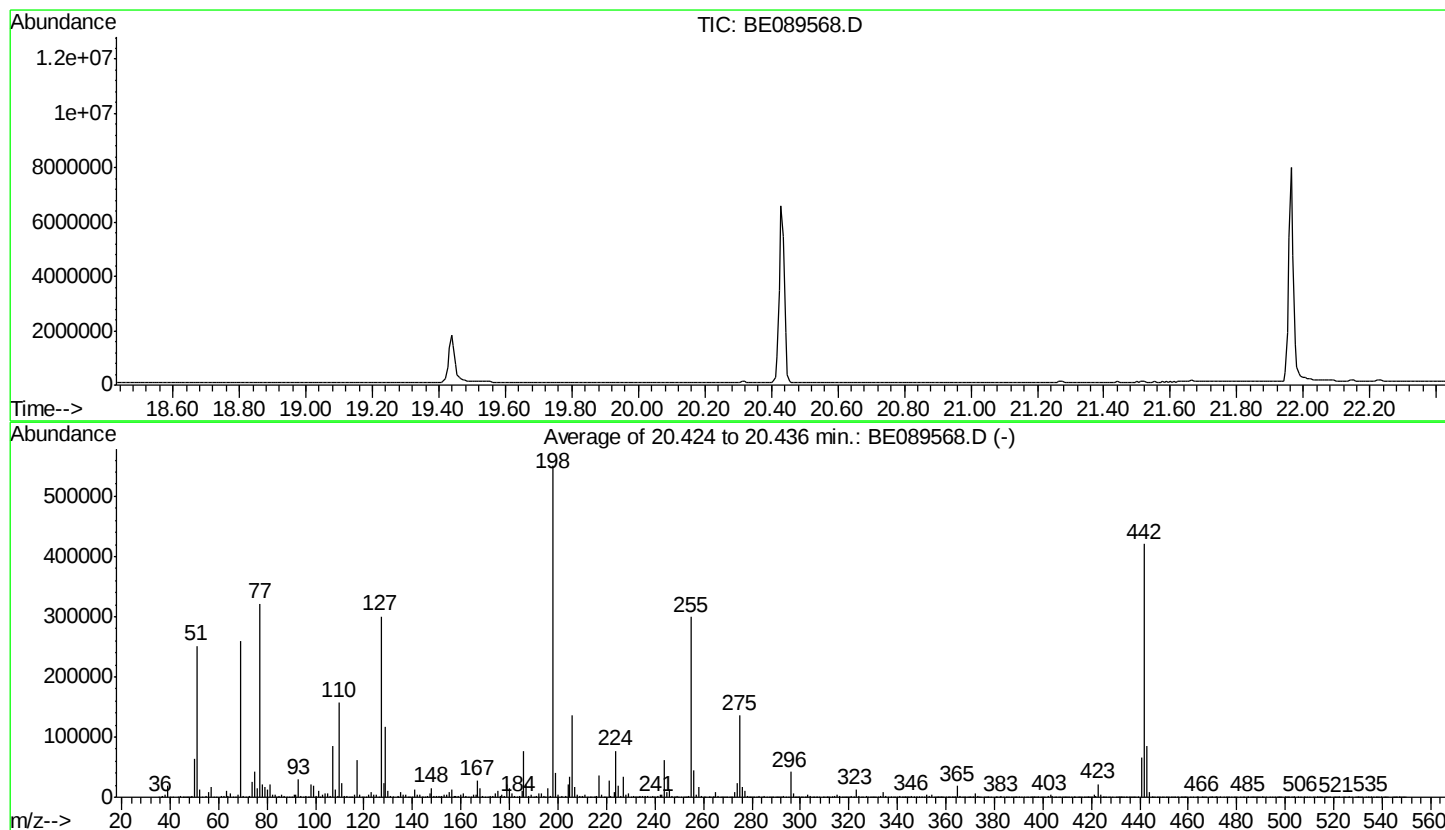

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3231

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	251448	PASS
68	69	0.00	2	1.7	4397	PASS
69	198	0.00	100	47.1	259626	PASS
70	69	0.00	2	0.6	1565	PASS
127	198	10	80	54.6	300609	PASS
197	198	0.00	2	0.2	1374	PASS
198	198	100	100	100.0	550861	PASS
199	198	5	9	7.2	39531	PASS
275	198	10	60	24.6	135468	PASS
365	198	1	100	3.4	18585	PASS
441	442	0.01	24	15.7	66048	PASS
442	198	50	100	76.4	420680	PASS
443	442	15	24	20.2	84933	PASS