

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021715\
 Data File : BE089596.D
 Acq On : 17 Feb 2015 15:49
 Operator : TP/IZ
 Sample : SSTDICC0.5
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTDICC0.5

Quant Time: Feb 18 01:21:53 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE021715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 18 00:56:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.34	152	56847	5.00	ng	0.00
7) Naphthalene-d8	12.24	136	223170	5.00	ng	0.00
13) Acenaphthene-d10	16.42	164	106357	5.00	ng	0.00
17) Phenanthrene-d10	19.77	188	208337	5.00	ng	0.00
20) Chrysene-d12	23.66	240	226882	5.00	ng	0.00
27) Perylene-d12	25.34	264	202710	5.00	ng	0.00

System Monitoring Compounds						
3) 2-Fluorophenol	6.50	112	7125	0.45	ng	0.00
4) Phenol-d6	8.62	99	9288	0.44	ng	0.00
8) Nitrobenzene-d5	10.61	82	4206	0.46	ng	0.00
14) 2,4,6-Tribromophenol	18.31	330	788	0.36	ng	0.00
15) 2-Fluorobiphenyl	14.88	172	13895	0.49	ng	0.00
22) Terphenyl-d14	22.30	244	13922	0.45	ng	0.00


Target Compounds				Qvalue		
2) n-Nitrosodimethylamine	3.38	42	3339m	0.41	ng	
5) Phenol	8.65	94	10122	0.44	ng	92
6) bis(2-Chloroethyl)ether	8.83	93	8159	0.47	ng	# 99
9) Nitrobenzene	10.65	77	4986	0.46	ng	98
10) 2,4-Dimethylphenol	11.58	122	5176	0.41	ng	97
11) 2,4-Dichlorophenol	11.96	162	4140	0.42	ng	97
12) Hexachlorobutadiene	12.63	225	3350	0.49	ng	99
16) 2,4-Dinitrophenol	16.67	184	129	0.34	ng	# 82
18) Hexachlorobenzene	18.99	284	4350	0.49	ng	96
19) Pentachlorophenol	19.44	266	531	0.36	ng	95
21) Benzidine	21.96	184	5119	0.30	ng	98
23) Benzo(a)anthracene	23.64	228	85345	0.40	ng	99
24) 3,3'-Dichlorobenzidine	23.63	252	3485	0.25	ng	99
25) Chrysene	23.69	228	106918	0.49	ng	99
26) Indeno(1,2,3-cd)pyrene	26.74	276	15082	0.31	ng	# 97
28) Benzo(b)fluoranthene	24.92	252	11658	0.31	ng	99
29) Benzo(k)fluoranthene	24.94	252	25186	0.46	ng	99
30) Benzo(a)pyrene	25.28	252	11220	0.31	ng	99
31) Dibenzo(a,h)anthracene	26.78	278	11543	0.32	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021715\
Data File : BE089596.D
Acq On : 17 Feb 2015 15:49
Operator : TP/IZ
Sample : SSTDICC0.5
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
LabSampleId :
SSTDICC0.5

Quant Time: Feb 18 01:21:53 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 00:56:39 2015
Response via : Initial Calibration

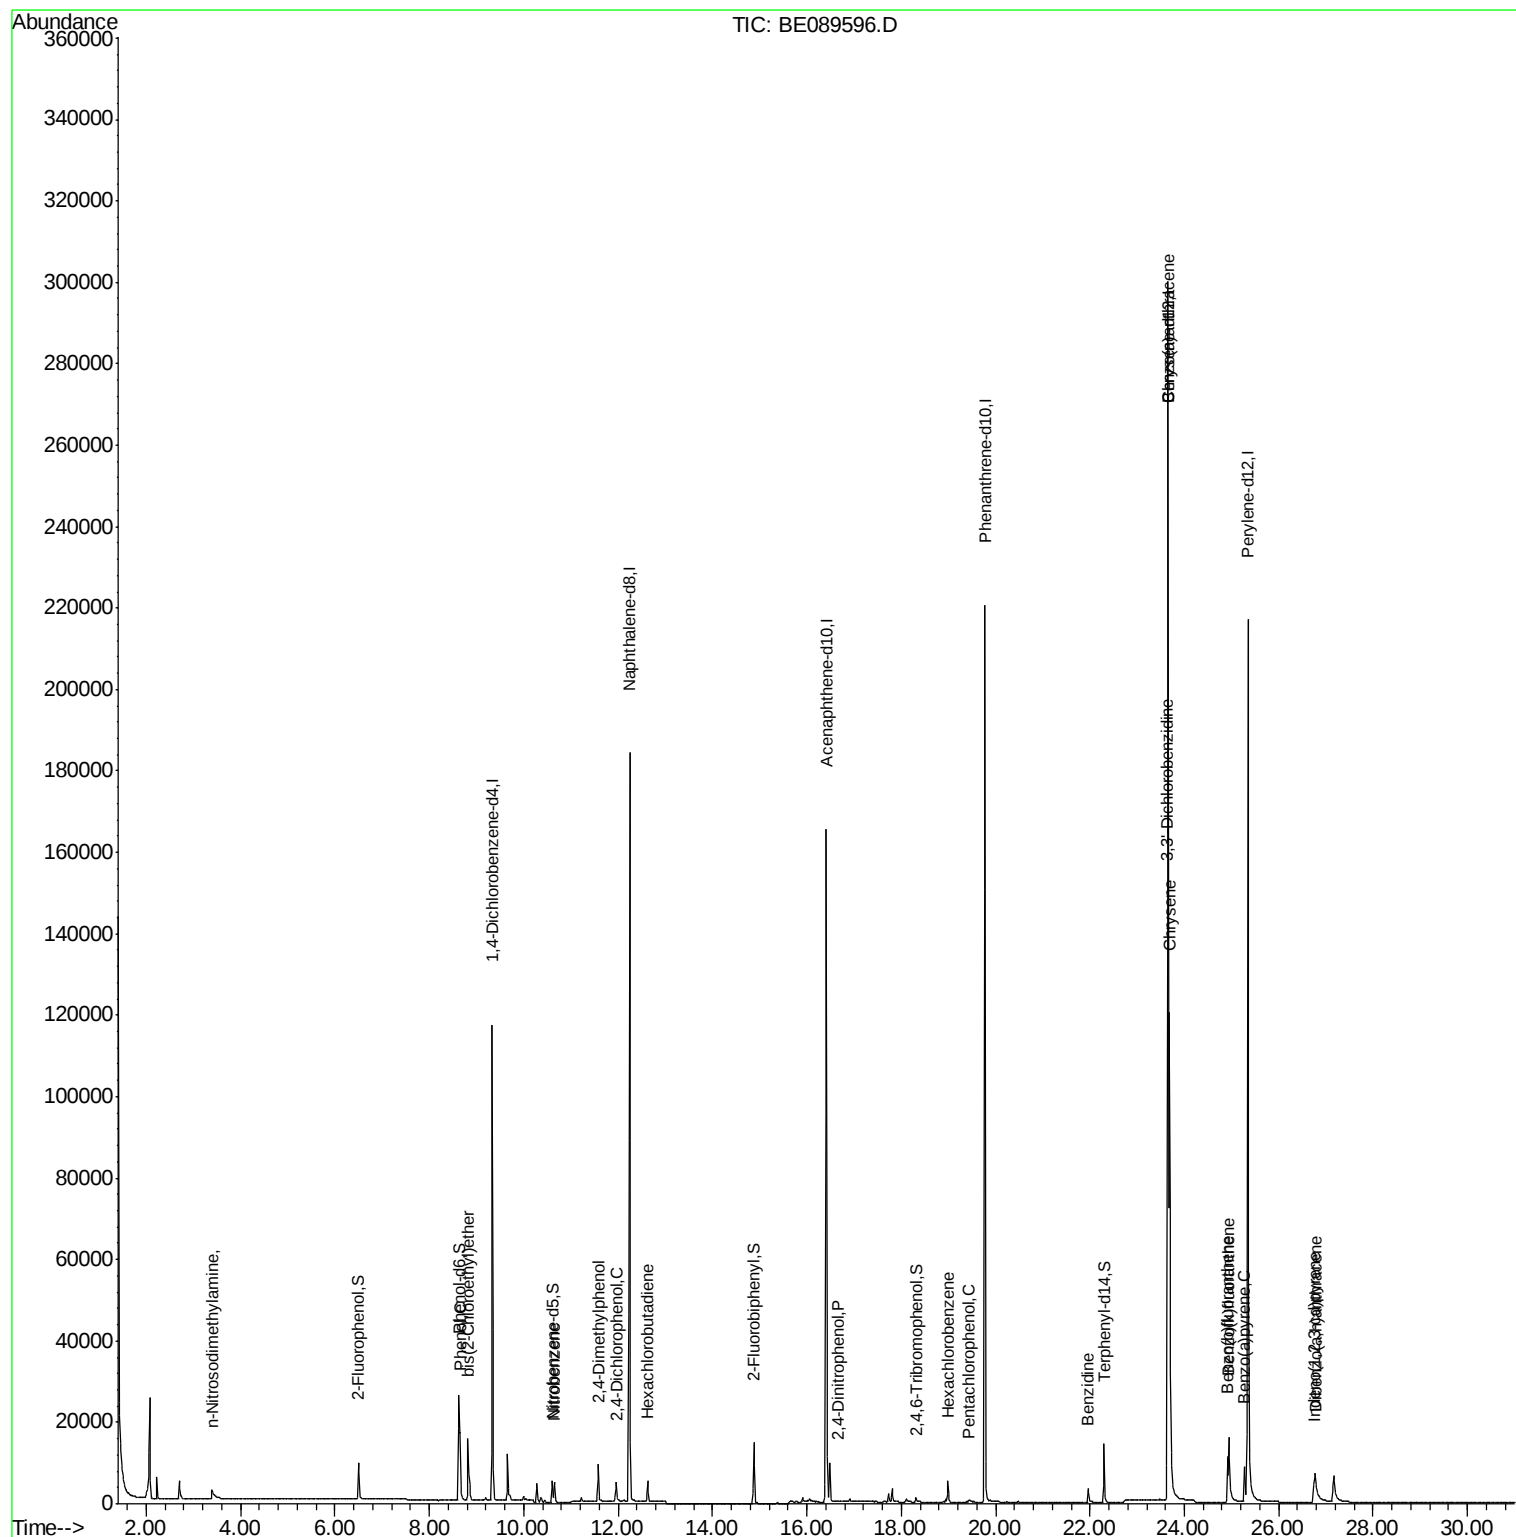



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 9.34 min Scan# 1105

Delta R.T. 0.01 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion: 152 Resp: 56847

Ion Ratio Lower Upper

152 100

150 148.4 130.7 196.1




115 52.8 49.6 74.4

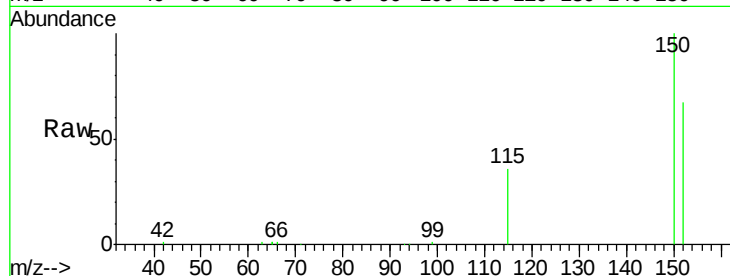

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

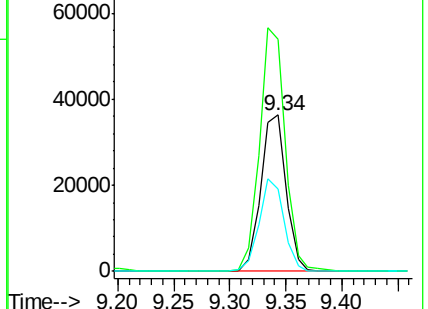

#2

n-Nitrosodimethylamine

Concen: 0.41 ng m

RT: 3.38 min Scan# 293

Delta R.T. 0.03 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion: 42 Resp: 3339

Ion Ratio Lower Upper

42 100

74 112.7 114.6 171.8#



44 77.2 27.5 41.3#




Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

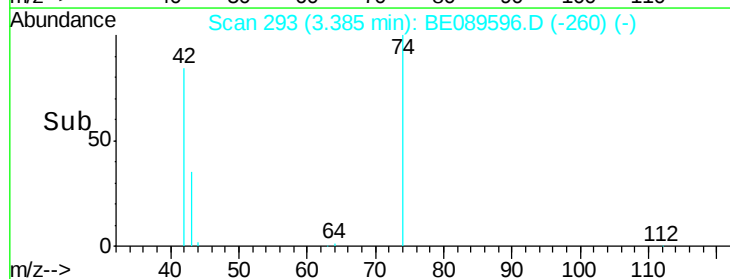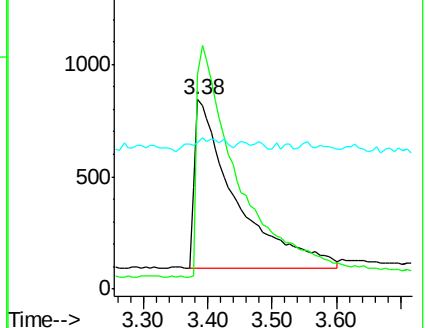



#3

2-Fluorophenol

Concen: 0.45 ng

RT: 6.50 min Scan# 753

Delta R.T. -0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDICC0.5


Tgt Ion: 112 Resp: 7125

Ion Ratio Lower Upper

112 100

64 56.0 41.7 62.5




63 28.6 20.3 30.5

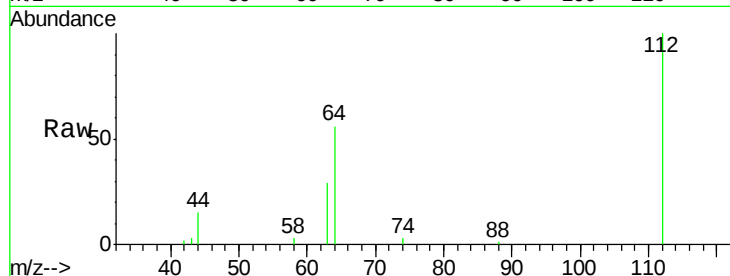

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

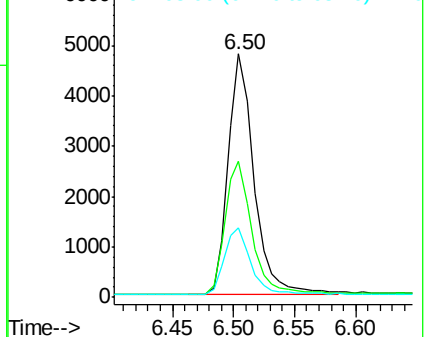

#4

Phenol-d6

Concen: 0.44 ng

RT: 8.62 min Scan# 1024

Delta R.T. -0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion: 99 Resp: 9288

Ion Ratio Lower Upper

99 100

42 15.8 10.8 16.2



71 29.3 21.8 32.6




Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

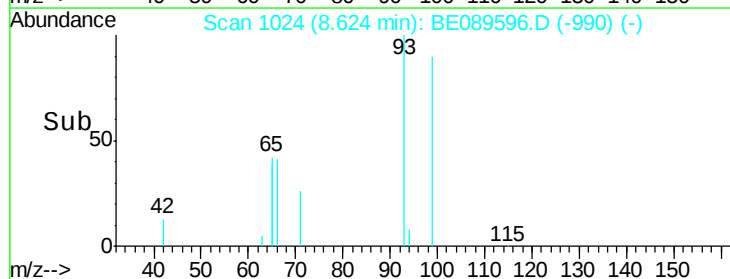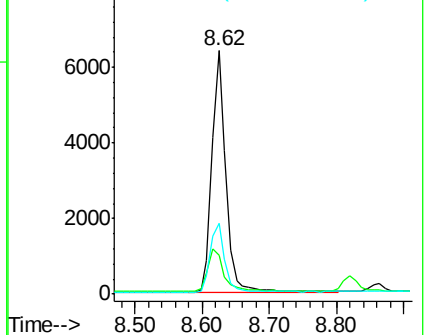



#5

Phenol

Concen: 0.44 ng

RT: 8.65 min Scan# 1027

Delta R.T. -0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDICC0.5





Tgt Ion: 94 Resp: 10122

Ion Ratio Lower Upper

94 100

65 108.0 78.6 118.6

66 36.2 14.0 54.0

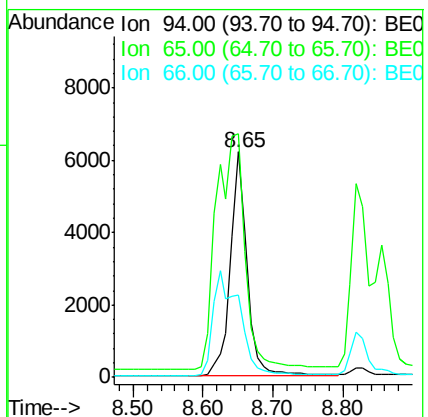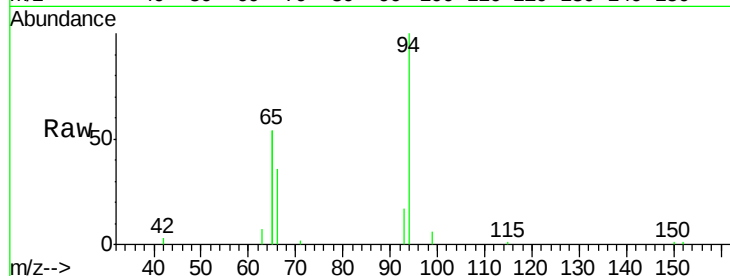

#6

bis(2-Chloroethyl)ether

Concen: 0.47 ng

RT: 8.83 min Scan# 1047

Delta R.T. 0.01 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49




Tgt Ion: 93 Resp: 8159


Ion Ratio Lower Upper

93 100

63 92.4 74.6 112.0

95 0.0 0.0 0.0

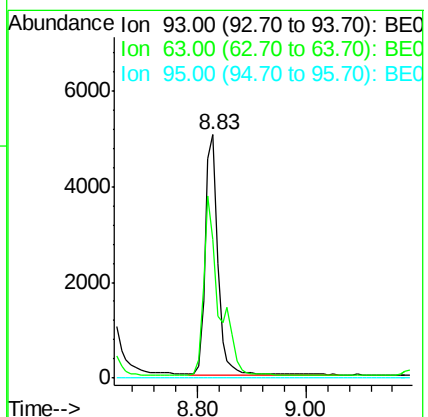



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 12.24 min Scan# 1497

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion: 136 Resp: 223170

Ion Ratio Lower Upper

136 100

137 11.1 8.8 13.2




54 7.0 5.7 8.5

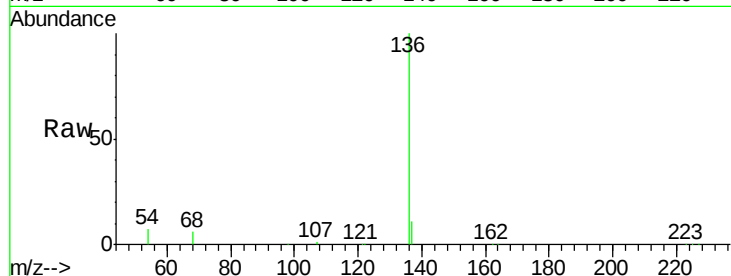

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

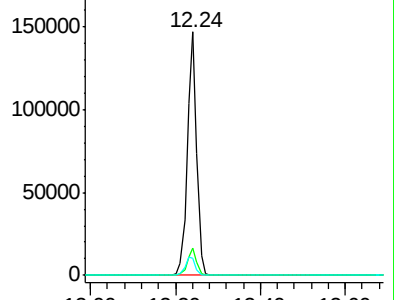

#8

Nitrobenzene-d5

Concen: 0.46 ng

RT: 10.61 min Scan# 1286

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion: 82 Resp: 4206

Ion Ratio Lower Upper

82 100

128 42.3 33.2 49.8



54 47.7 39.6 59.4




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

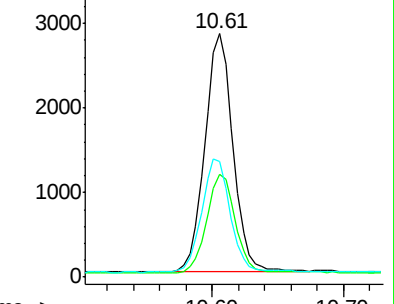



#9

Nitrobenzene

Concen: 0.46 ng

RT: 10.65 min Scan# 1295

Delta R.T. -0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion: 77 Resp: 4986

Ion Ratio Lower Upper




77 100

123 44.3 36.5 54.7

65 13.0 10.2 15.4

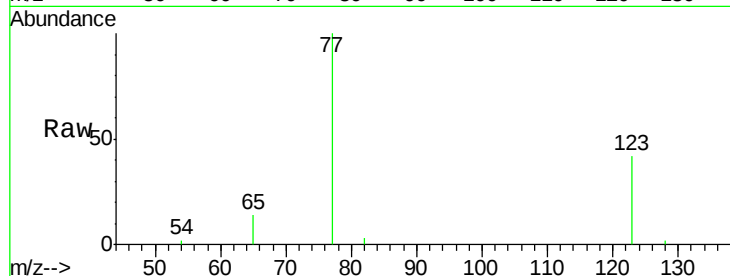

Abundance Ion 77.00 (76.70 to 77.70): BE0
Ion 123.00 (122.70 to 123.70): BE0
Ion 65.00 (64.70 to 65.70): BE0

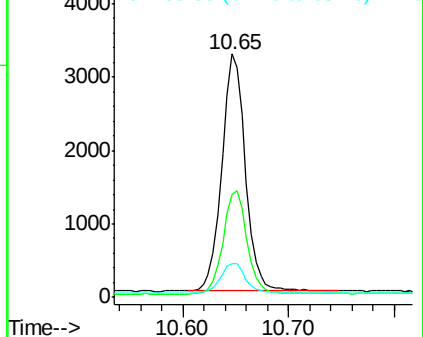

#10

2,4-Dimethylphenol

Concen: 0.41 ng

RT: 11.58 min Scan# 1429

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion: 122 Resp: 5176

Ion Ratio Lower Upper



122 100


107 108.2 83.9 125.9

121 57.1 44.9 67.3



Abundance Ion 122.00 (121.70 to 122.70): E
Ion 107.00 (106.70 to 107.70): E
Ion 121.00 (120.70 to 121.70): E

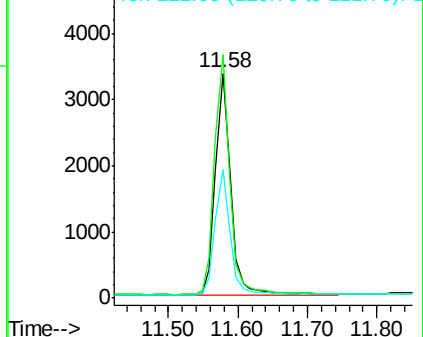







#11
 2,4-Dichlorophenol
 Concen: 0.42 ng
 RT: 11.96 min Scan# 1468
 Delta R.T. 0.00 min
 Lab File: BE089596.D
 Acq: 17 Feb 2015 15:49

Instrument :
 BNA_E
 LabSampleId :
 SSTDICC0.5

Tgt Ion:162 Resp: 4140
 Ion Ratio Lower Upper
 162 100
 164 64.8 44.7 84.7
 98 34.8 10.3 50.3

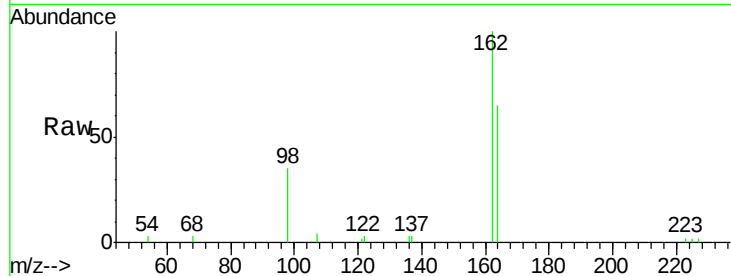


Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): BE0


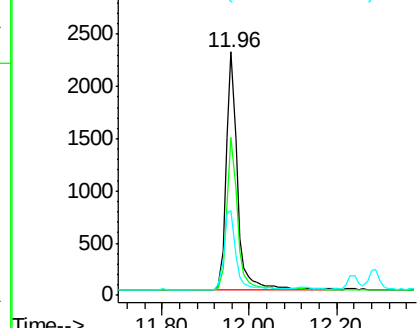



#12
 Hexachlorobutadiene
 Concen: 0.49 ng
 RT: 12.63 min Scan# 1537
 Delta R.T. 0.00 min
 Lab File: BE089596.D
 Acq: 17 Feb 2015 15:49

Tgt Ion:225 Resp: 3350
 Ion Ratio Lower Upper
 225 100
 223 63.0 50.3 75.5
 227 64.2 50.6 75.8



Abundance Ion 225.00 (224.70 to 225.70): E
 Ion 223.00 (222.70 to 223.70): E
 Ion 227.00 (226.70 to 227.70): E




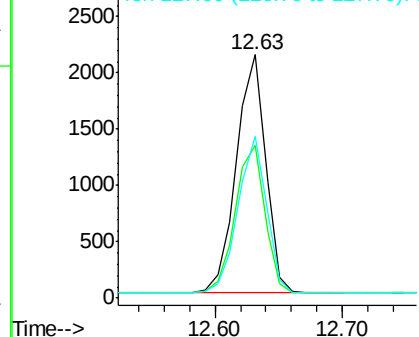




#13
Acenaphthene-d10
Concen: 5.00 ng
RT: 16.42 min Scan# 2804
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49




Instrument :
BNA_E
LabSampleId :
SSTDIC0.5


Tgt Ion:164 Resp: 106357
Ion Ratio Lower Upper
164 100
162 93.8 76.3 114.5
160 42.0 33.9 50.9

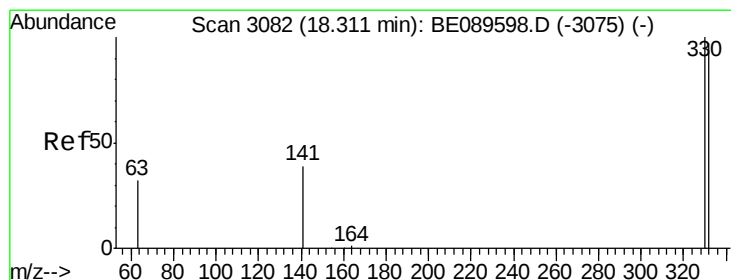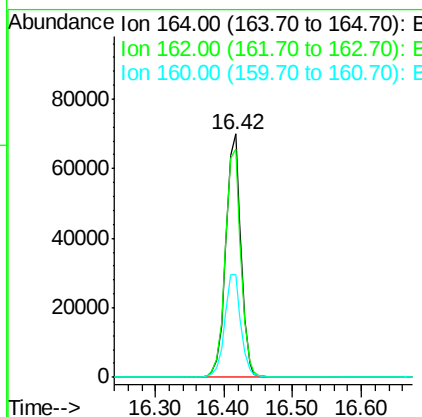

#14
2,4,6-Tribromophenol
Concen: 0.36 ng
RT: 18.31 min Scan# 3083
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49

Tgt Ion:330 Resp: 788
Ion Ratio Lower Upper
330 100
332 96.8 76.7 115.1
141 38.5 30.1 45.1



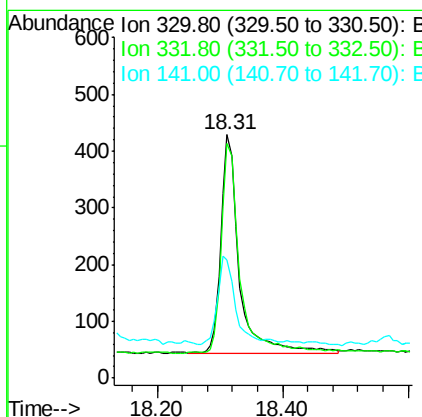
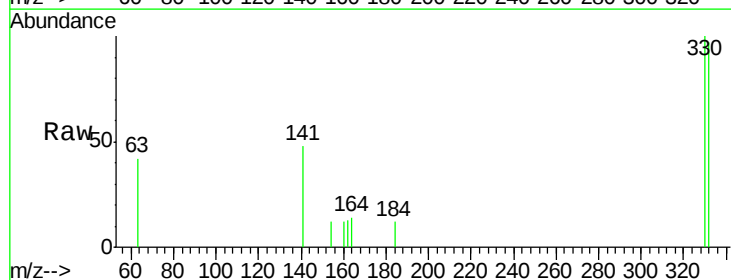




#15
2-Fluorobiphenyl
Concen: 0.49 ng
RT: 14.88 min Scan# 2376
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49




Instrument :
BNA_E
LabSampleId :
SSTDIC0.5


Tgt Ion:172 Resp: 13895
Ion Ratio Lower Upper
172 100
171 33.8 27.4 41.0
170 22.0 17.9 26.9

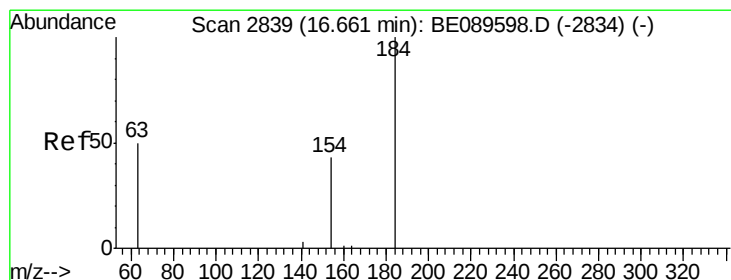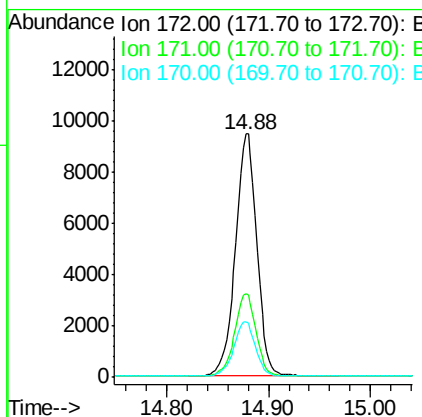

#16
2,4-Dinitrophenol
Concen: 0.34 ng
RT: 16.67 min Scan# 2841
Delta R.T. 0.01 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49

Tgt Ion:184 Resp: 129
Ion Ratio Lower Upper
184 100
63 94.8 61.0 91.4#
154 78.4 53.4 80.0

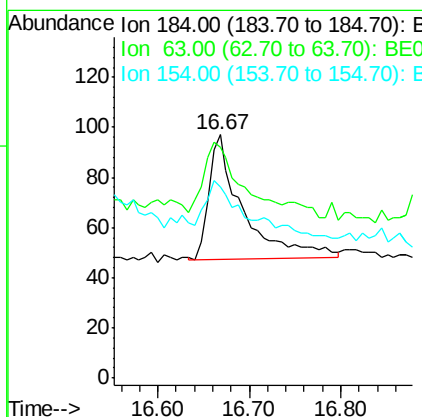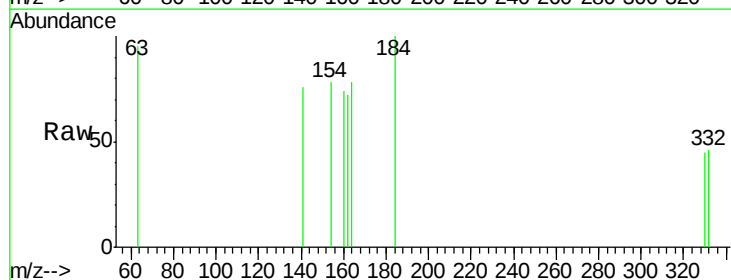







#17
Phenanthrene-d10
Concen: 5.00 ng
RT: 19.77 min Scan# 3295
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49

Instrument :
BNA_E
LabSampleId :
SSTDIC0.5

Tgt Ion:188 Resp: 208337
Ion Ratio Lower Upper
188 100
94 11.5 9.4 14.2
80 11.8 9.8 14.8

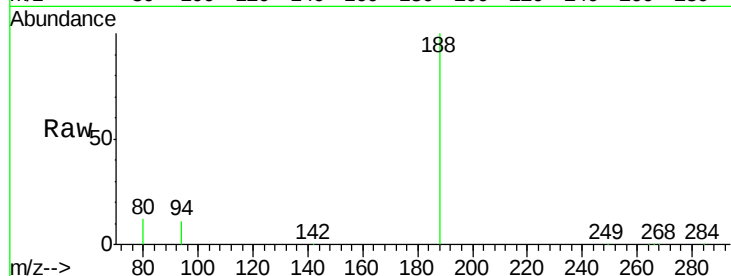


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0


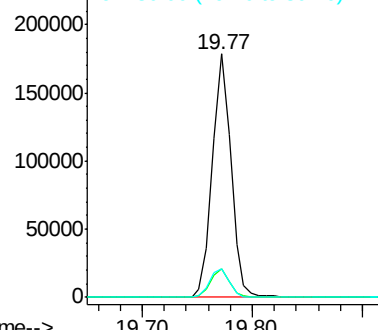



#18
Hexachlorobenzene
Concen: 0.49 ng
RT: 18.99 min Scan# 3180
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49

Tgt Ion:284 Resp: 4350
Ion Ratio Lower Upper
284 100
142 41.0 35.6 53.4
249 29.8 25.2 37.8



Abundance Ion 284.00 (283.70 to 284.70): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

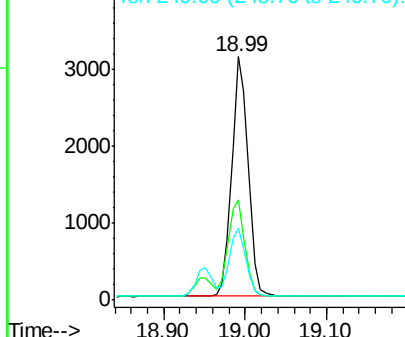







#19
Pentachlorophenol
Concen: 0.36 ng
RT: 19.44 min Scan# 3246
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49

Instrument :
BNA_E
LabSampleId :
SSTDIC0.5

Tgt Ion: 266 Resp: 531
Ion Ratio Lower Upper
266 100
268 70.8 53.0 79.4
264 68.4 51.9 77.9

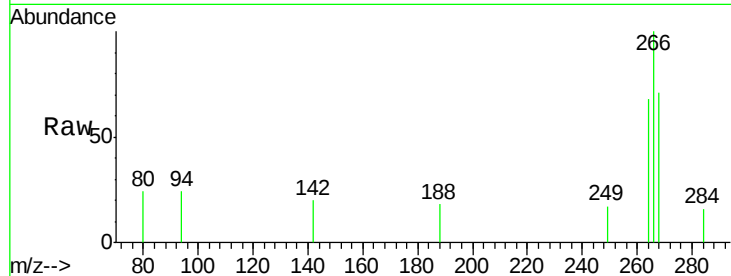


Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E


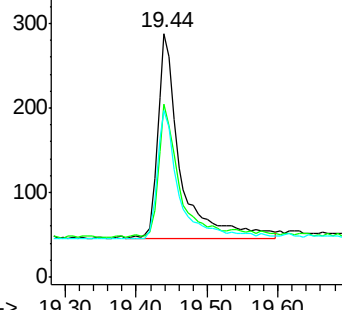



#20
Chrysene-d12
Concen: 5.00 ng
RT: 23.66 min Scan# 3933
Delta R.T. 0.00 min
Lab File: BE089596.D
Acq: 17 Feb 2015 15:49

Tgt Ion: 240 Resp: 226882
Ion Ratio Lower Upper
240 100
120 5.9 5.4 8.0
236 24.2 19.8 29.6



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

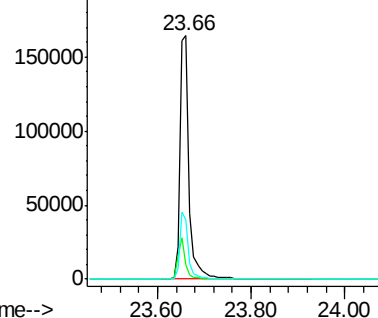

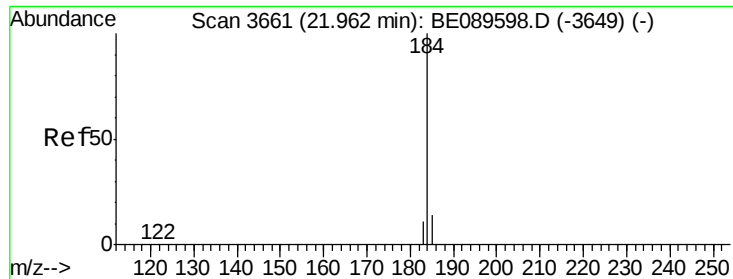

#21

Benzidine

Concen: 0.30 ng

RT: 21.96 min Scan# 3661

Delta R.T. -0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion:184 Resp: 5119

Ion Ratio Lower Upper

184 100

185 14.6 11.8 17.8




183 12.8 9.3 13.9

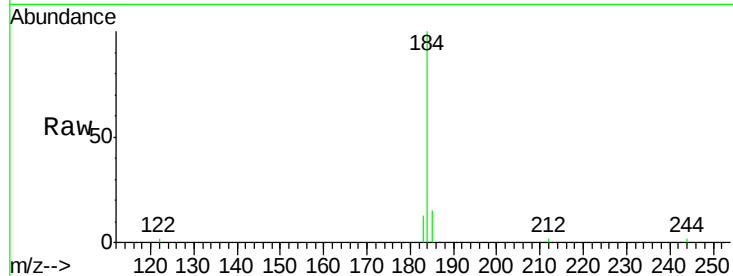

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

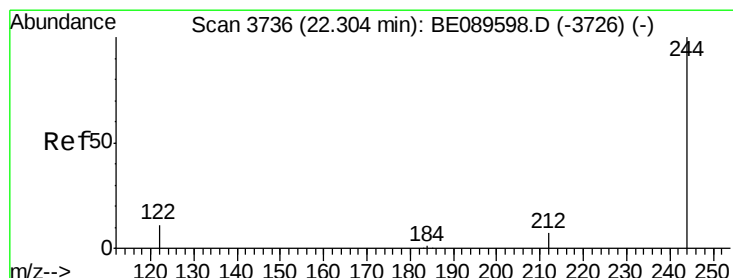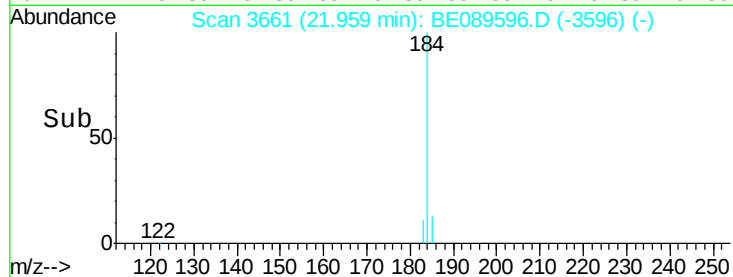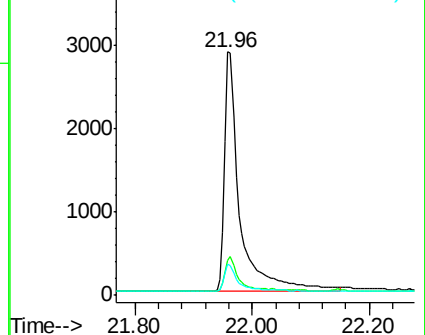

#22

Terphenyl-d14

Concen: 0.45 ng

RT: 22.30 min Scan# 3736

Delta R.T. -0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion:244 Resp: 13922

Ion Ratio Lower Upper

244 100

212 7.6 5.7 8.5



122 14.6 8.6 13.0#

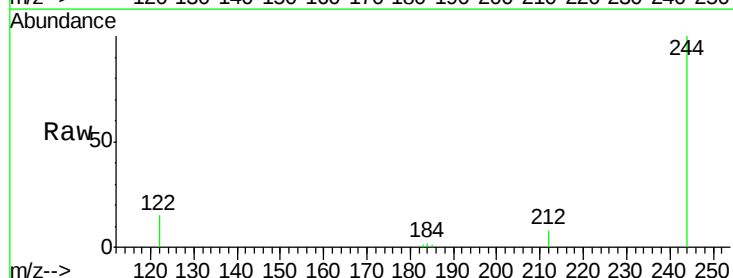


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

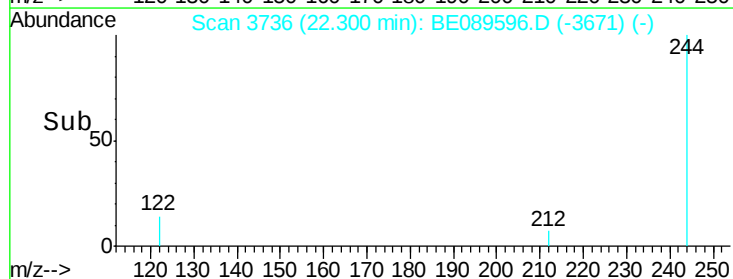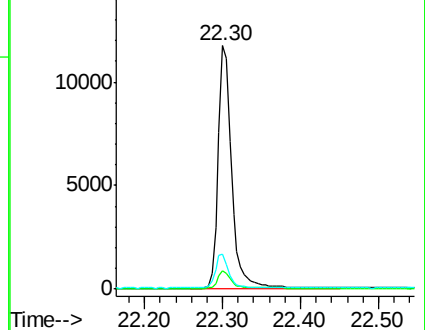

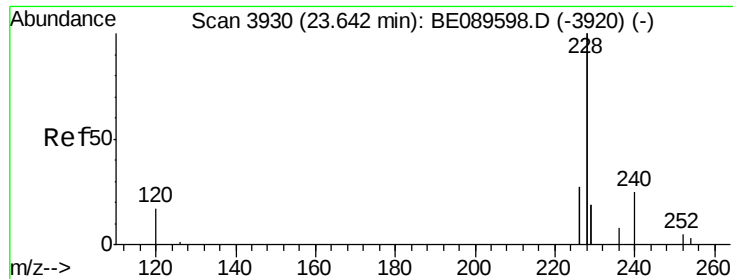

#23

Benzo(a)anthracene

Concen: 0.40 ng

RT: 23.64 min Scan# 3931

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion:228 Resp: 85345

Ion Ratio Lower Upper

228 100

226 27.2 21.5 32.3




229 18.5 15.0 22.6

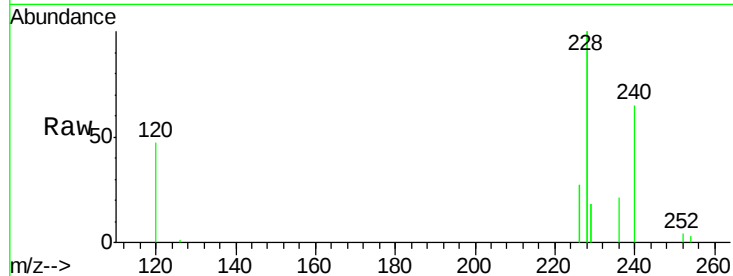

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

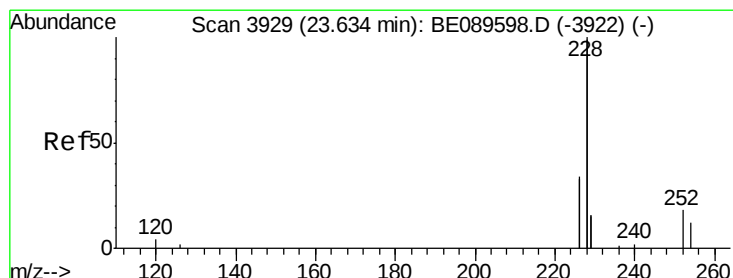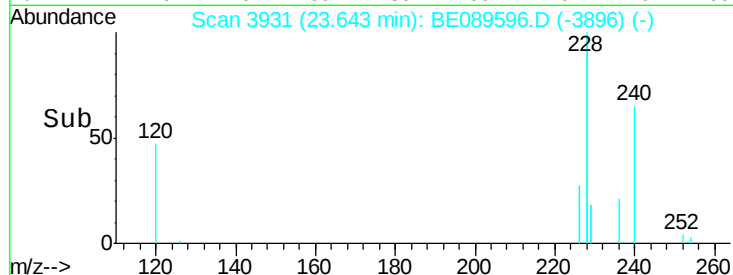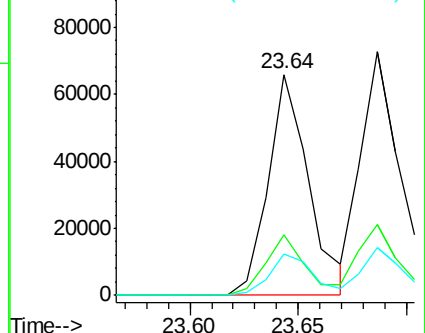

#24

3,3'-Dichlorobenzidine

Concen: 0.25 ng

RT: 23.63 min Scan# 3930

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion:252 Resp: 3485

Ion Ratio Lower Upper

252 100

254 65.8 51.7 77.5



126 12.7 9.9 14.9

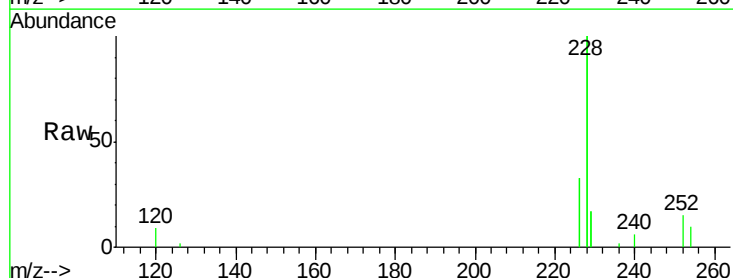


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E

Ion 126.00 (125.70 to 126.70): E

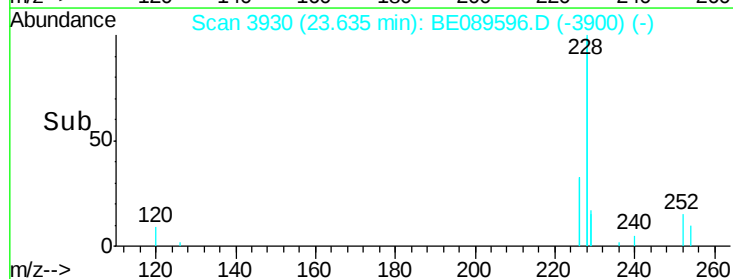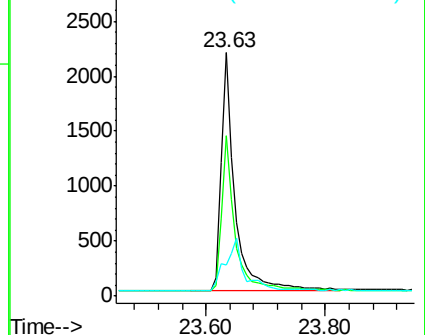

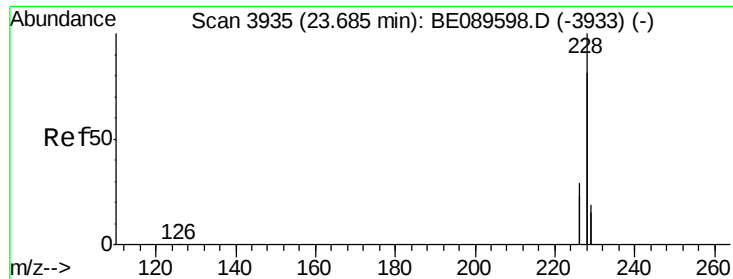

#25

Chrysene

Concen: 0.49 ng

RT: 23.69 min Scan# 3936

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion:228 Resp: 106918

Ion Ratio Lower Upper

228 100

226 28.9 23.4 35.2




229 19.5 15.3 22.9

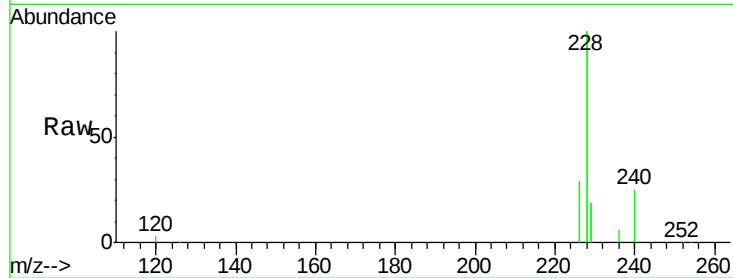

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

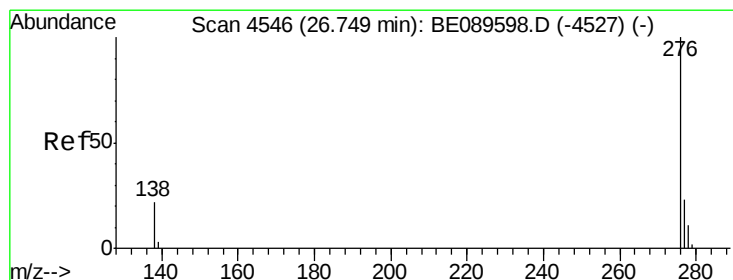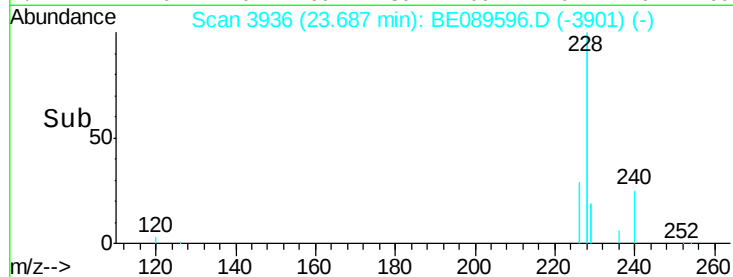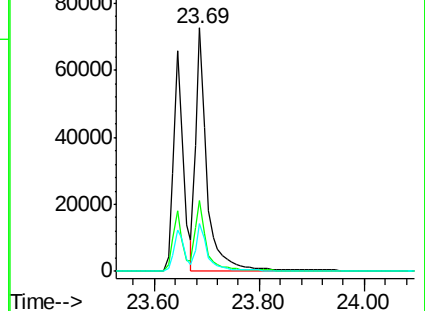

#26

Indeno(1,2,3-cd)pyrene

Concen: 0.31 ng

RT: 26.74 min Scan# 4546

Delta R.T. -0.01 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion:276 Resp: 15082

Ion Ratio Lower Upper

276 100

138 7.6 0.0 0.0#



277 23.6 19.9 29.9

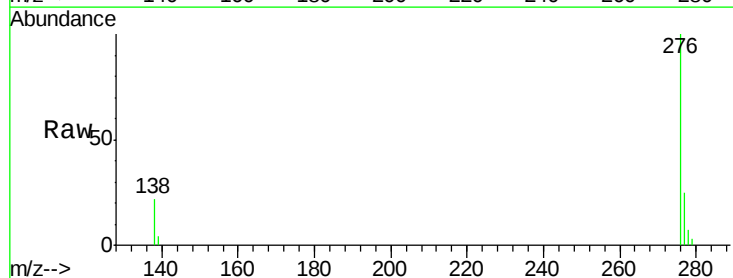


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



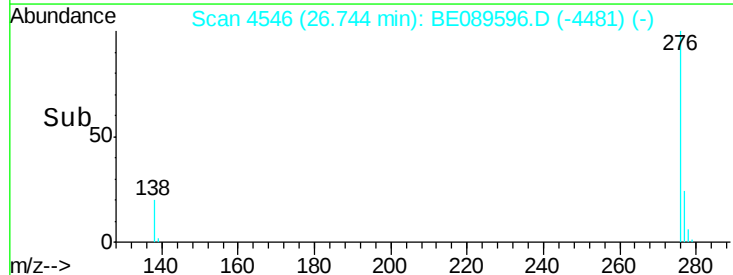
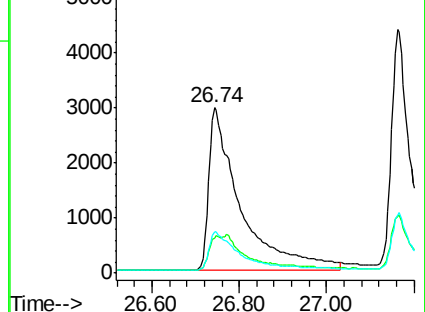


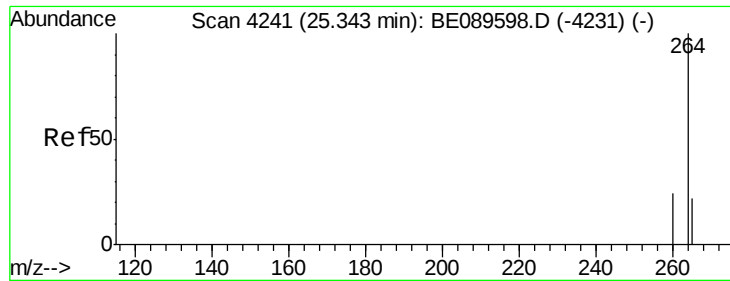

#27
 Perylene-d12
 Concen: 5.00 ng
 RT: 25.34 min Scan# 4242
 Delta R.T. 0.00 min
 Lab File: BE089596.D
 Acq: 17 Feb 2015 15:49




Instrument :
 BNA_E
 LabSampleId :
 SSTDICC0.5


Tgt Ion: 264 Resp: 202710
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.0 28.4
 265 21.9 17.8 26.8

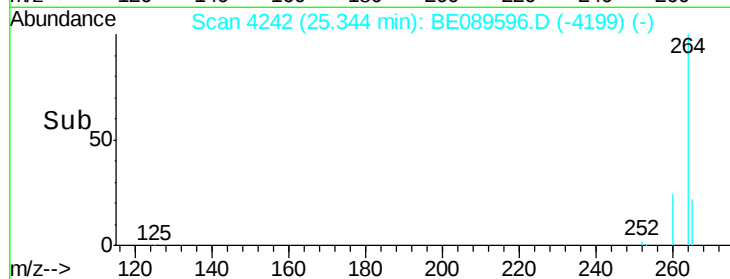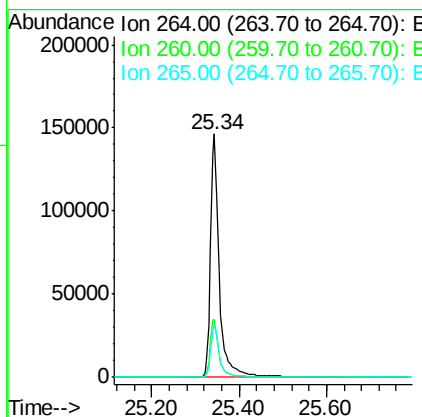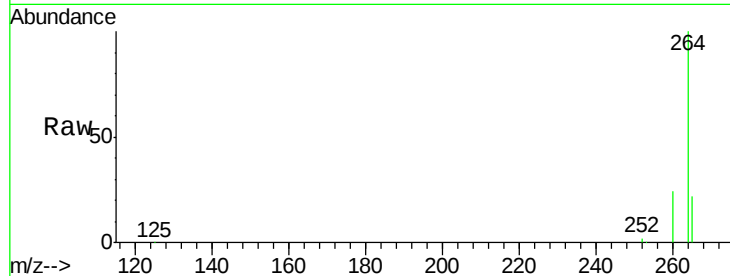

#28
 Benzo(b)fluoranthene
 Concen: 0.31 ng
 RT: 24.92 min Scan# 4148
 Delta R.T. 0.00 min
 Lab File: BE089596.D
 Acq: 17 Feb 2015 15:49

Tgt Ion: 252 Resp: 11658
 Ion Ratio Lower Upper
 252 100
 253 22.1 17.8 26.8
 125 11.4 8.9 13.3

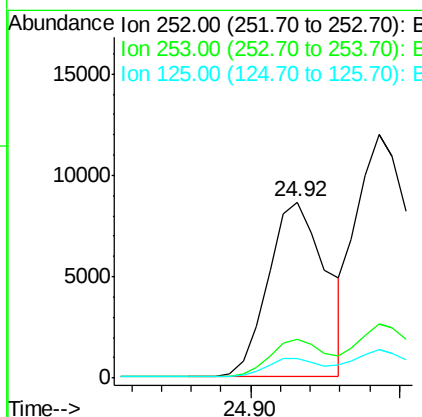



#29

Benzo(k)fluoranthene

Concen: 0.46 ng

RT: 24.94 min Scan# 4154

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5


Tgt Ion:252 Resp: 25186

Ion Ratio Lower Upper




252 100

253 22.3 17.3 25.9

125 11.5 8.9 13.3

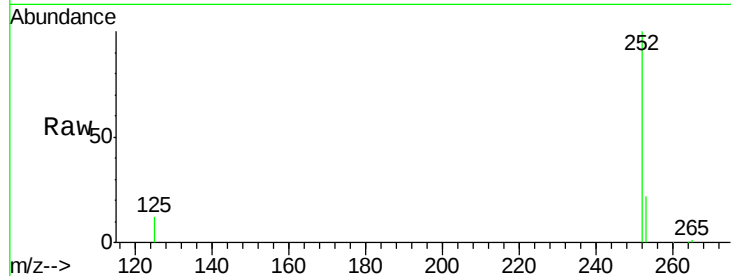

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

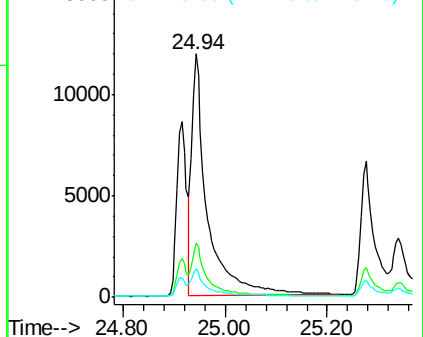

#30

Benzo(a)pyrene

Concen: 0.31 ng

RT: 25.28 min Scan# 4227

Delta R.T. 0.00 min

Lab File: BE089596.D

Acq: 17 Feb 2015 15:49


Tgt Ion:252 Resp: 11220

Ion Ratio Lower Upper



252 100


253 21.9 17.1 25.7

125 12.4 9.8 14.8



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

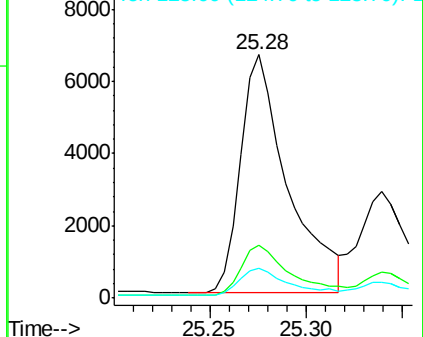



#31

Dibenzo(a,h)anthracene

Concen: 0.32 ng

RT: 26.78 min Scan# 4553

Delta R.T. -0.00 min

Lab File: BE089596.D


Acq: 17 Feb 2015 15:49

Instrument :

BNA_E

LabSampleId :

SSTDIC0.5




Tgt Ion: 278 Resp: 11543

Ion Ratio Lower Upper

278 100

139 17.7 14.6 21.8

279 25.1 19.4 29.0



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

