


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021715\
 Data File : BE089593.D
 Acq On : 17 Feb 2015 13:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE021715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 18 14:11:34 2015

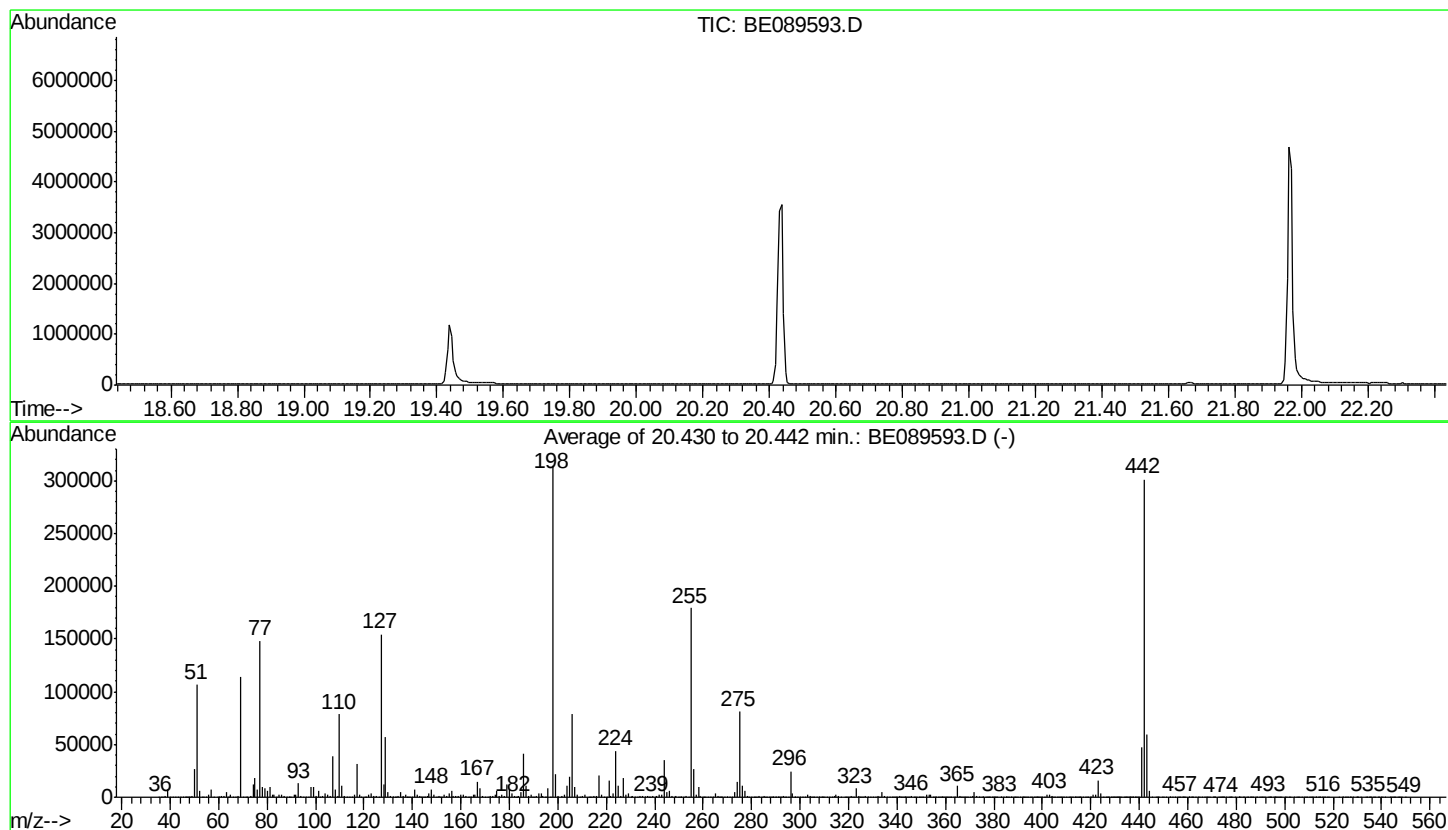

AutoFind: Scans 3241, 3242, 3243; Background Corrected with Scan 3231

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	106299	PASS
68	69	0.00	2	1.4	1589	PASS
69	198	0.00	100	36.4	114423	PASS
70	69	0.00	2	0.5	581	PASS
127	198	10	80	49.1	154397	PASS
197	198	0.00	2	0.1	289	PASS
198	198	100	100	100.0	314388	PASS
199	198	5	9	6.9	21703	PASS
275	198	10	60	25.8	81012	PASS
365	198	1	100	3.5	10886	PASS
441	442	0.01	24	15.6	47080	PASS
442	198	50	100	95.9	301546	PASS
443	442	15	24	19.8	59738	PASS