


Data Path : Z:\HPCHEM1\BNA E\DATA\BE021716\
Data File : BE091403.D
Acq On : 17 Feb 2016 12:26
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 03 00:27:53 2016

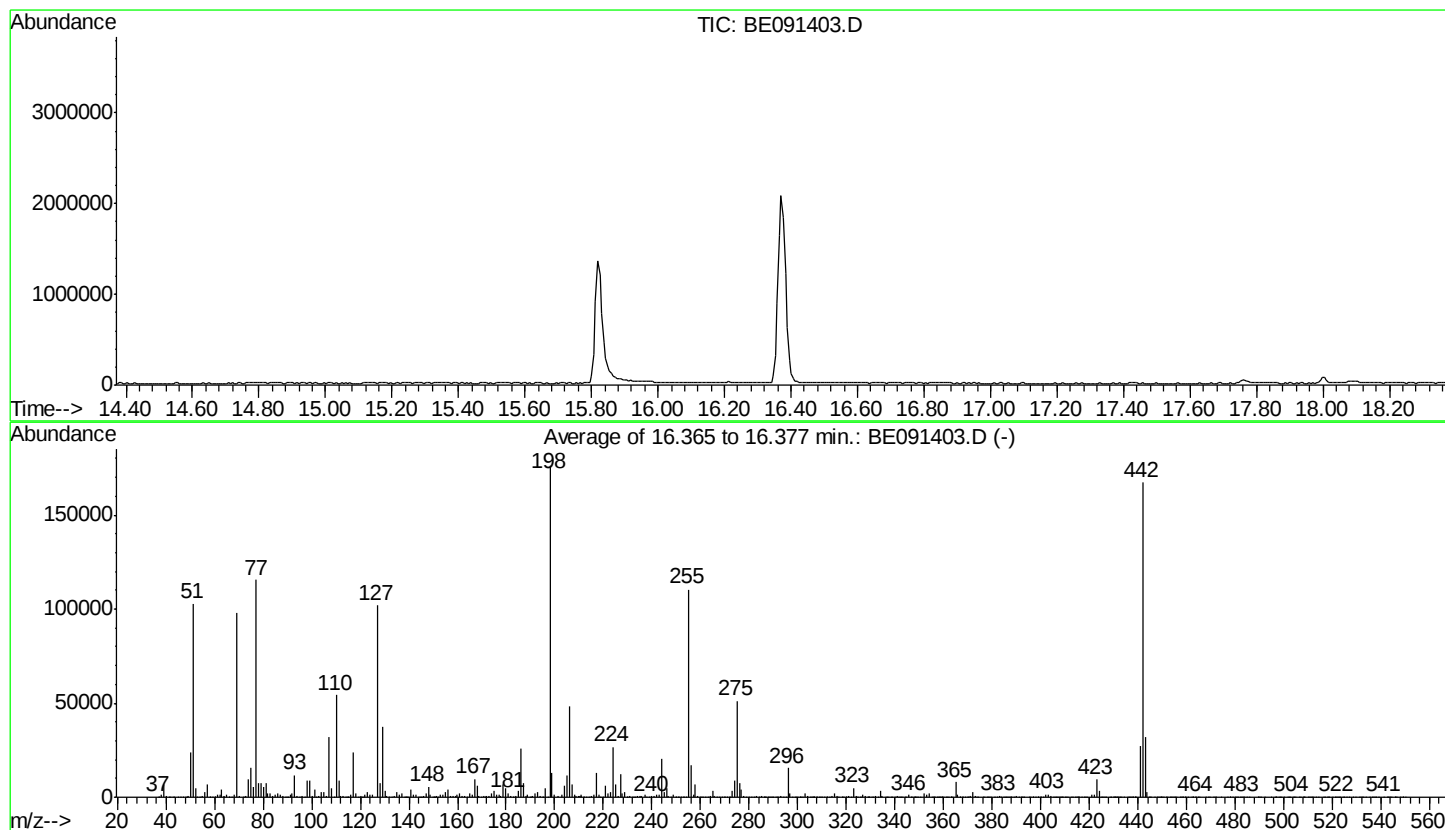

AutoFind: Scans 2345, 2346, 2347; Background Corrected with Scan 2334

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.3	102739	PASS
68	69	0.00	2	1.7	1632	PASS
69	198	0.00	100	55.6	97890	PASS
70	69	0.00	2	0.6	618	PASS
127	198	10	80	57.8	101800	PASS
197	198	0.00	2	0.1	259	PASS
198	198	100	100	100.0	176213	PASS
199	198	5	9	7.2	12737	PASS
275	198	10	60	29.1	51202	PASS
365	198	1	100	4.6	8067	PASS
441	442	0.01	24	16.2	27157	PASS
442	198	50	100	94.9	167262	PASS
443	442	15	24	19.0	31788	PASS