


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021815\
 Data File : BE089633.D
 Acq On : 19 Feb 2015 1:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE021815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 18 13:01:39 2015

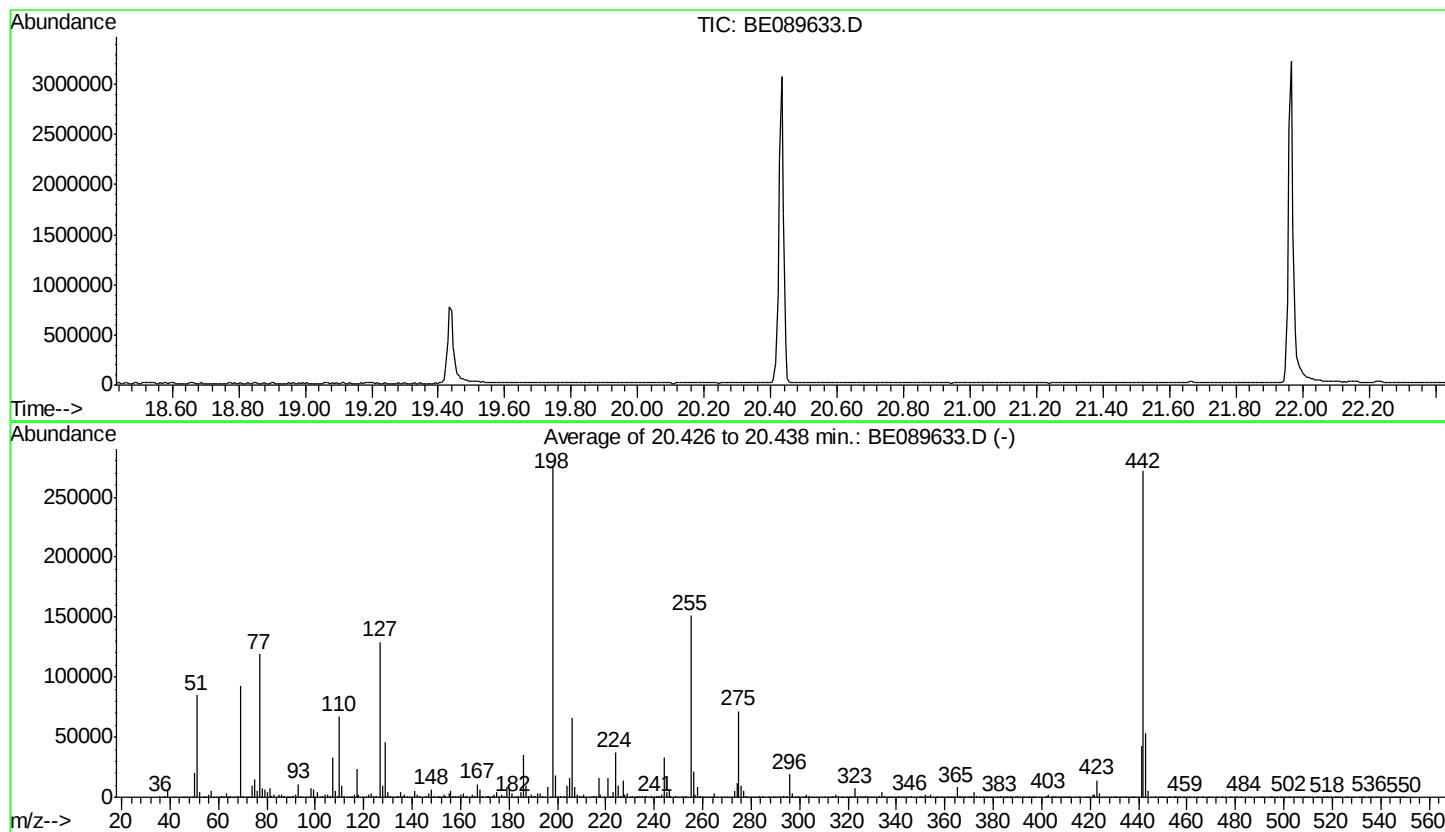

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3232

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	85198	PASS
68	69	0.00	2	1.5	1350	PASS
69	198	0.00	100	33.7	93057	PASS
70	69	0.00	2	0.7	630	PASS
127	198	10	80	46.9	129545	PASS
197	198	0.00	2	0.1	271	PASS
198	198	100	100	100.0	276202	PASS
199	198	5	9	6.6	18117	PASS
275	198	10	60	26.0	71865	PASS
365	198	1	100	3.1	8494	PASS
441	442	0.01	24	15.8	42837	PASS
442	198	50	100	98.3	271420	PASS
443	442	15	24	19.5	52824	PASS