


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE021815\
Data File : BE089647.D
Acq On : 20 Feb 2015 6:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE021815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 18 13:01:39 2015

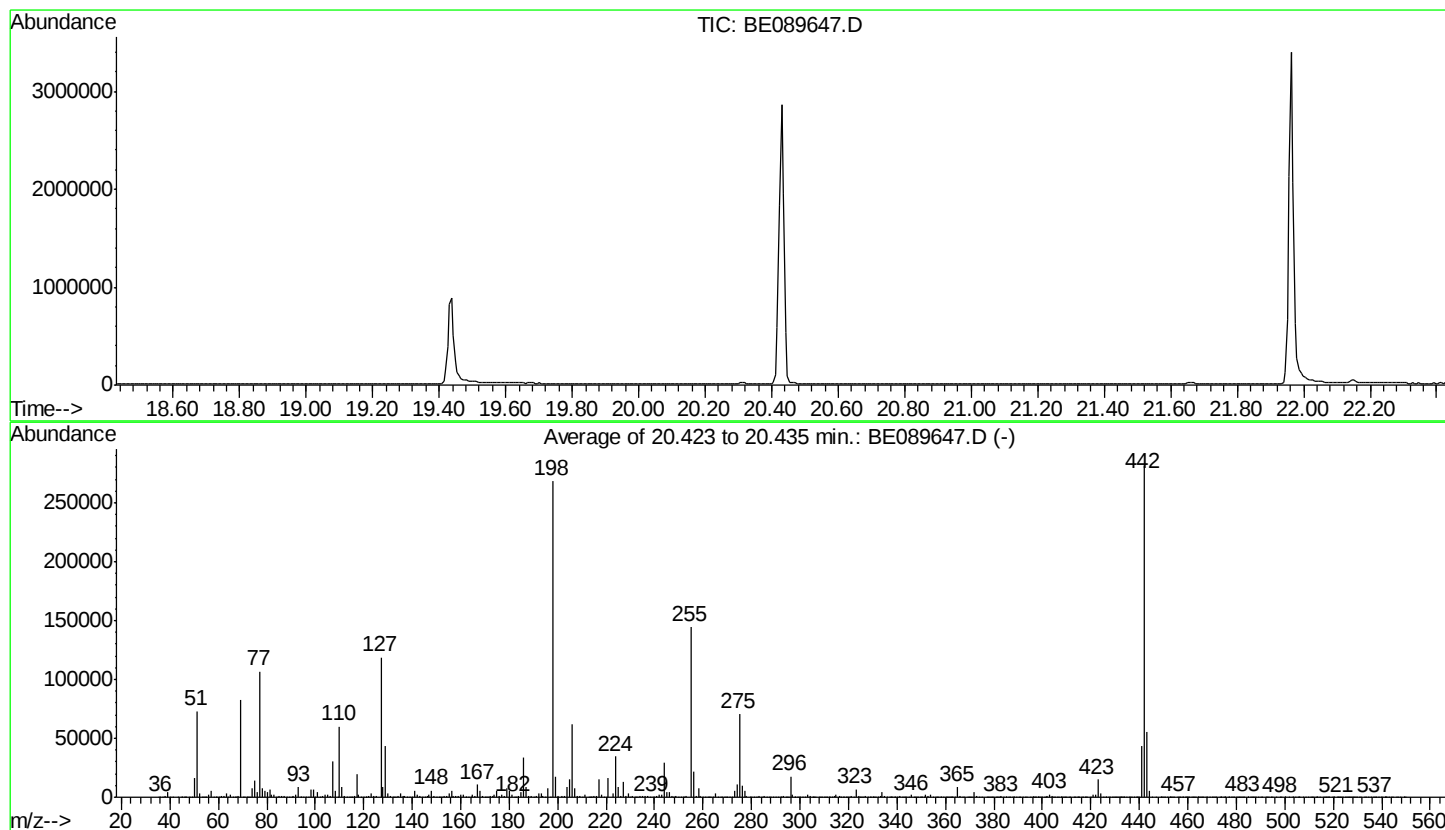

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3232

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	72980	PASS
68	69	0.00	2	1.5	1272	PASS
69	198	0.00	100	30.7	82365	PASS
70	69	0.00	2	0.4	294	PASS
127	198	10	80	44.1	118485	PASS
197	198	0.00	2	0.2	492	PASS
198	198	100	100	100.0	268524	PASS
199	198	5	9	6.6	17757	PASS
275	198	10	60	26.4	70898	PASS
365	198	1	100	3.3	8775	PASS
441	442	0.01	24	15.3	42997	PASS
442	198	50	100	104.8	281514	FAIL*
443	442	15	24	19.8	55842	PASS