

Data Path : Z:\HPCHEM1\BNA E\DATA\BE021815\
 Data File : BE089642.D
 Acq On : 20 Feb 2015 1:09
 Operator : TP/IZ
 Sample : MDL-04-W
 Misc : MDL-WATER-0.2/0.4
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 MDL-04-W

Quant Time: Feb 20 02:32:37 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SIMPAH-BE021815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 18 13:01:39 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.34	152	36160	5.00	ng	0.00
4) Naphthalene-d8	12.24	136	143455	5.00	ng	0.00
8) Acenaphthene-d10	16.42	164	72522	5.00	ng	0.00
13) Phenanthrene-d10	19.77	188	143322	5.00	ng	0.00
19) Chrysene-d12	23.66	240	135795	5.00	ng	0.00
25) Perylene-d12	25.34	264	110972	5.00	ng	0.00
System Monitoring Compounds						
5) Nitrobenzene-d5	10.61	82	67693	10.86	ng	0.00
9) 2-Fluorobiphenyl	14.88	172	188481	9.70	ng	0.00
21) Terphenyl-d14	22.30	244	246700	12.63	ng	0.00
Target Compounds						Ovalue
2) 1,4-Dioxane	2.72	88	614	0.14	ng	# 83
3) n-Nitrosodimethylamine	3.48	42	348	0.08	ng	# 42
6) Naphthalene	12.29	128	5129	0.16	ng	97
7) 2-Methylnaphthalene	13.95	142	2878	0.15	ng	99
10) Acenaphthylene	16.07	152	16233	0.14	ng	100
11) Acenaphthene	16.49	154	2919	0.15	ng	95
12) Fluorene	17.74	166	3368	0.15	ng	99
14) Hexachlorobenzene	19.00	284	1029	0.17	ng	94
15) Pentachlorophenol	19.45	266	70	0.05	ng	# 79
16) Phenanthrene	19.81	178	5754	0.16	ng	98
17) Anthracene	19.91	178	4240	0.14	ng	100
18) Fluoranthene	21.72	202	4662	0.14	ng	99
20) Pyrene	22.04	202	5049	0.15	ng	99
22) Benzo(a)anthracene	23.65	228	15471	0.13	ng	95
23) Chrysene	23.69	228	25354	0.19	ng	98
24) Indeno(1,2,3-cd)pyrene	26.74	276	5854	0.22	ng	91
26) Benzo(b)fluoranthene	24.91	252	1073	0.31	ng	# 90
27) Benzo(k)fluoranthene	24.94	252	3761m	0.12	ng	
28) Benzo(a)pyrene	25.27	252	1280	0.29	ng	# 88
29) Dibenzo(a,h)anthracene	26.77	278	890	0.27	ng	# 77
30) Benzo(g,h,i)perylene	27.16	276	7515	0.21	ng	# 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE021815\
Data File : BE089642.D
Acq On : 20 Feb 2015 1:09
Operator : TP/IZ
Sample : MDL-04-W
Misc : MDL-WATER-0.2/0.4
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
MDL-04-W

Quant Time: Feb 20 02:32:37 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SIMPAH-BE021815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 13:01:39 2015
Response via : Initial Calibration

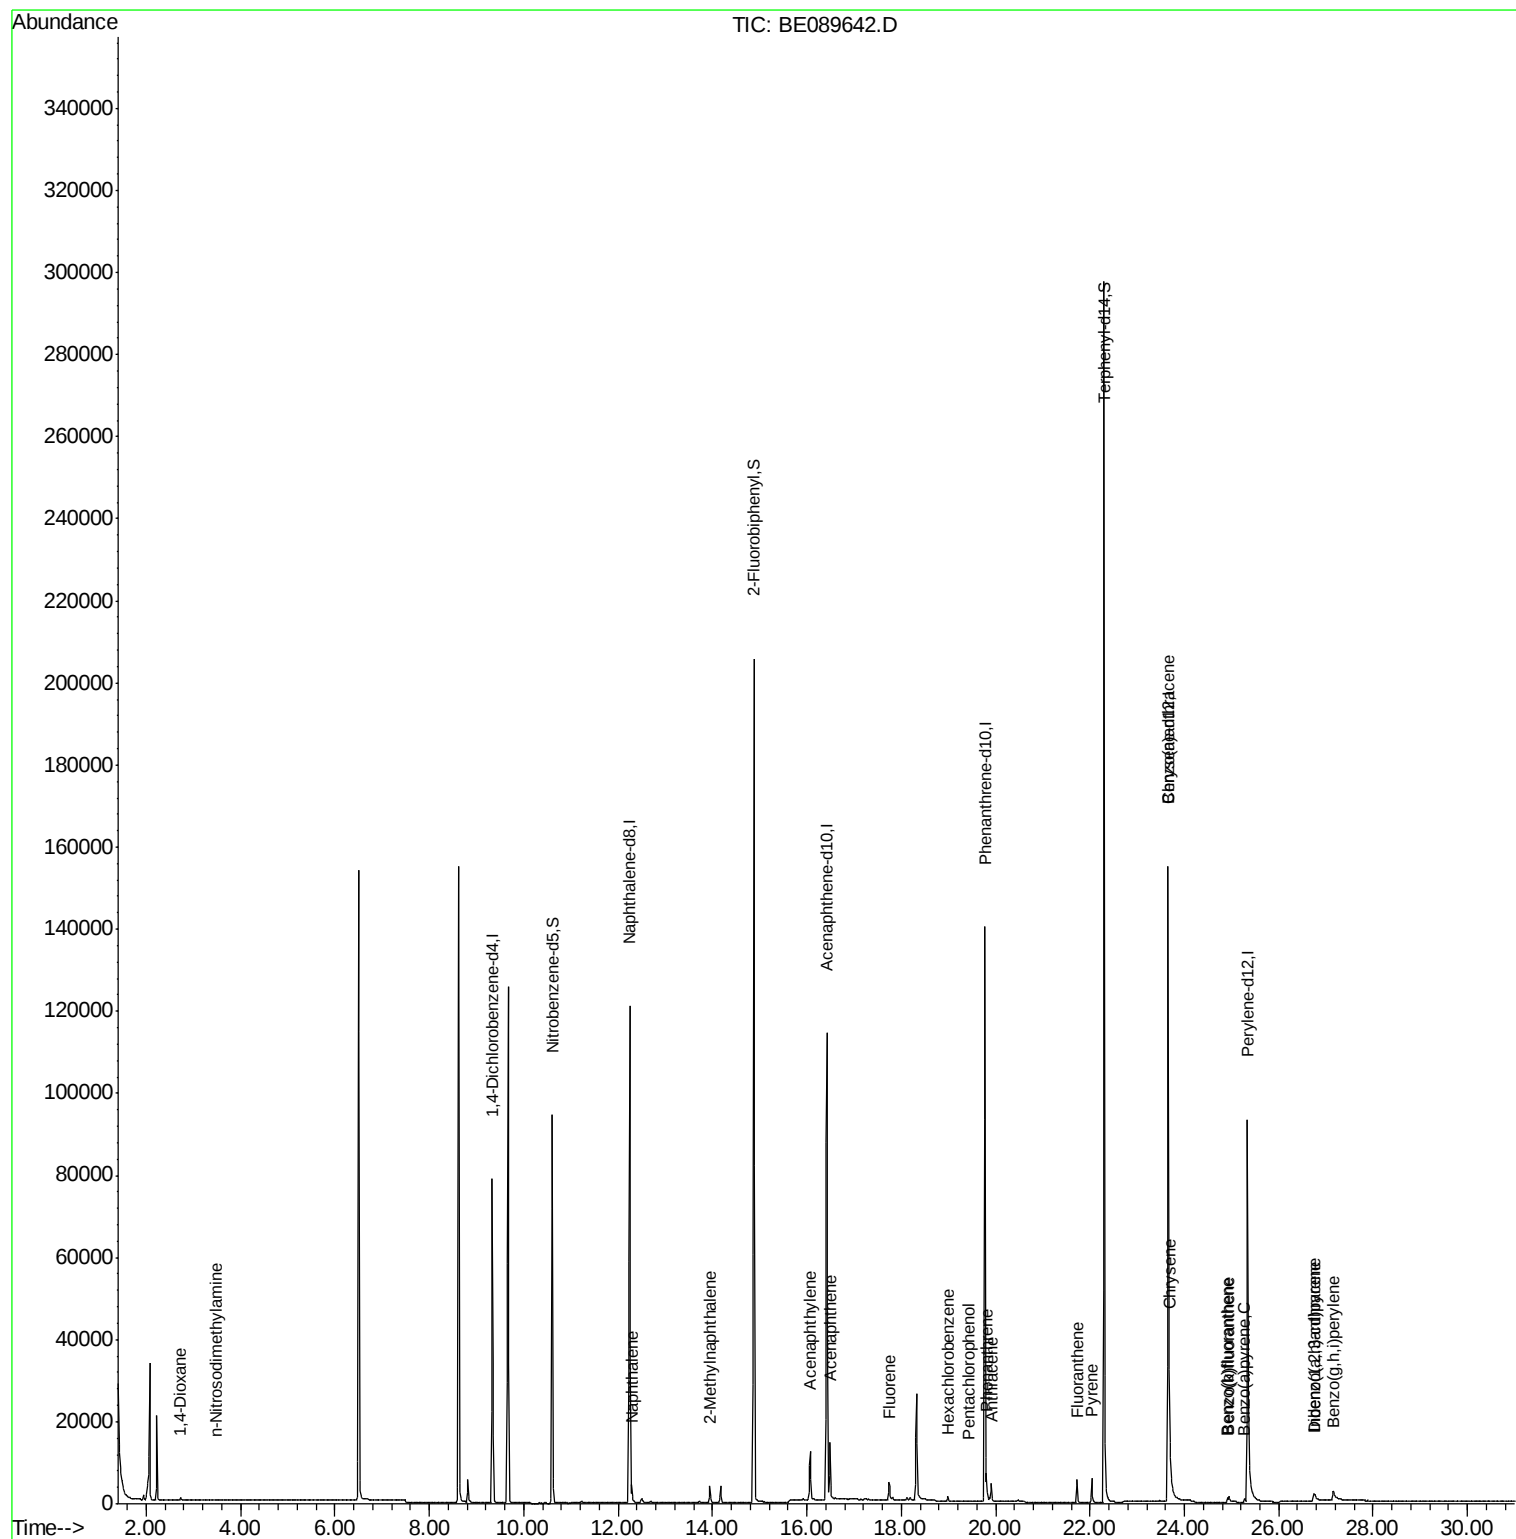



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 9.34 min Scan# 1299

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:152 Resp: 36160

Ion Ratio Lower Upper

152 100

150 158.1 122.4 183.6




115 57.1 44.2 66.2

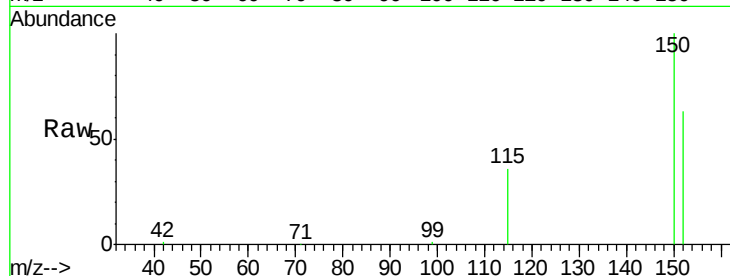

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

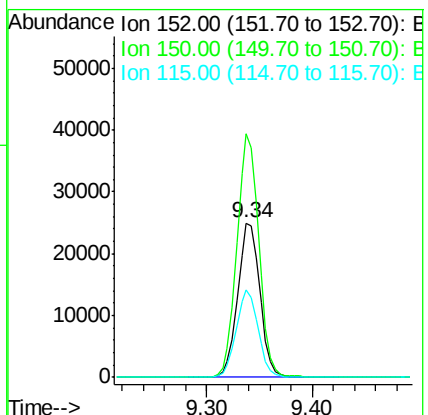

#2

1,4-Dioxane

Concen: 0.14 ng

RT: 2.72 min Scan# 195

Delta R.T. 0.03 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion: 88 Resp: 614

Ion Ratio Lower Upper

88 100

58 71.7 54.6 81.8



43 0.0 20.6 30.8#




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

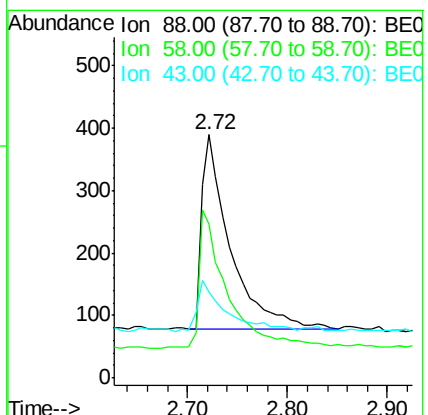

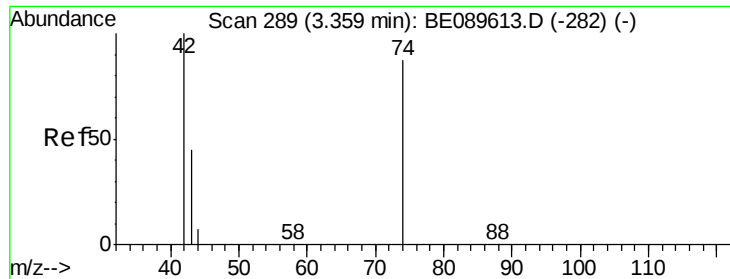


#3




n-Nitrosodimethylamine
 Concen: 0.08 ng
 RT: 3.48 min Scan# 307
 Delta R.T. 0.12 min
 Lab File: BE089642.D
 Acq: 20 Feb 2015 1:09

Instrument :
 BNA_E
 ClientSampleId :
 MDL-04-W

Tot Ion: 42 Resp: 348
 Ion Ratio Lower Upper
 42 100
 74 227.9 121.4 182.0#
 44 7.2 4.5 6.7#

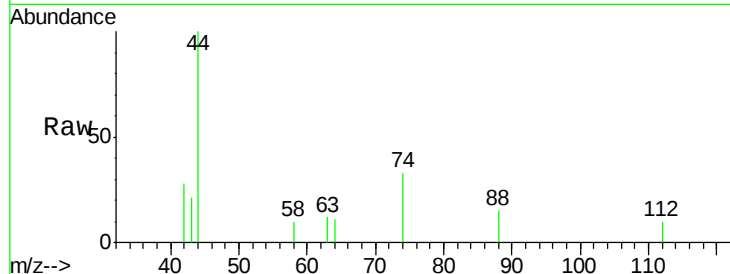


Abundance Ion 42.00 (41.70 to 42.70): BE0
 Ion 74.00 (73.70 to 74.70): BE0
 Ion 44.00 (43.70 to 44.70): BE0

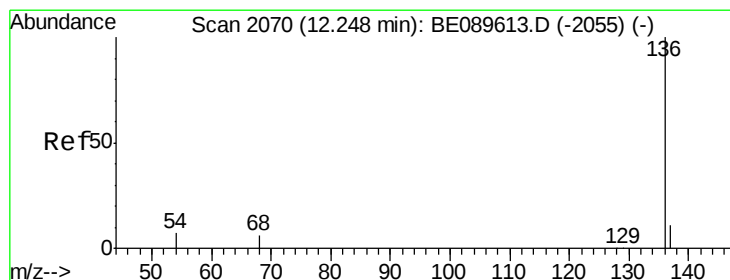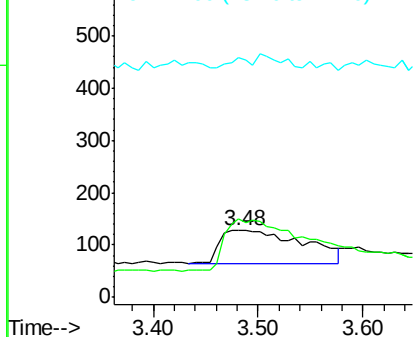



#4


Naphthalene-d8
 Concen: 5.00 ng
 RT: 12.24 min Scan# 2069
 Delta R.T. -0.01 min
 Lab File: BE089642.D
 Acq: 20 Feb 2015 1:09

Tgt Ion: 136 Resp: 143455
 Ion Ratio Lower Upper
 136 100
 137 11.0 8.9 13.3
 54 7.4 5.3 7.9



Abundance Ion 136.00 (135.70 to 136.70): E
 Ion 137.00 (136.70 to 137.70): E
 Ion 54.00 (53.70 to 54.70): BE0

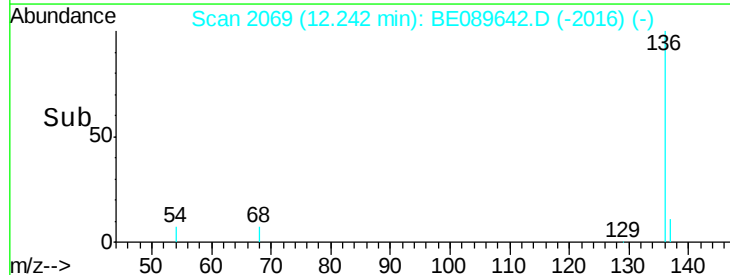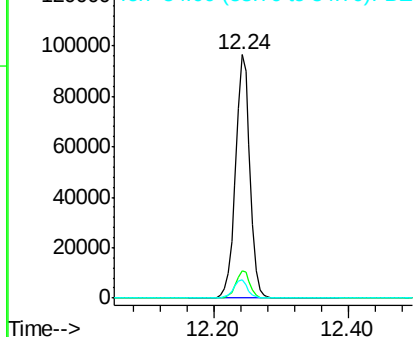

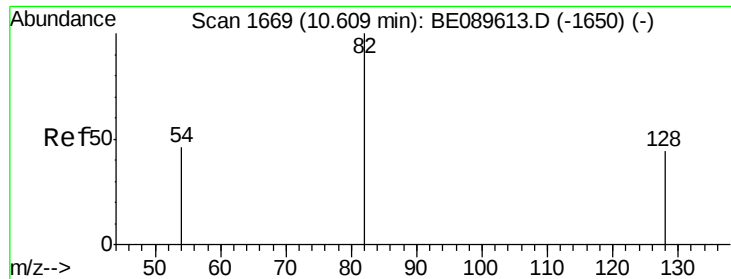

#5

Nitrobenzene-d5

Concen: 10.86 ng

RT: 10.61 min Scan# 1668

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion: 82 Resp: 67693

Ion Ratio Lower Upper

82 100

128 48.6 35.5 53.3




54 44.3 37.5 56.3

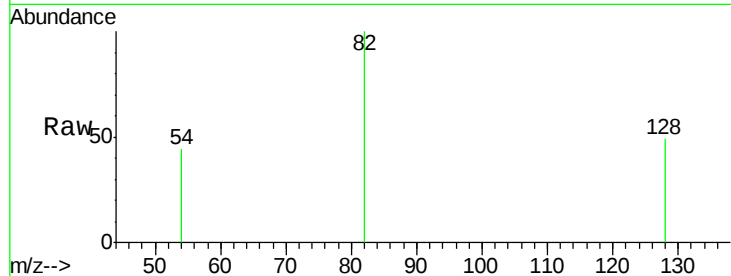

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

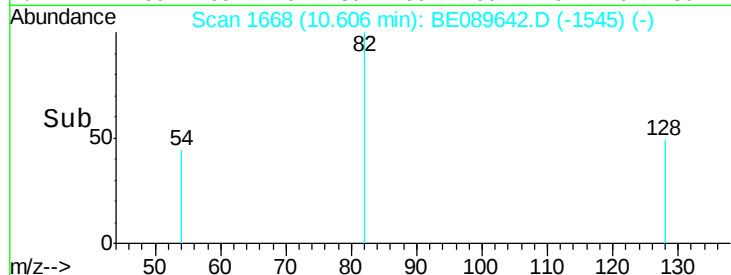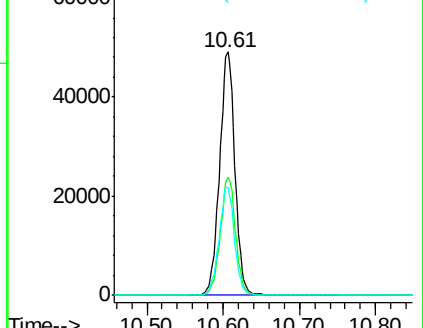

#6

Naphthalene

Concen: 0.16 ng

RT: 12.29 min Scan# 2078

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion: 128 Resp: 5129

Ion Ratio Lower Upper

128 100

129 11.9 8.9 13.3



127 13.9 9.8 14.8



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

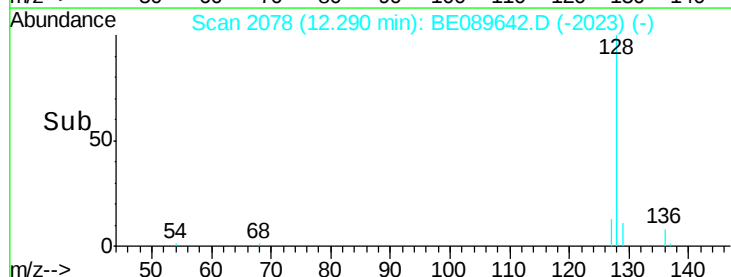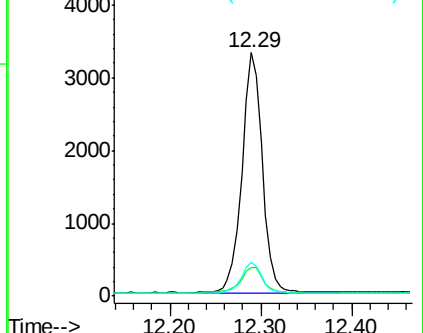



#7

2-Methylnaphthalene

Concen: 0.15 ng

RT: 13.95 min Scan# 2417

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:142 Resp: 2878

Ion Ratio Lower Upper

142 100

141 85.6 68.3 102.5




115 32.2 25.1 37.7

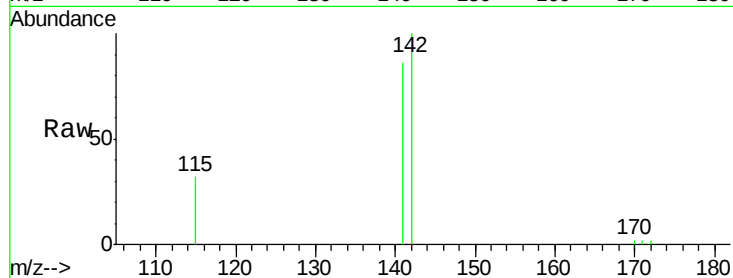

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

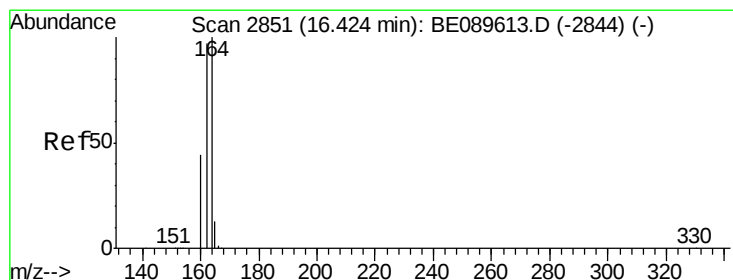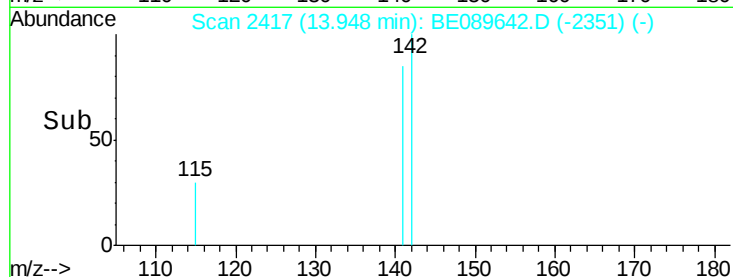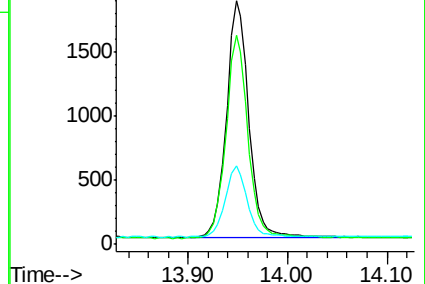

#8

Acenaphthene-d10

Concen: 5.00 ng

RT: 16.42 min Scan# 2852

Delta R.T. 0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:164 Resp: 72522

Ion Ratio Lower Upper

164 100

162 92.8 77.5 116.3



160 41.4 35.5 53.3

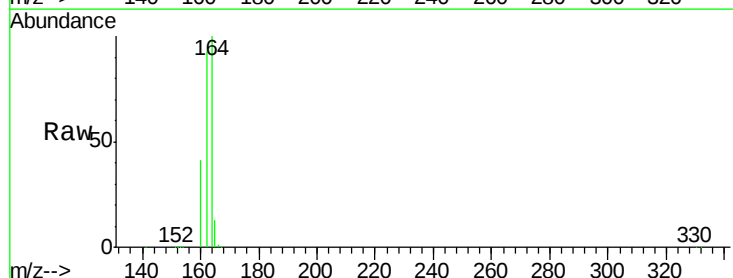

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

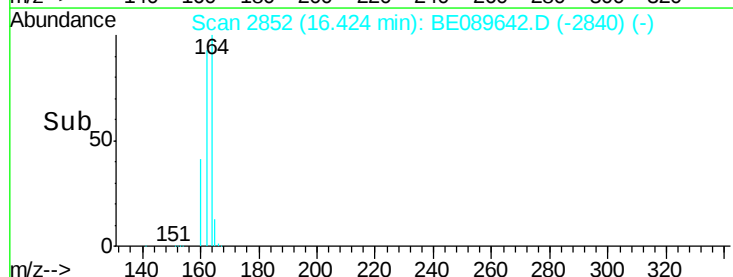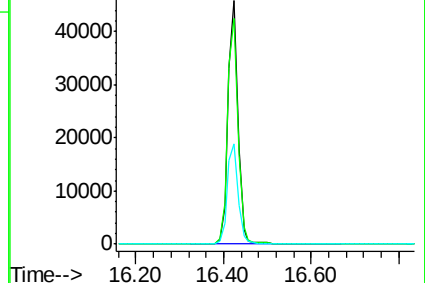



#9

2-Fluorobiphenyl

Concen: 9.70 ng

RT: 14.88 min Scan# 2621

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:172 Resp: 188481

Ion Ratio Lower Upper

172 100

171 34.8 26.9 40.3




170 23.5 17.4 26.0

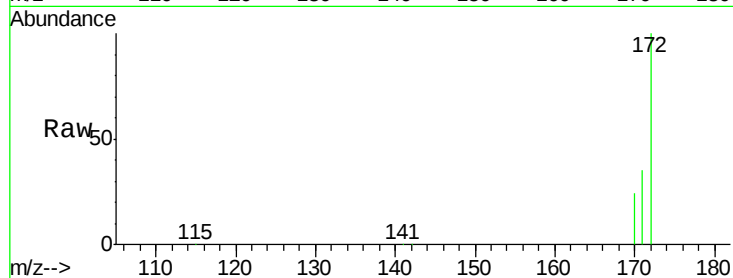

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

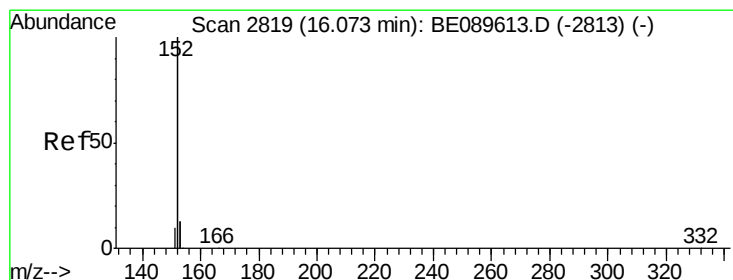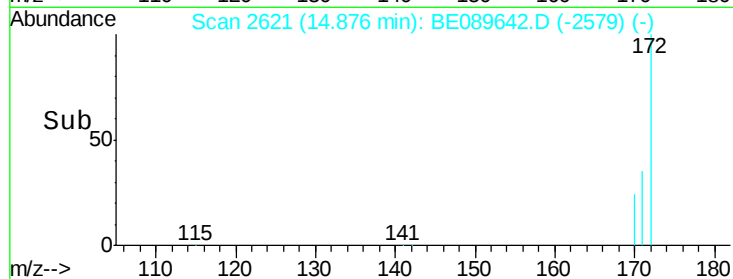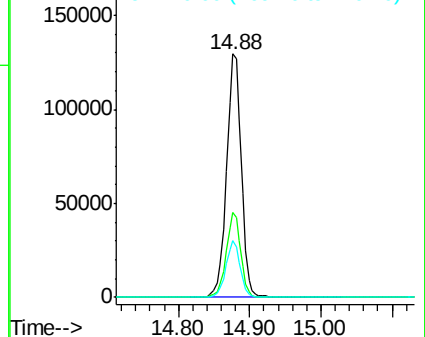

#10

Acenaphthylene

Concen: 0.14 ng

RT: 16.07 min Scan# 2820

Delta R.T. 0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:152 Resp: 16233

Ion Ratio Lower Upper

152 100

151 5.0 3.9 5.9



153 13.2 10.5 15.7

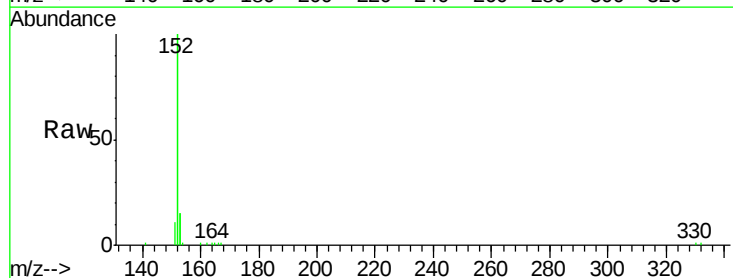


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

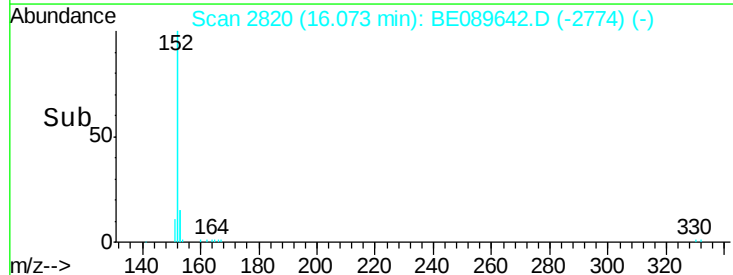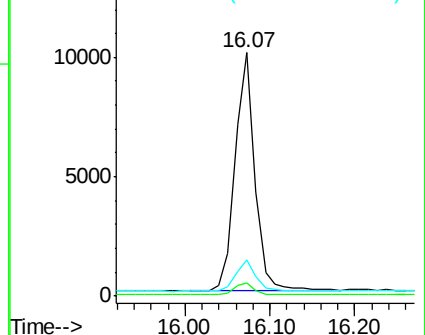



#11

Acenaphthene

Concen: 0.15 ng

RT: 16.49 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:154 Resp: 2919

Ion Ratio Lower Upper

154 100

153 441.8 348.9 523.3




152 223.8 166.6 249.8

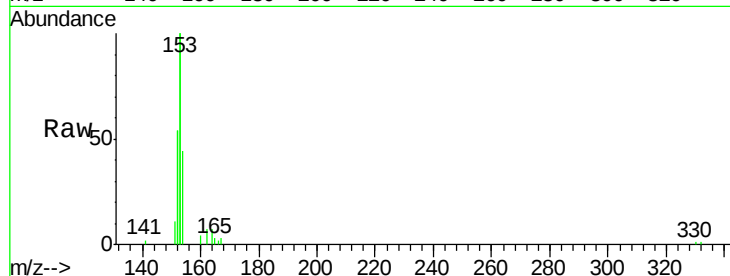

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

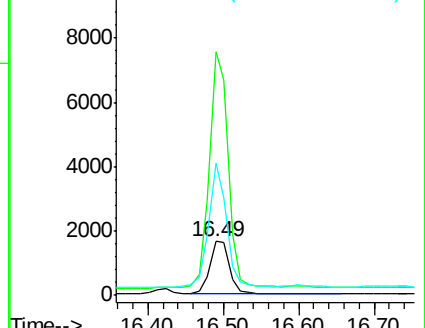

#12

Fluorene

Concen: 0.15 ng

RT: 17.74 min Scan# 2972

Delta R.T. 0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:166 Resp: 3368

Ion Ratio Lower Upper

166 100

165 92.1 74.7 112.1



167 13.7 10.5 15.7




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

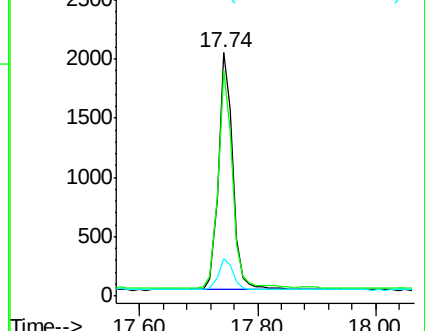

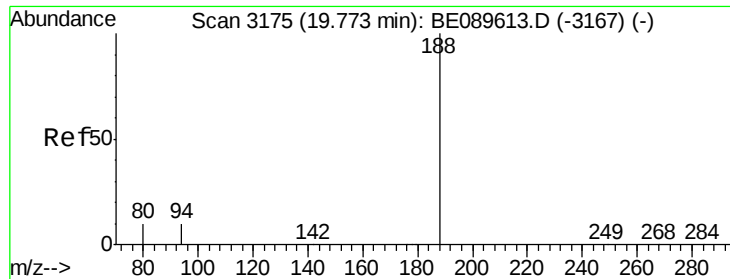

#13

Phenanthrene-d10

Concen: 5.00 ng

RT: 19.77 min Scan# 3176

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:188 Resp: 143322

Ion Ratio Lower Upper

188 100

94 9.6 8.2 12.4




80 9.3 8.1 12.1



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

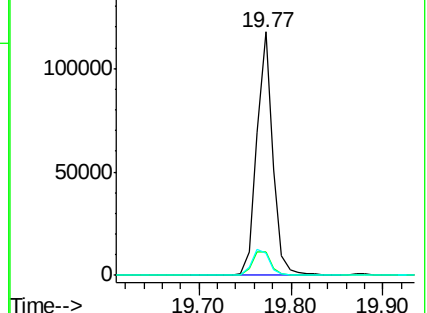

#14

Hexachlorobenzene

Concen: 0.17 ng

RT: 19.00 min Scan# 3090

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:284 Resp: 1029

Ion Ratio Lower Upper

284 100

142 46.2 32.3 48.5



249 28.1 22.3 33.5



Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E



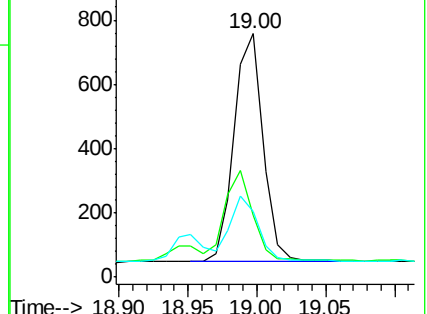





#15
 Pentachlorophenol
 Concen: 0.05 ng
 RT: 19.45 min Scan# 3140
 Delta R.T. 0.01 min
 Lab File: BE089642.D
 Acq: 20 Feb 2015 1:09




Instrument :
 BNA_E
 ClientSampleId :
 MDL-04-W

Tot Ion:266 Resp: 70
 Ion Ratio Lower Upper
 266 100
 268 82.9 52.6 79.0#
 264 81.6 51.8 77.8#

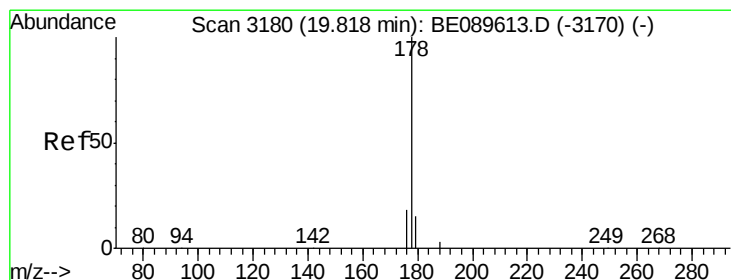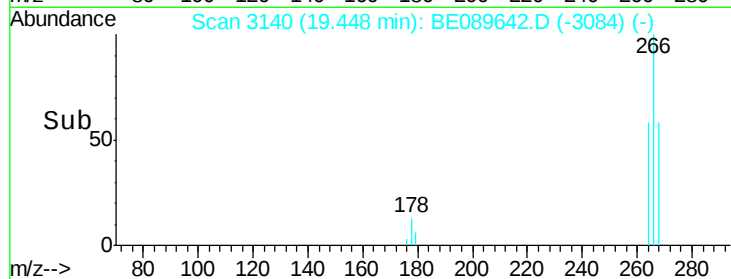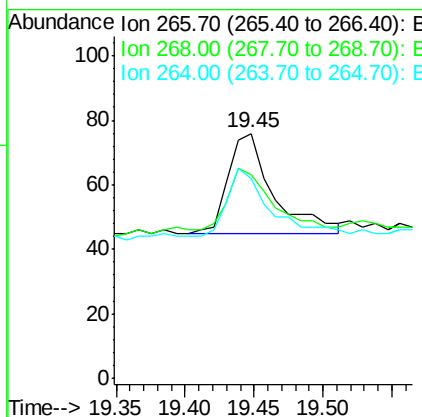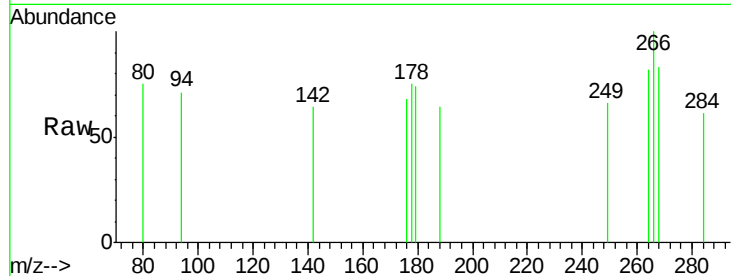

#16
 Phenanthrene
 Concen: 0.16 ng
 RT: 19.81 min Scan# 3180
 Delta R.T. -0.01 min
 Lab File: BE089642.D
 Acq: 20 Feb 2015 1:09

Tgt Ion:178 Resp: 5754
 Ion Ratio Lower Upper
 178 100
 176 18.4 15.1 22.7
 179 16.4 12.3 18.5


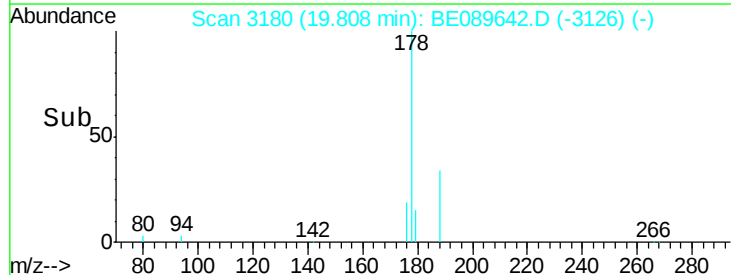
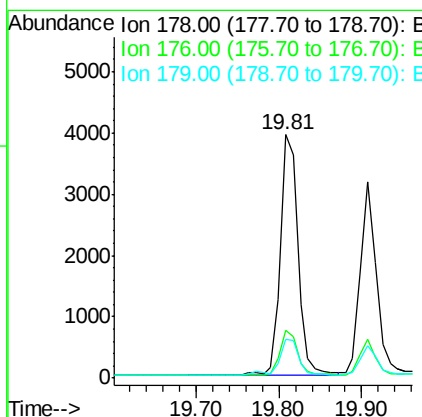





#17
 Anthracene
 Concen: 0.14 ng
 RT: 19.91 min Scan# 3191
 Delta R.T. -0.00 min
 Lab File: BE089642.D
 Acq: 20 Feb 2015 1:09




Instrument :
 BNA_E
 ClientSampleId :
 MDL-04-W


Tot Ion:178 Resp: 4240
 Ion Ratio Lower Upper
 178 100
 176 18.5 14.6 22.0
 179 15.5 12.3 18.5

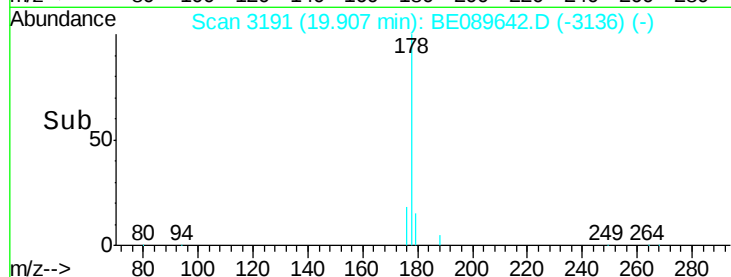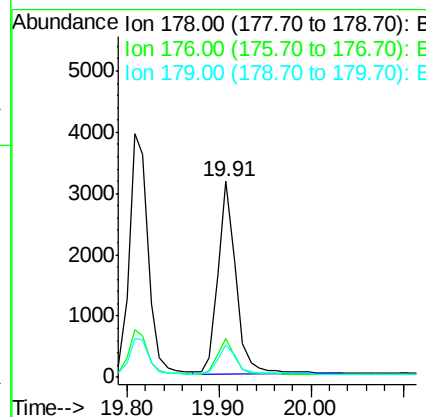

#18
 Fluoranthene
 Concen: 0.14 ng
 RT: 21.72 min Scan# 3476
 Delta R.T. 0.00 min
 Lab File: BE089642.D
 Acq: 20 Feb 2015 1:09

Tgt Ion:202 Resp: 4662
 Ion Ratio Lower Upper
 202 100
 101 12.5 10.4 15.6
 203 17.0 13.9 20.9

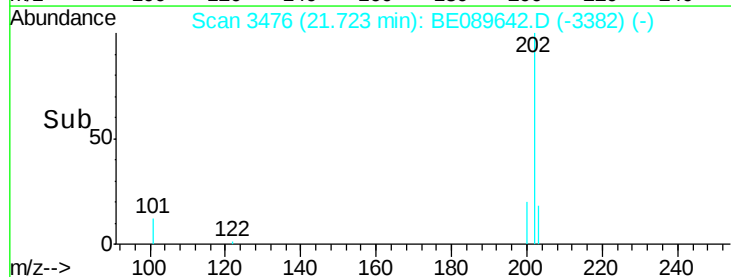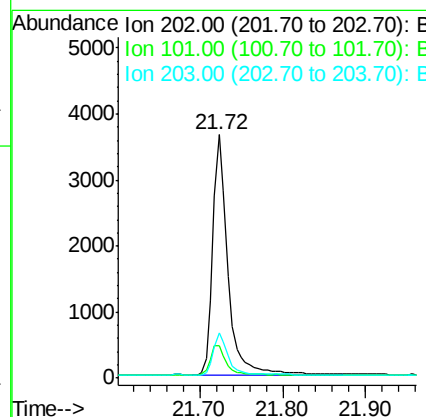

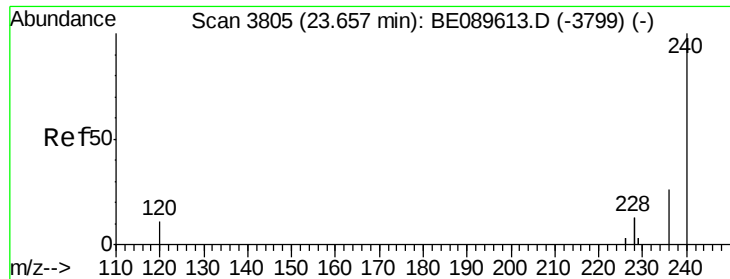

#19

Chrysene-d12

Concen: 5.00 ng

RT: 23.66 min Scan# 3807

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:240 Resp: 135795

Ion Ratio Lower Upper

240 100

120 10.7 9.0 13.4




236 25.7 21.0 31.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

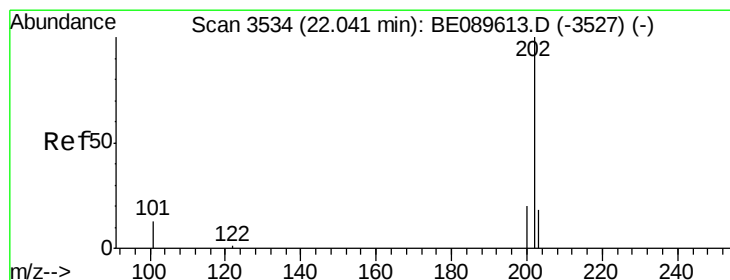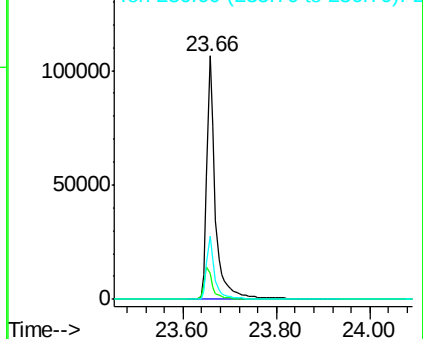

#20

Pyrene

Concen: 0.15 ng

RT: 22.04 min Scan# 3536

Delta R.T. 0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:202 Resp: 5049

Ion Ratio Lower Upper

202 100

200 20.4 16.3 24.5



203 17.7 13.8 20.8



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

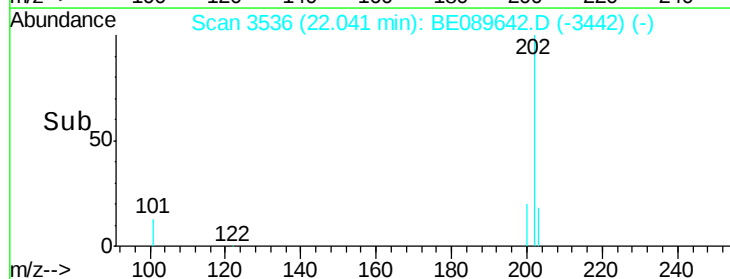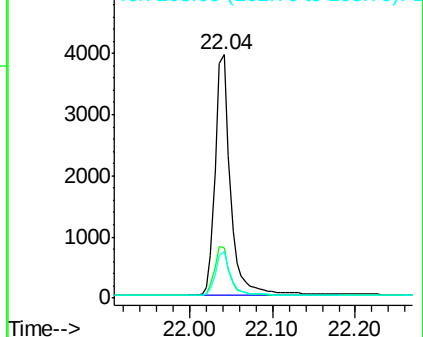



#21

Terphenyl-d14

Concen: 12.63 ng

RT: 22.30 min Scan# 3585

Delta R.T. 0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:244 Resp: 246700

Ion Ratio Lower Upper

244 100

212 6.6 5.8 8.8




122 12.1 11.8 17.8

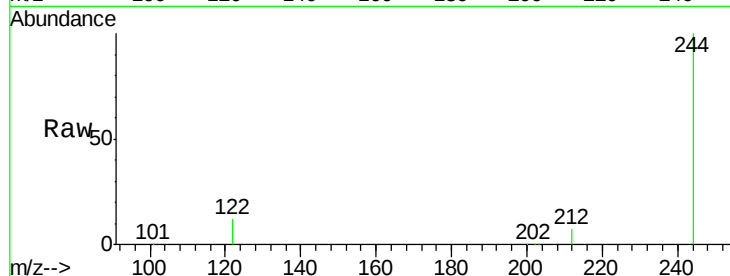

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

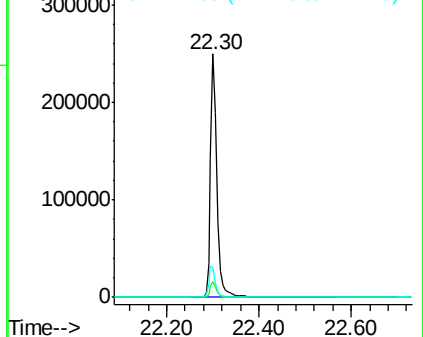

#22

Benzo(a)anthracene

Concen: 0.13 ng

RT: 23.65 min Scan# 3806

Delta R.T. 0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:228 Resp: 15471

Ion Ratio Lower Upper

228 100

226 24.8 21.2 31.8



229 22.4 15.2 22.8



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

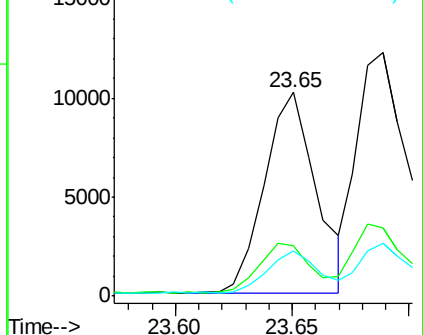



#23

Chrysene

Concen: 0.19 ng

RT: 23.69 min Scan# 3812

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W





Tot Ion:228 Resp: 25354

Ion Ratio Lower Upper

228 100

226 28.3 22.2 33.4

229 21.6 16.0 24.0

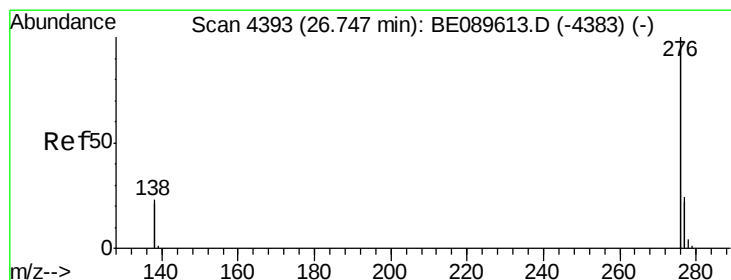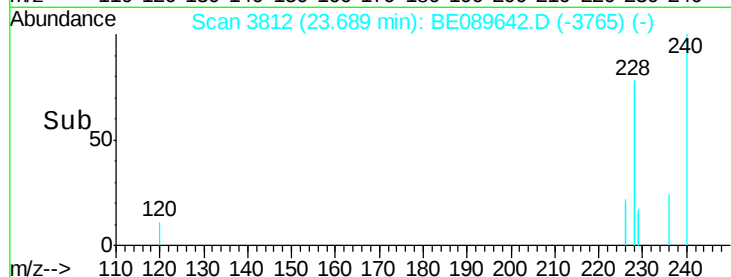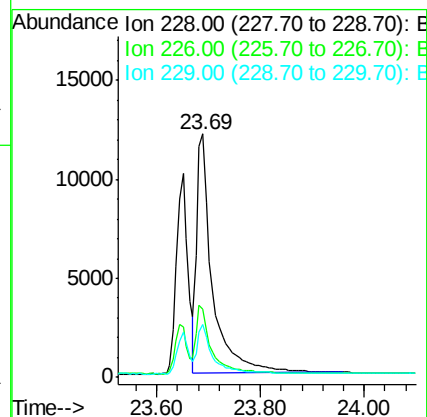

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.22 ng

RT: 26.74 min Scan# 4394

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09




Tgt Ion:276 Resp: 5854


Ion Ratio Lower Upper

276 100

138 22.5 21.4 32.2

277 19.9 19.9 29.9


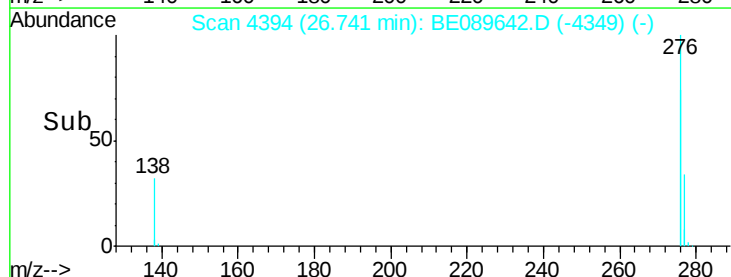
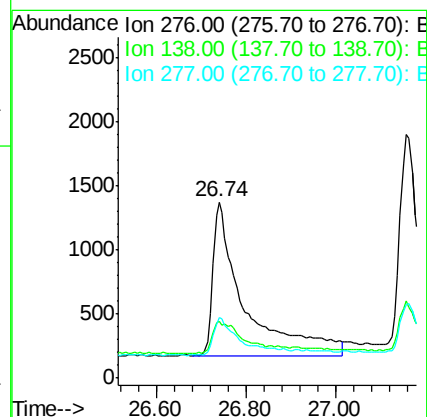



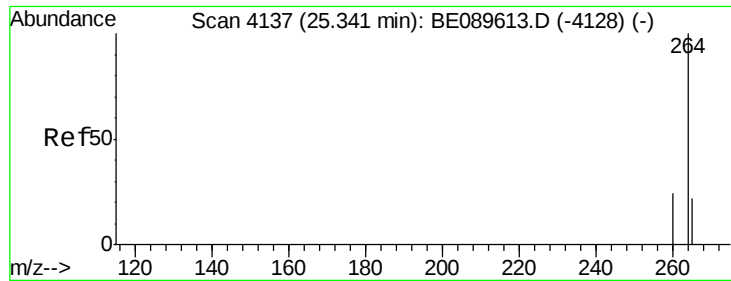

#25
Pervlene-d12
Concen: 5.00 ng
RT: 25.34 min Scan# 4139
Delta R.T. 0.00 min
Lab File: BE089642.D
Acq: 20 Feb 2015 1:09




Instrument :
BNA_E
ClientSampleId :
MDL-04-W

Tot Ion:264 Resp: 110972
Ion Ratio Lower Upper
264 100
260 23.5 19.0 28.6
265 21.6 17.4 26.0

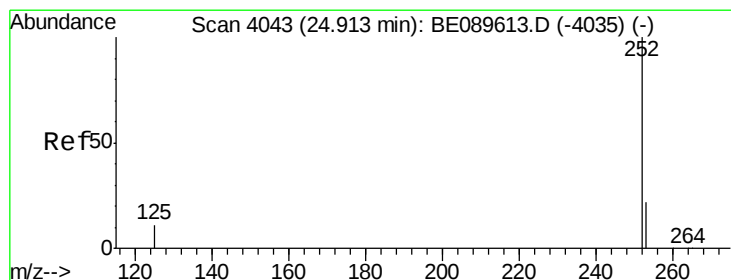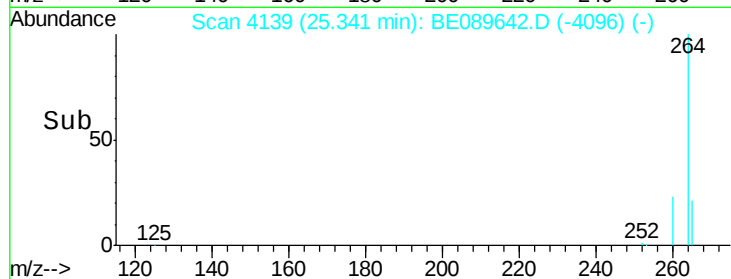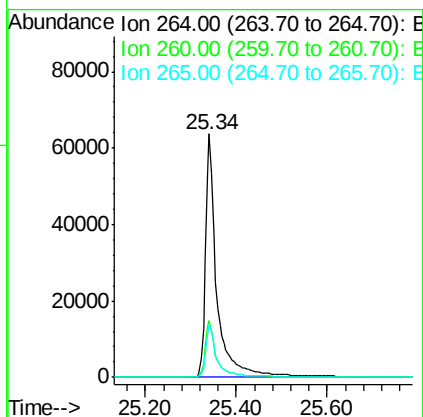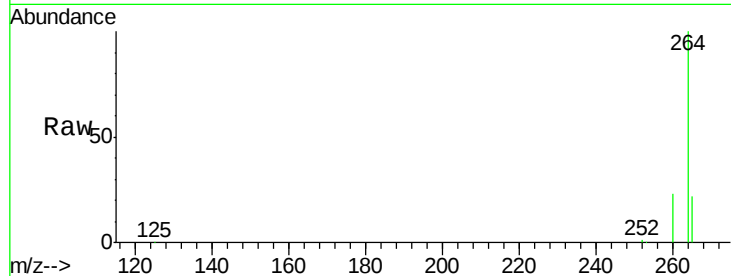

#26
Benzo(b)fluoranthene
Concen: 0.31 ng
RT: 24.91 min Scan# 4044
Delta R.T. -0.00 min
Lab File: BE089642.D
Acq: 20 Feb 2015 1:09

Tgt Ion:252 Resp: 1073
Ion Ratio Lower Upper
252 100
253 25.6 17.6 26.4
125 16.2 8.8 13.2#

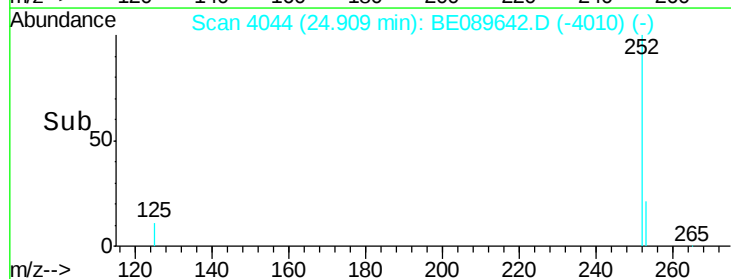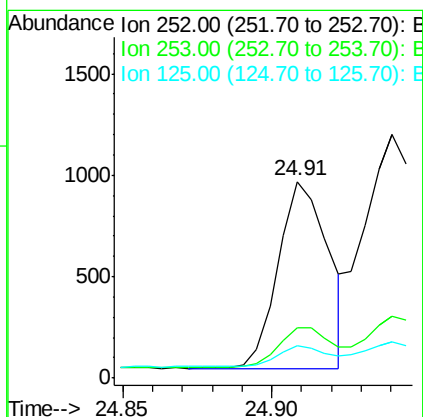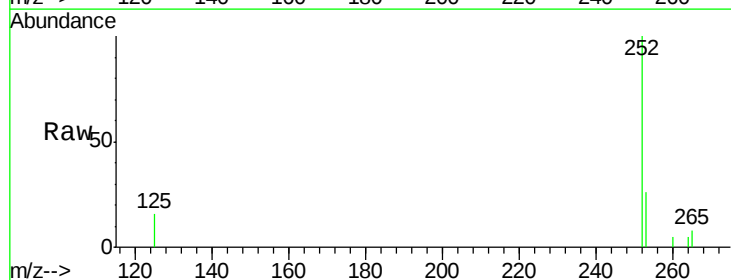



#27

Benzo(k)fluoranthene

Concen: 0.12 ng/mL

RT: 24.94 min Scan# 4051

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleID :

MDL-04-W


Tot Ion:252 Resp: 3761

Ion Ratio Lower Upper

252 100

253 25.2 17.7 26.5




125 14.8 8.8 13.2#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

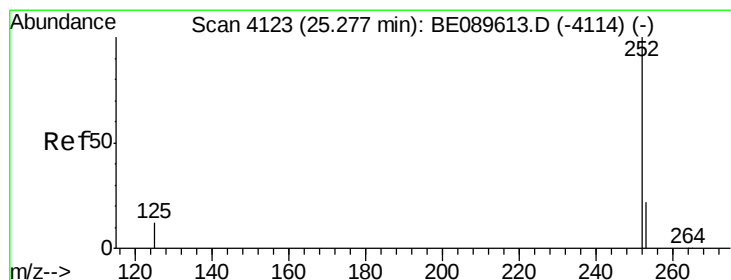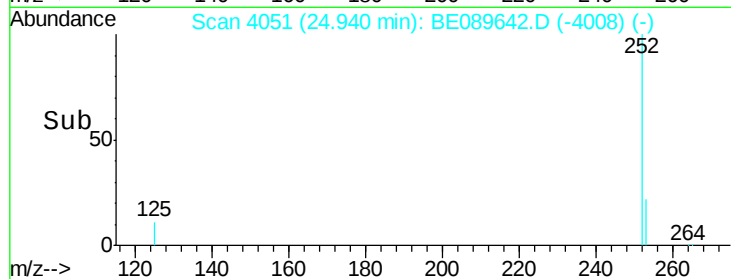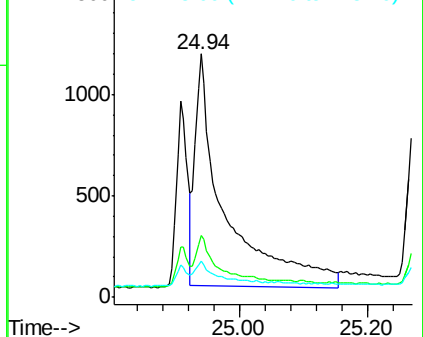

#28

Benzo(a)pyrene

Concen: 0.29 ng/mL

RT: 25.27 min Scan# 4124

Delta R.T. -0.00 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:252 Resp: 1280

Ion Ratio Lower Upper

252 100

253 27.0 18.1 27.1



125 18.3 9.6 14.4#

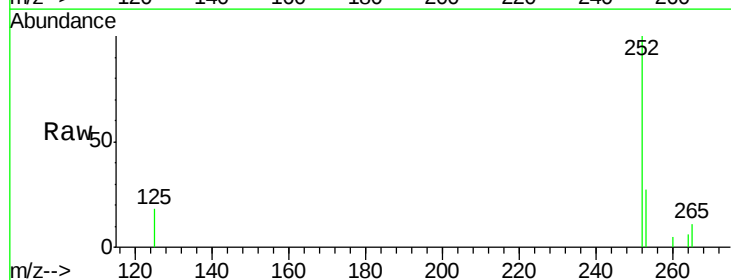


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

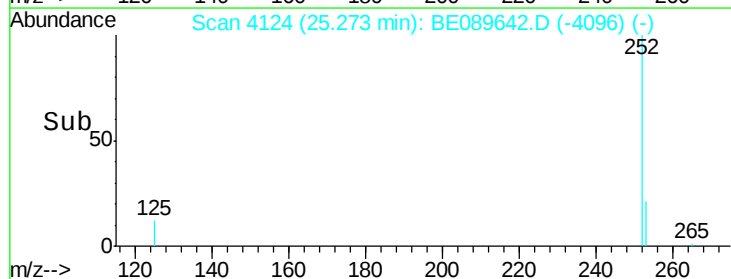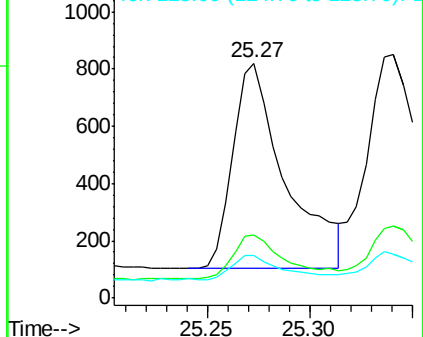

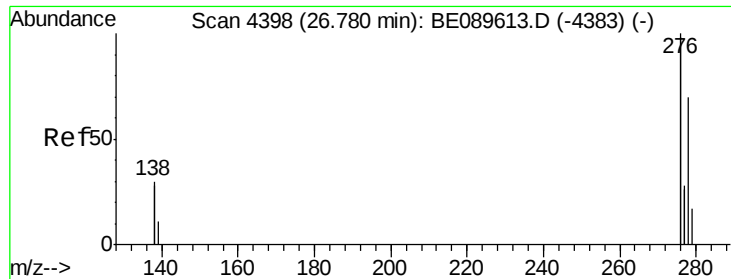

#29

Dibenzo(a,h)anthracene

Concen: 0.27 ng

RT: 26.77 min Scan# 4399

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09

Instrument :

BNA_E

ClientSampleId :

MDL-04-W


Tot Ion:278 Resp: 890

Ion Ratio Lower Upper

278 100

139 28.6 13.7 20.5#

279 34.6 19.7 29.5#



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

26.77



300

200

100

0

Time--> 26.60 26.80

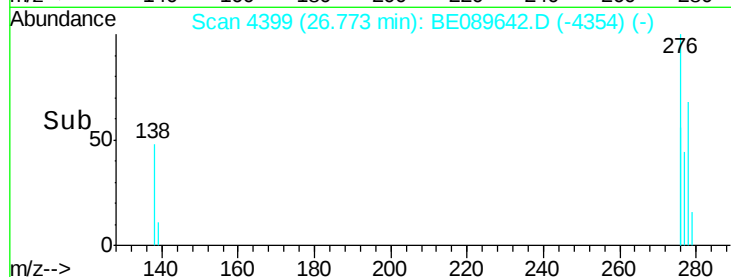

#30

Benzo(g,h,i)perylene

Concen: 0.21 ng

RT: 27.16 min Scan# 4458

Delta R.T. -0.01 min

Lab File: BE089642.D

Acq: 20 Feb 2015 1:09


Tgt Ion:276 Resp: 7515

Ion Ratio Lower Upper

276 100

277 30.4 19.1 28.7#

138 31.8 18.7 28.1#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

27.16

2500

2000

1500

1000

500

0

Time--> 27.00 27.20 27.40

