


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE021815\  
 Data File : BE089608.D  
 Acq On : 18 Feb 2015 00:16  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIMPAH-BE021815.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Feb 18 13:01:39 2015

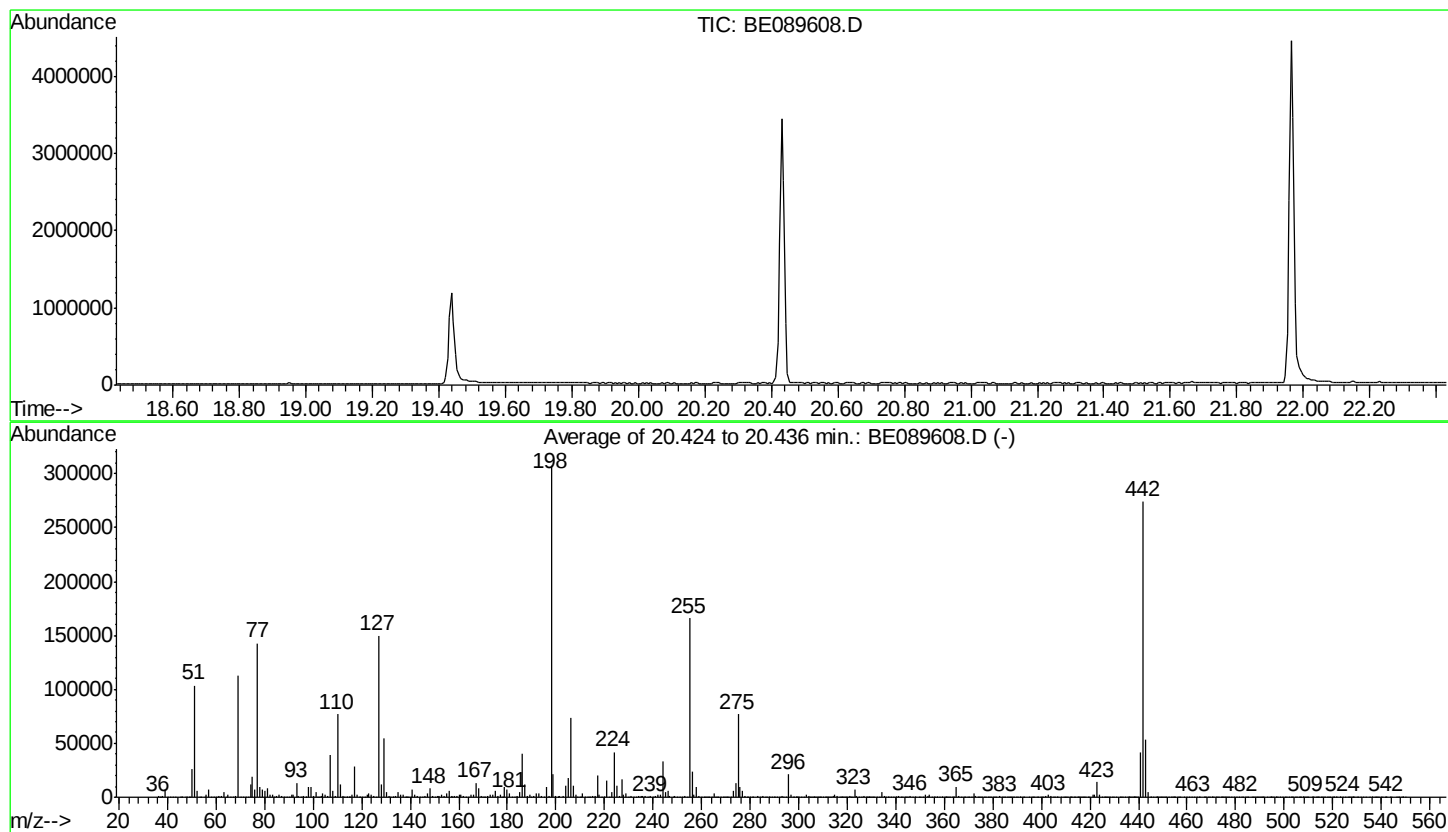

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3231

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 33.7      | 103599  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 1653    | PASS             |
| 69          | 198          | 0.00         | 100          | 36.5      | 112330  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 529     | PASS             |
| 127         | 198          | 10           | 80           | 48.7      | 149809  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 707     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 307554  | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 21524   | PASS             |
| 275         | 198          | 10           | 60           | 25.0      | 76804   | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 9808    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.4      | 42121   | PASS             |
| 442         | 198          | 50           | 100          | 89.0      | 273860  | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 53130   | PASS             |