


Data Path : Z:\HPCHEM1\BNA E\Data\BE021815\
Data File : BE089633.D
Acq On : 19 Feb 2015 11:22
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE021815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 18 13:01:39 2015

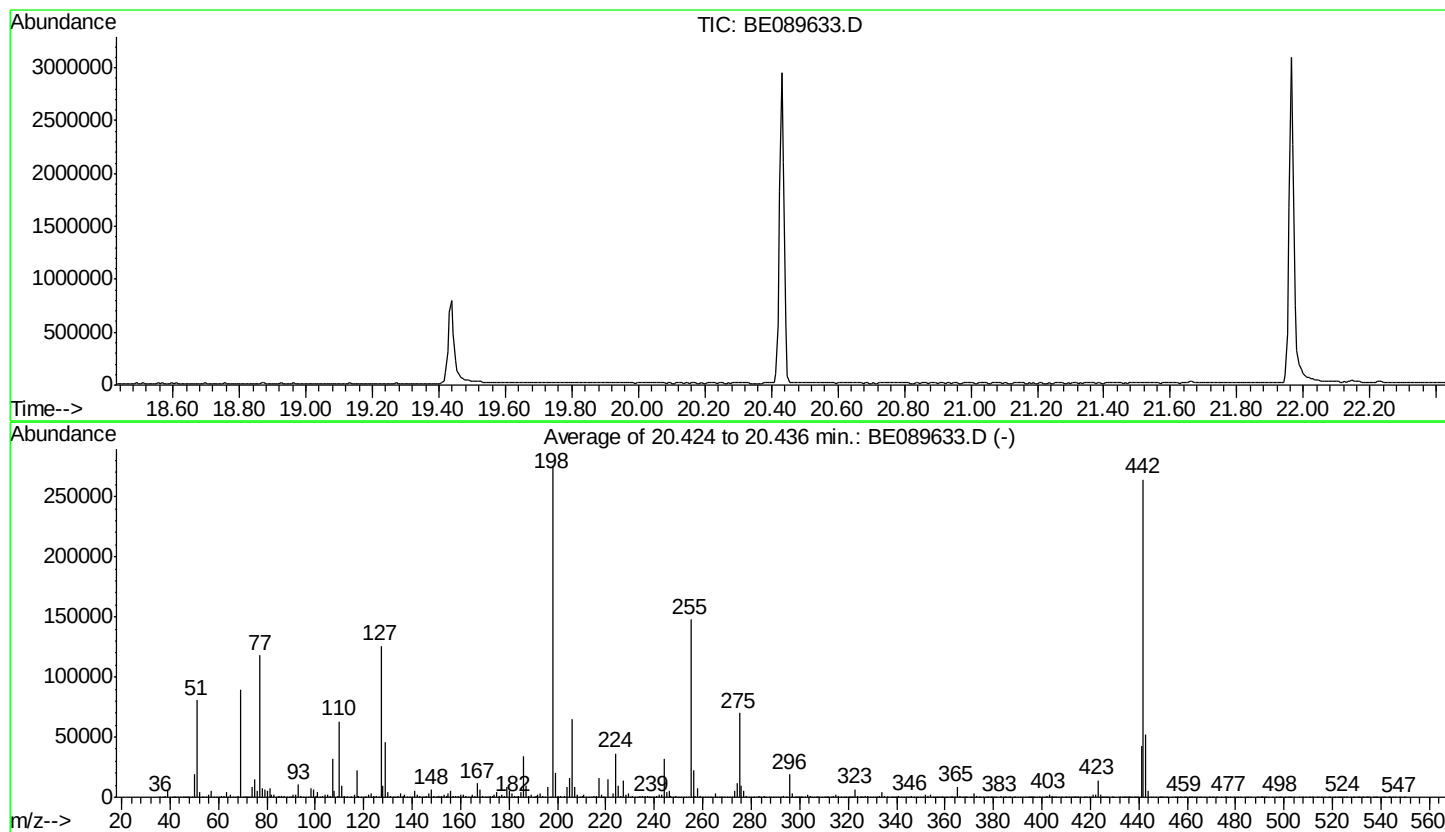

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3233

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	80551	PASS
68	69	0.00	2	1.7	1505	PASS
69	198	0.00	100	32.4	89500	PASS
70	69	0.00	2	0.4	324	PASS
127	198	10	80	45.6	125707	PASS
197	198	0.00	2	0.1	321	PASS
198	198	100	100	100.0	275840	PASS
199	198	5	9	7.3	20150	PASS
275	198	10	60	25.4	69946	PASS
365	198	1	100	3.2	8747	PASS
441	442	0.01	24	16.1	42466	PASS
442	198	50	100	95.9	264459	PASS
443	442	15	24	19.8	52459	PASS